

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 15:14
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 15:51:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 15:50:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	91400117	165.8E6	50.000	50.000
28)	SA Decachlor...	8.902	7.720	77411466	106.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.573	3.599	37033953	50553663	500.000	500.000
24)	Chlordane-2	5.107	4.169	39395339	53884695	500.000	500.000
25)	Chlordane-3	5.818	4.793	148.7E6	154.4E6	500.000	500.000
26)	Chlordane-4	5.897	4.854	178.9E6	161.6E6	500.000	500.000
27)	Chlordane-5	6.756	5.517	29552542	41102291	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 15:14
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 15:51:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 15:50:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

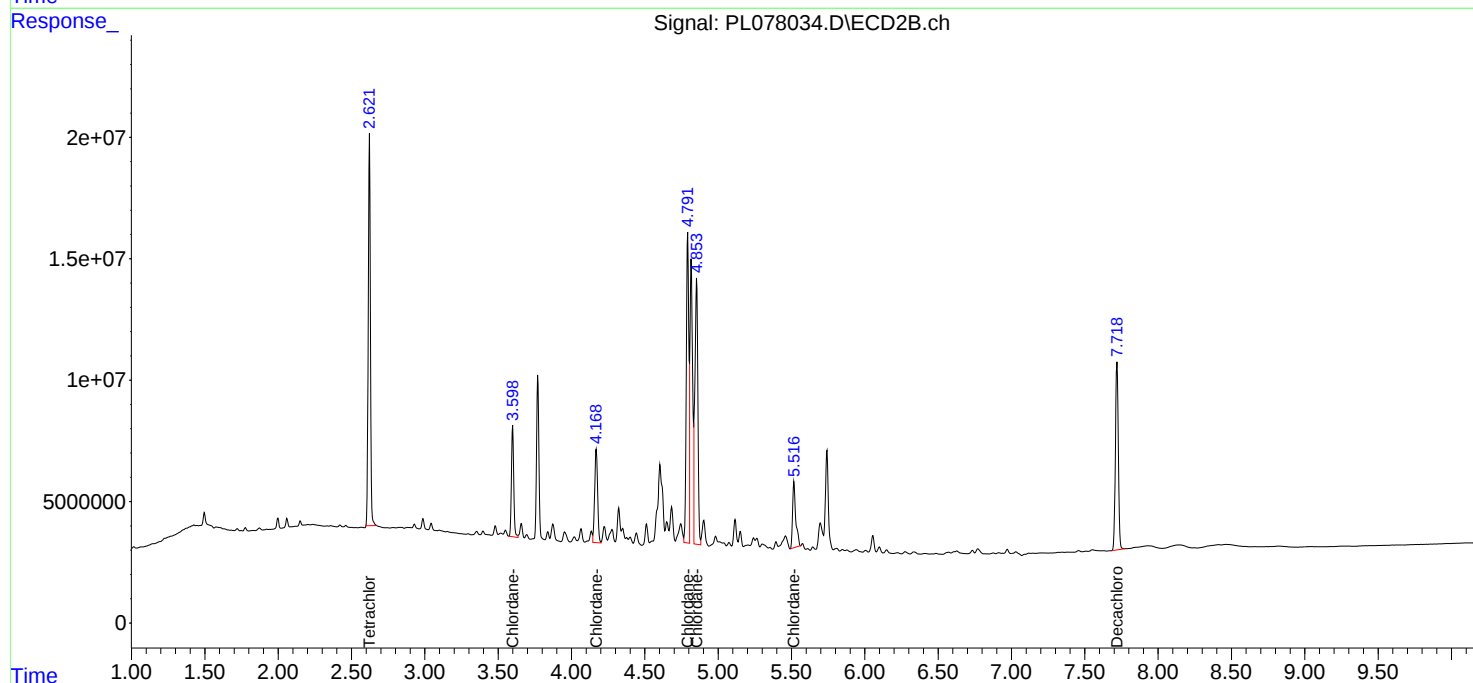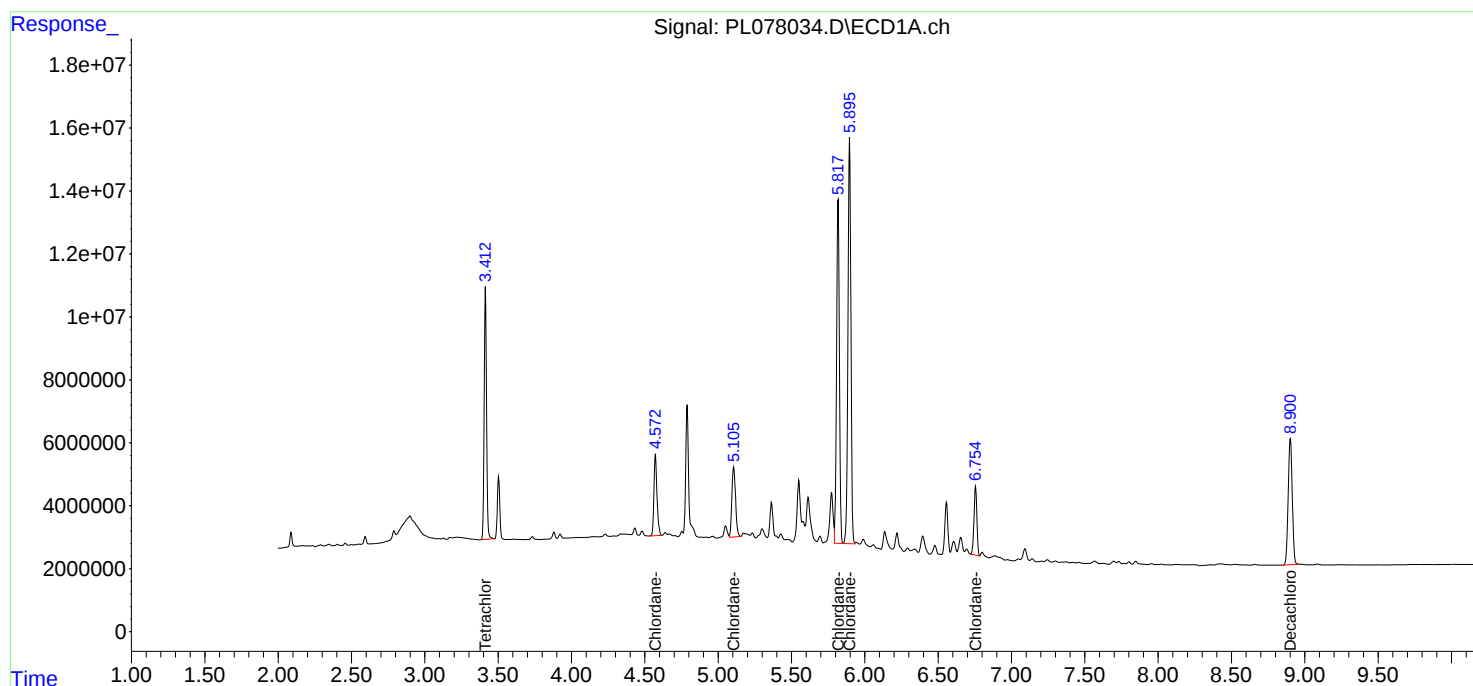


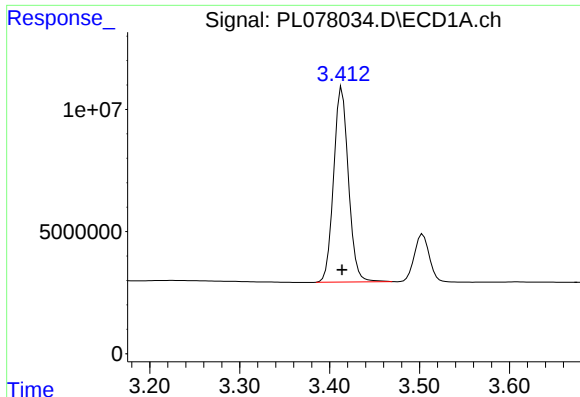

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.000 min
Response: 91400117
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

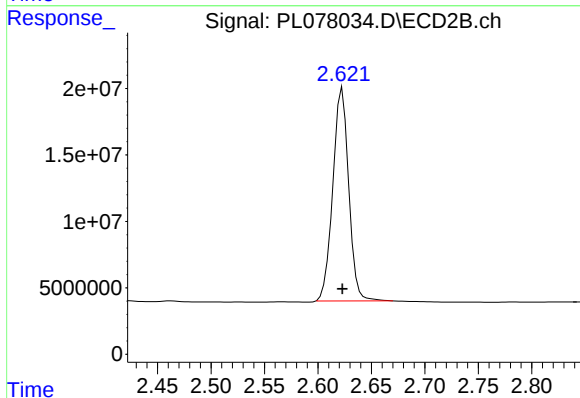


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 165840624
Conc: 50.00 ng/ml

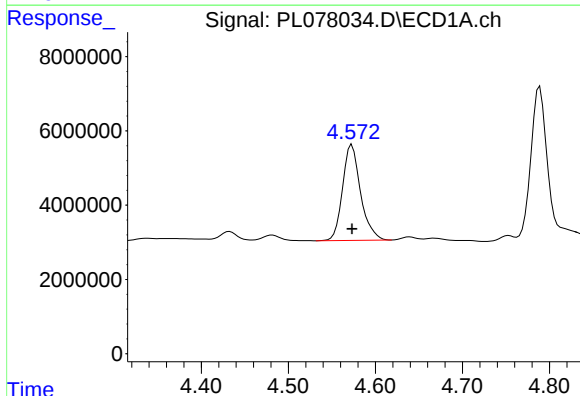


#23 Chlordane-1

R.T.: 4.573 min
Delta R.T.: 0.000 min
Response: 37033953
Conc: 500.00 ng/ml

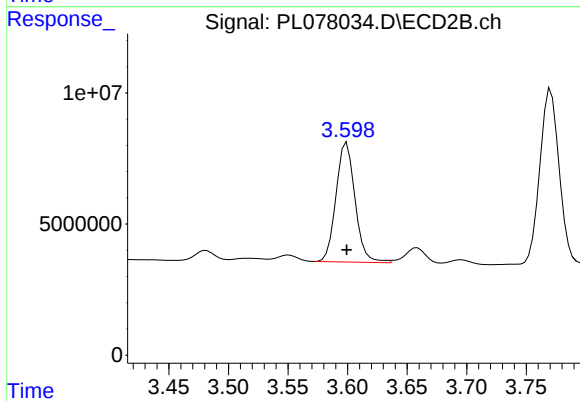

#23 Chlordane-1


R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 50553663
Conc: 500.00 ng/ml

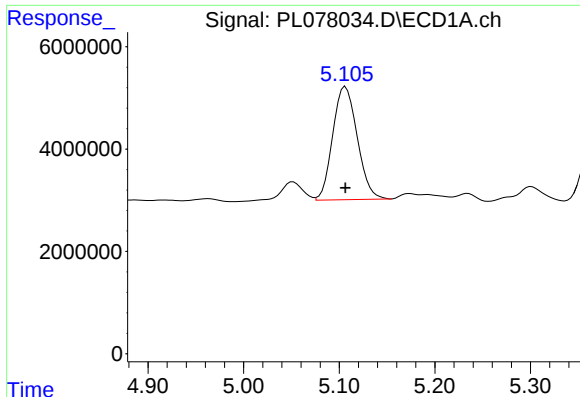

#24 Chlordane-2


R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 39395339
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

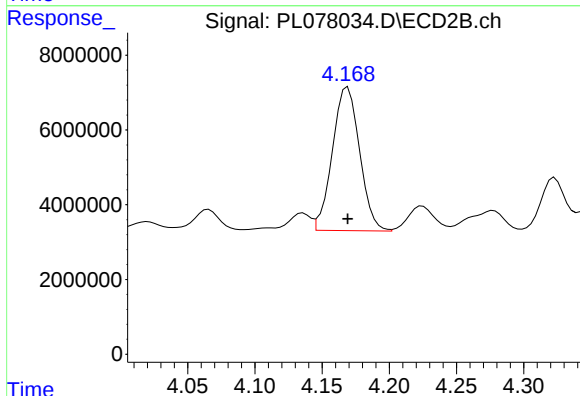


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 53884695
Conc: 500.00 ng/ml

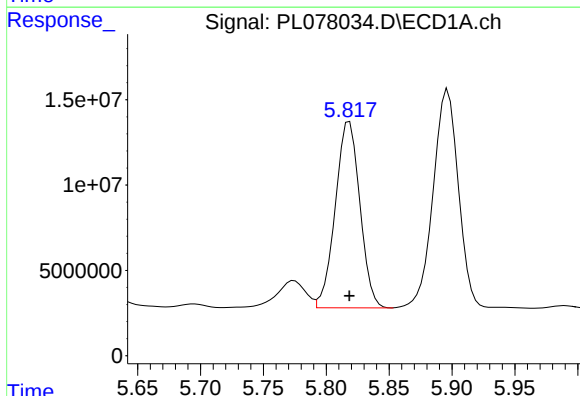


#25 Chlordane-3

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 148652405
Conc: 500.00 ng/ml

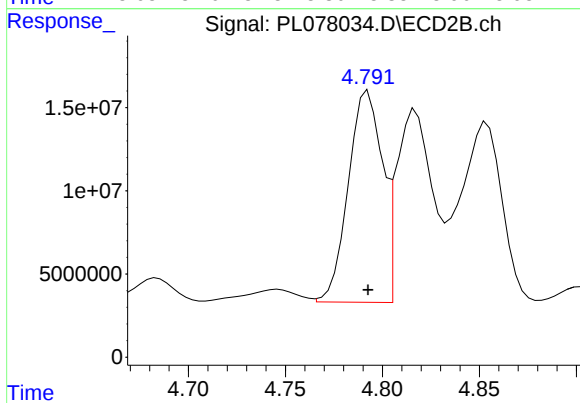

#25 Chlordane-3


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 154413109
Conc: 500.00 ng/ml

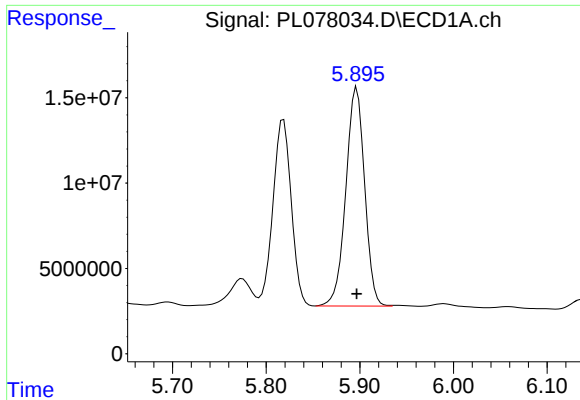

#26 Chlordane-4


R.T.: 5.897 min
Delta R.T.: 0.000 min
Response: 178918685
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

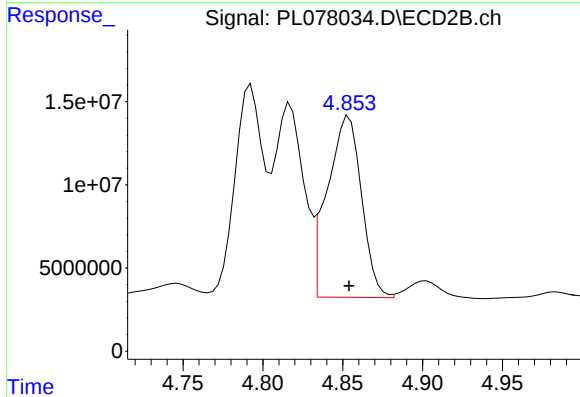


#26 Chlordane-4

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 161644755
Conc: 500.00 ng/ml

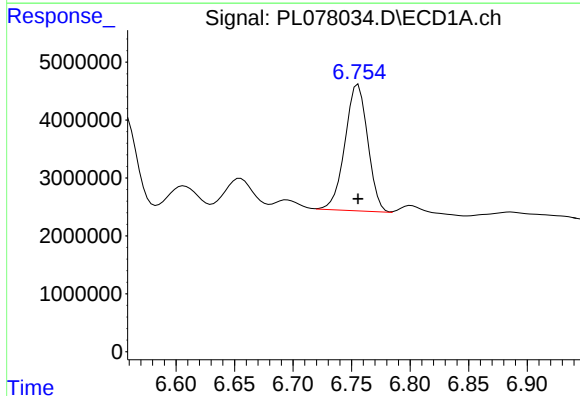


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.000 min
Response: 29552542
Conc: 500.00 ng/ml

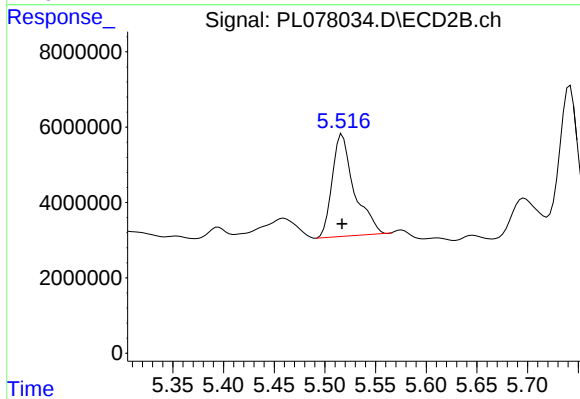

#27 Chlordane-5


R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 41102291
Conc: 500.00 ng/ml

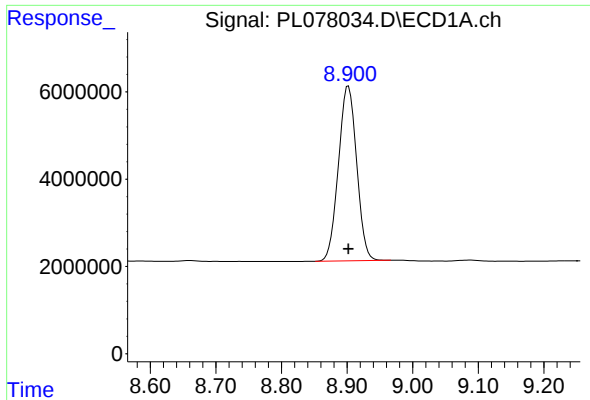

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 77411466
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

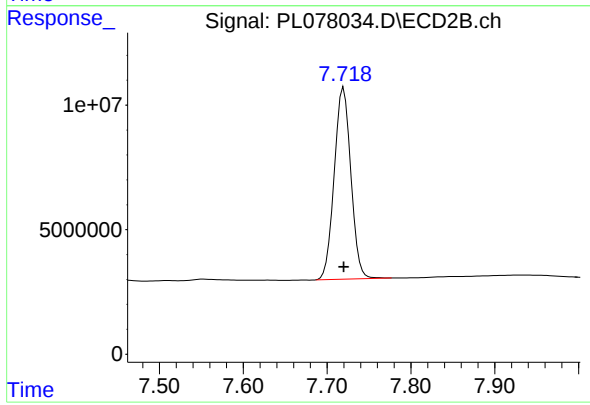

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: 0.000 min
Response: 105978164
Conc: 50.00 ng/ml