

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 15:28
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 15:51:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 15:50:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	46075975	84610322	25.206	25.510
28)	SA Decachlor...	8.902	7.719	40772985	56082721	26.335	26.460
Target Compounds							
23)	Chlordane-1	4.573	3.599	18394464	25797203	248.346	255.147
24)	Chlordane-2	5.107	4.169	20326383	28221165	257.980	261.866
25)	Chlordane-3	5.818	4.792	72512892	79511793	243.901	257.465
26)	Chlordane-4	5.897	4.854	88342453	83328677	246.879	257.752
27)	Chlordane-5	6.755	5.517	14419095	21378997	243.957	260.071



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 15:28
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 15:51:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 15:50:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

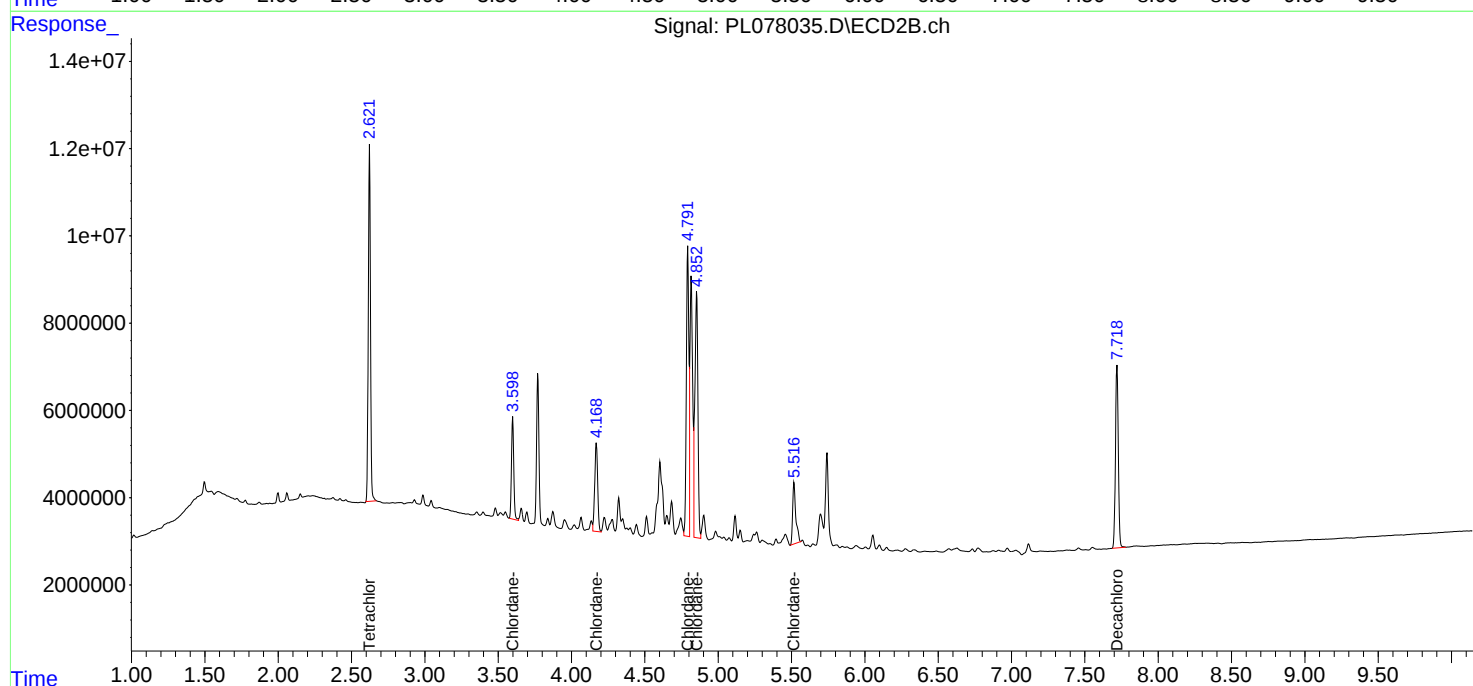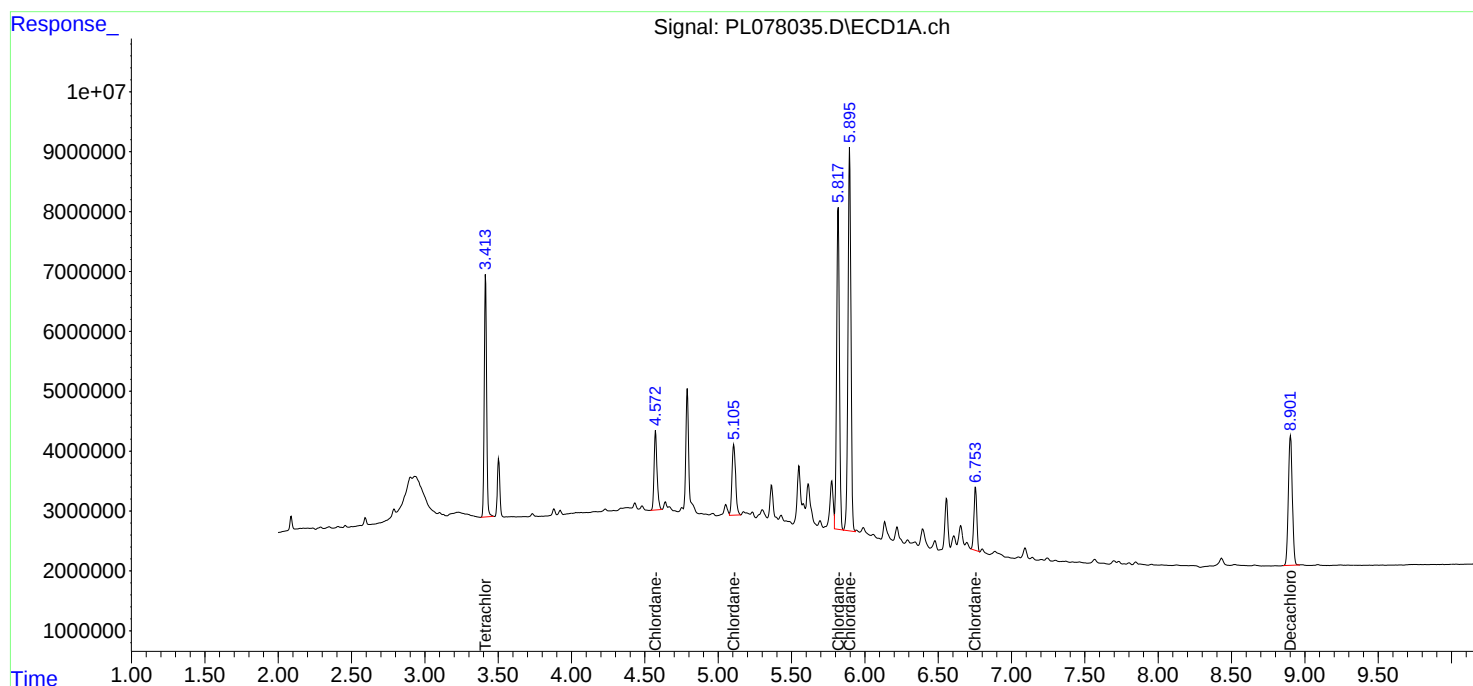


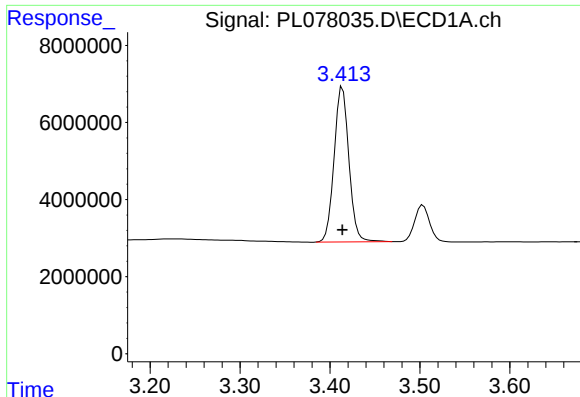

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.000 min
Response: 46075975
Conc: 25.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

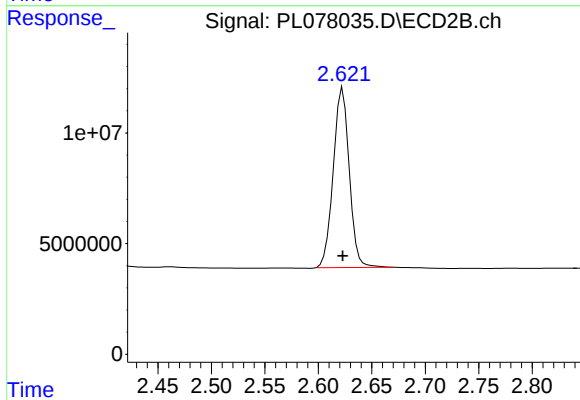


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 84610322
Conc: 25.51 ng/ml

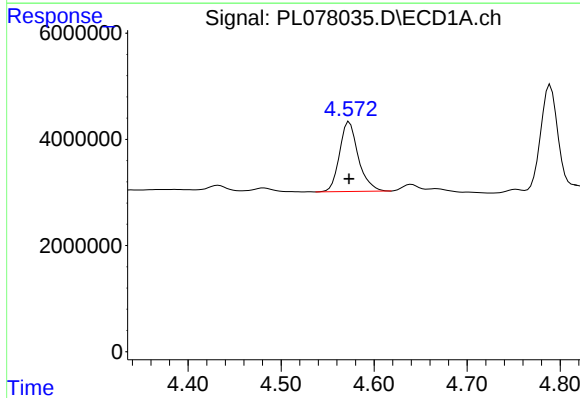


#23 Chlordane-1

R.T.: 4.573 min
Delta R.T.: 0.000 min
Response: 18394464
Conc: 248.35 ng/ml

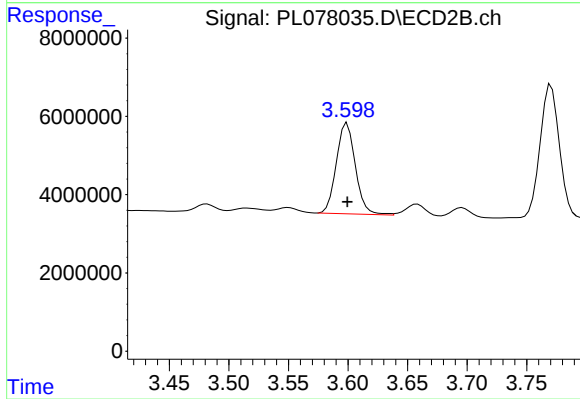

#23 Chlordane-1


R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 25797203
Conc: 255.15 ng/ml

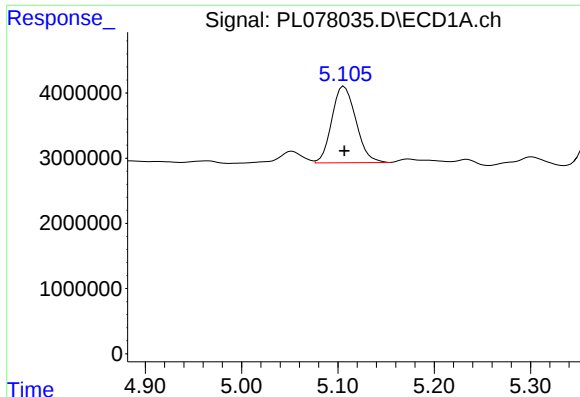

#24 Chlordane-2


R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 20326383
Conc: 257.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

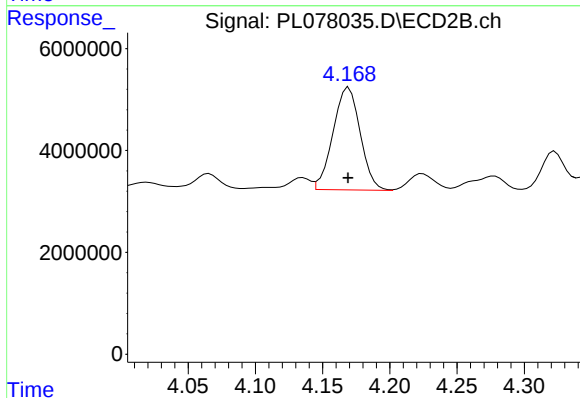


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 28221165
Conc: 261.87 ng/ml

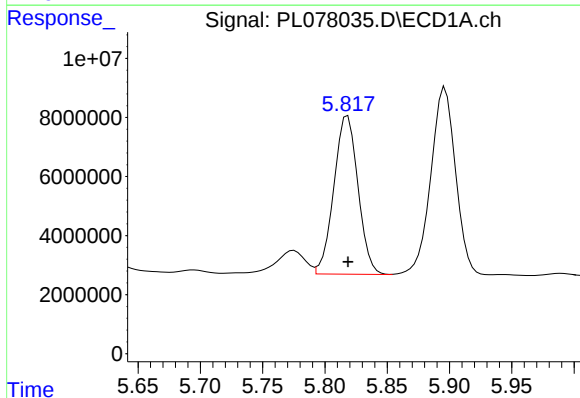


#25 Chlordane-3

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 72512892
Conc: 243.90 ng/ml

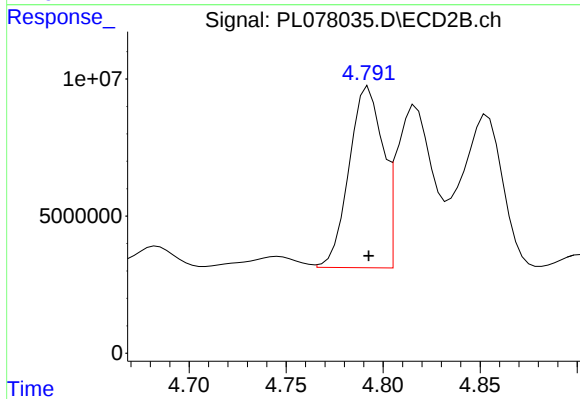

#25 Chlordane-3


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 79511793
Conc: 257.46 ng/ml

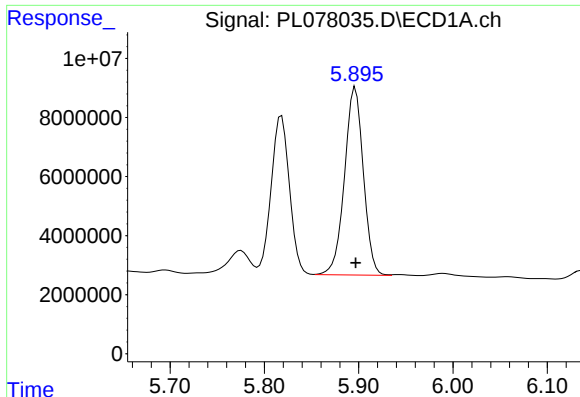

#26 Chlordane-4


R.T.: 5.897 min
Delta R.T.: 0.000 min
Response: 88342453
Conc: 246.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

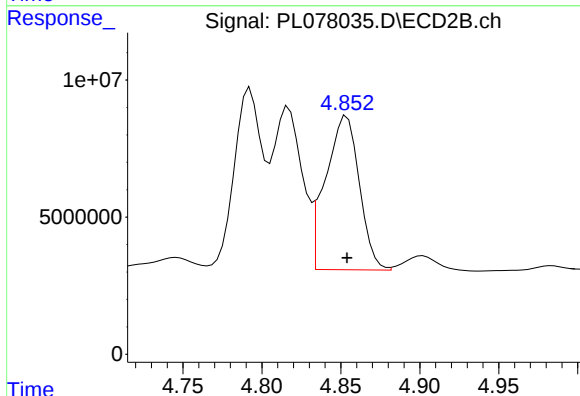


#26 Chlordane-4

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 83328677
Conc: 257.75 ng/ml

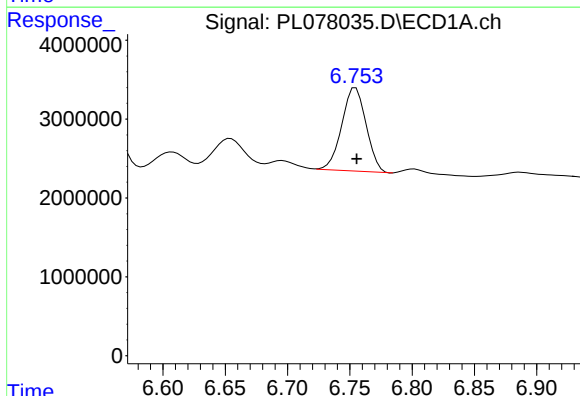


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 14419095
Conc: 243.96 ng/ml

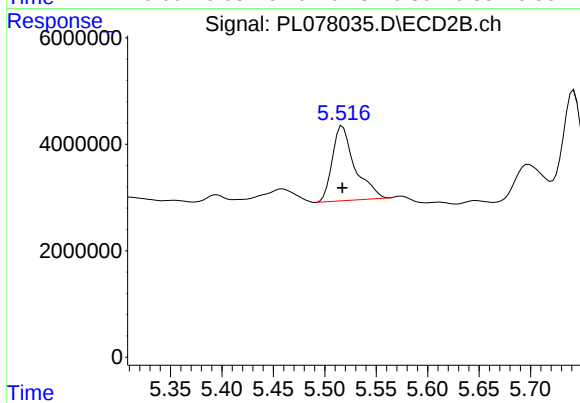

#27 Chlordane-5


R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 21378997
Conc: 260.07 ng/ml

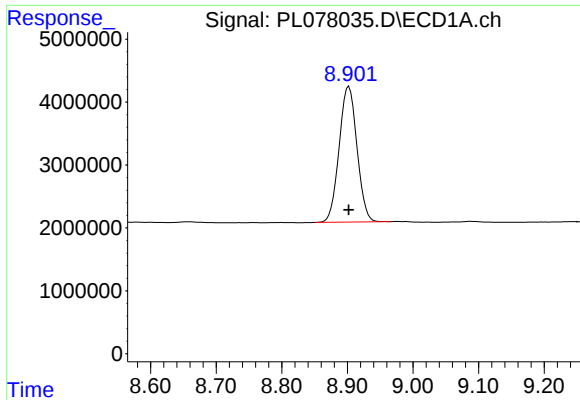

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 40772985
Conc: 26.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

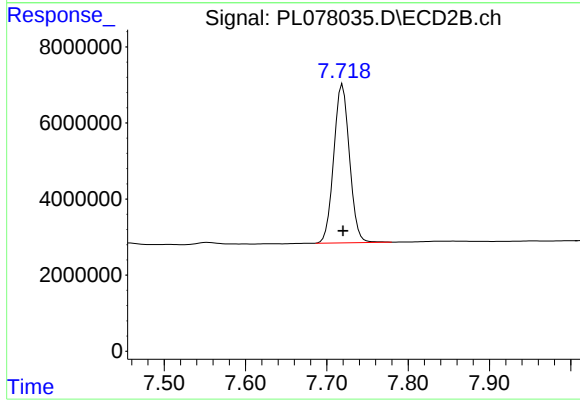

#28 Decachlorobiphenyl

R.T.: 7.719 min
Delta R.T.: 0.000 min
Response: 56082721
Conc: 26.46 ng/ml