

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 15:41
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 16:31:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 15:50:40 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	2.623	9926963	18436076	5.430	5.558
28)	SA Decachlor...	8.902	7.720	9534207	13210845	6.158	6.233
Target Compounds							
23)	Chlordane-1	4.573	3.599	3555390	5491953	48.002	54.318
24)	Chlordane-2	5.106	4.169	4499233	6422480	57.104	59.595
25)	Chlordane-3	5.818	4.793	14844331	18239616	49.930	59.061
26)	Chlordane-4	5.896	4.853	18312942	19054252	51.177	58.939
27)	Chlordane-5	6.755	5.518	3365606	4431346	56.943	53.906



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 15:41
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 16:31:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 15:50:40 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

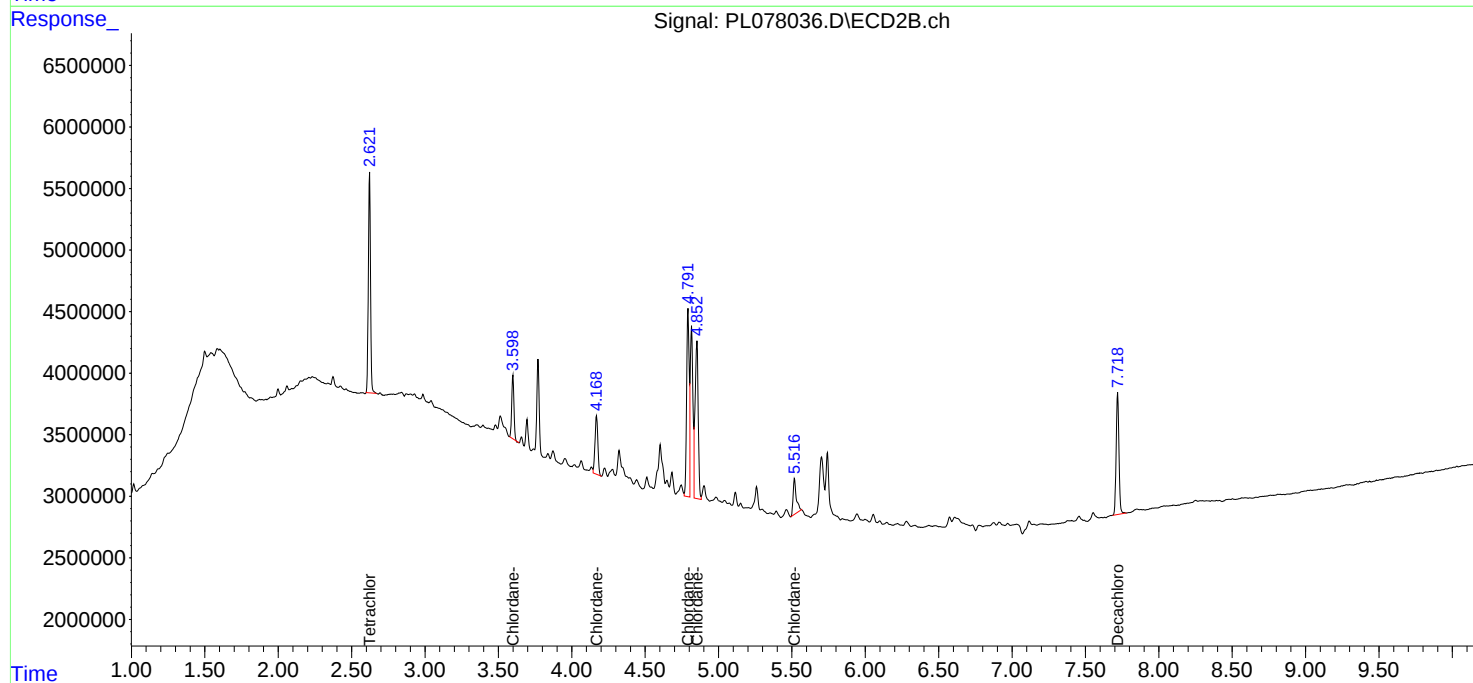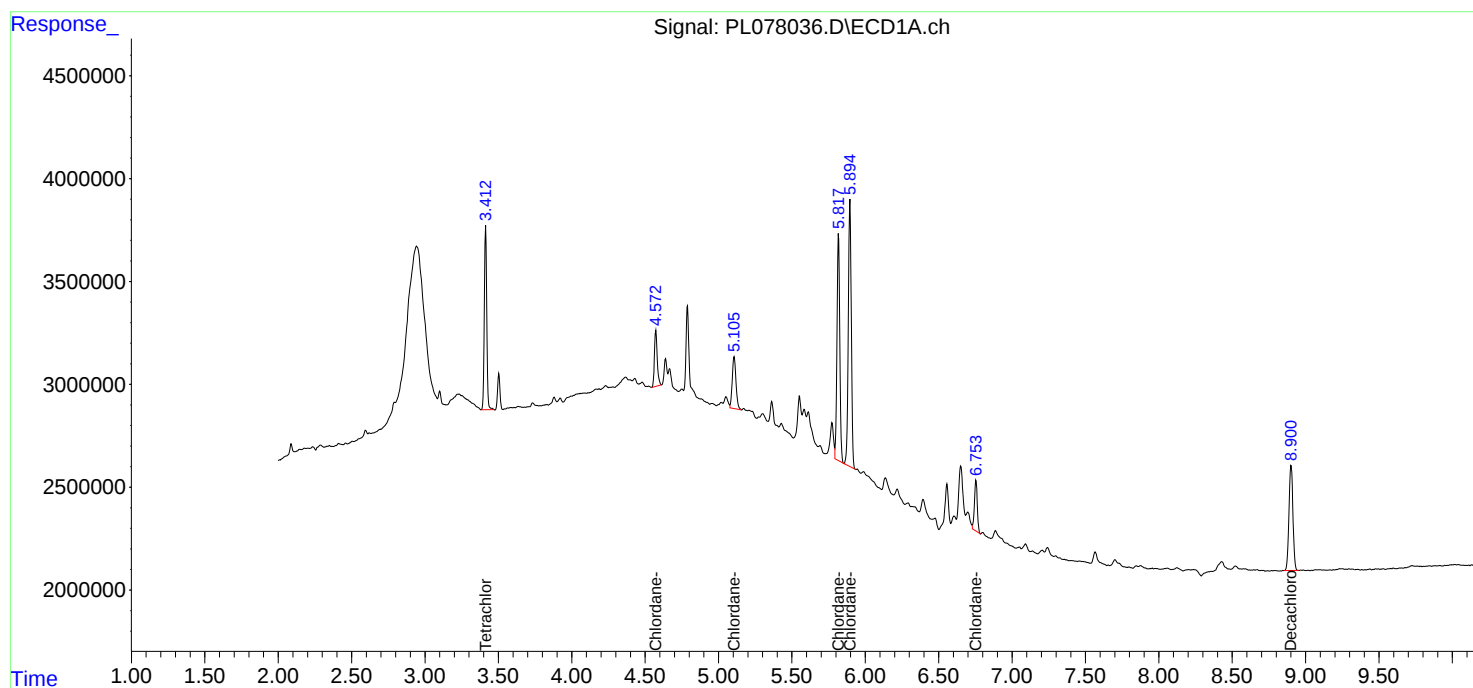


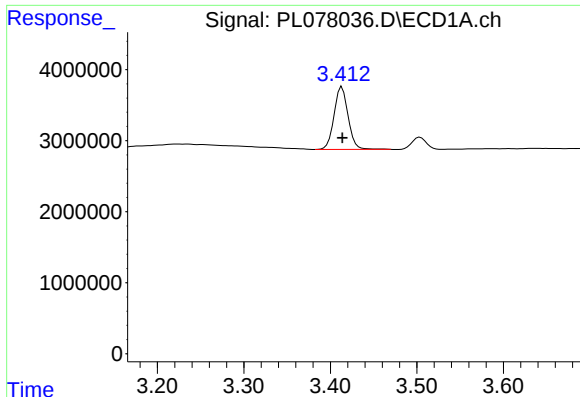

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 9926963
Conc: 5.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

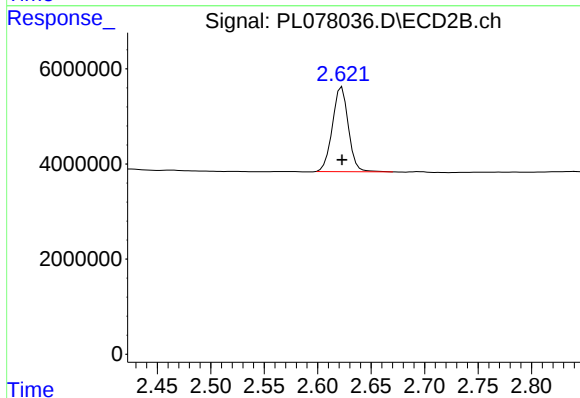


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 18436076
Conc: 5.56 ng/ml

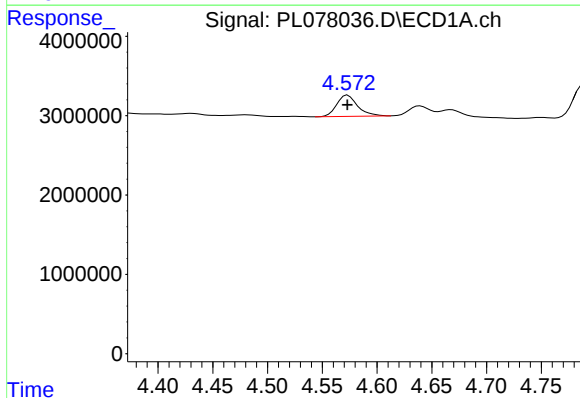


#23 Chlordane-1

R.T.: 4.573 min
Delta R.T.: 0.000 min
Response: 3555390
Conc: 48.00 ng/ml

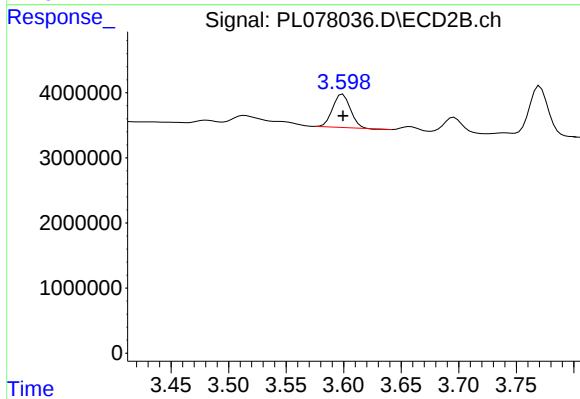

#23 Chlordane-1


R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 5491953
Conc: 54.32 ng/ml

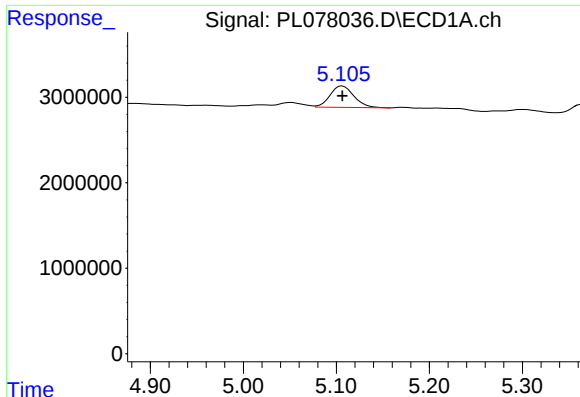

#24 Chlordane-2


R.T.: 5.106 min
Delta R.T.: 0.000 min
Response: 4499233
Conc: 57.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

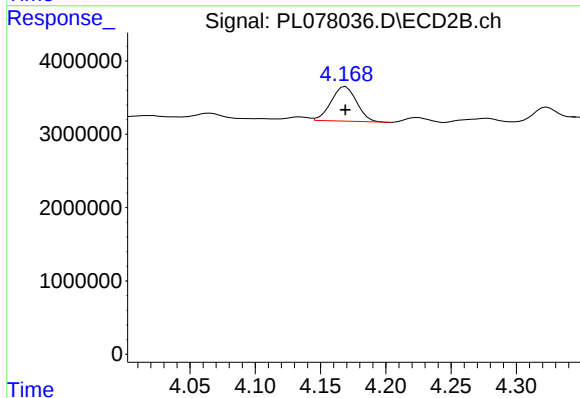


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 6422480
Conc: 59.59 ng/ml

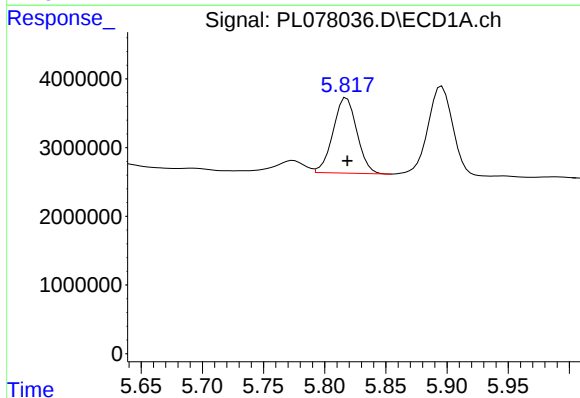


#25 Chlordane-3

R.T.: 5.818 min
Delta R.T.: 0.000 min
Response: 14844331
Conc: 49.93 ng/ml

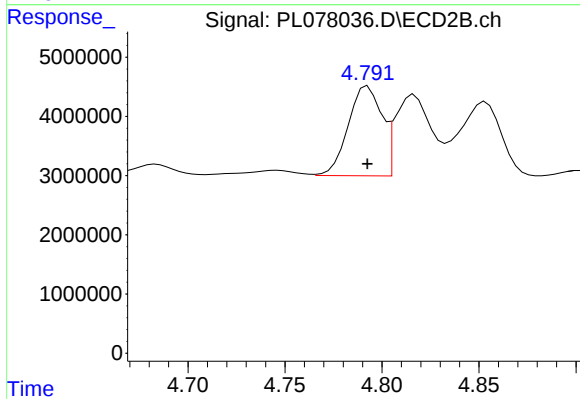

#25 Chlordane-3


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 18239616
Conc: 59.06 ng/ml

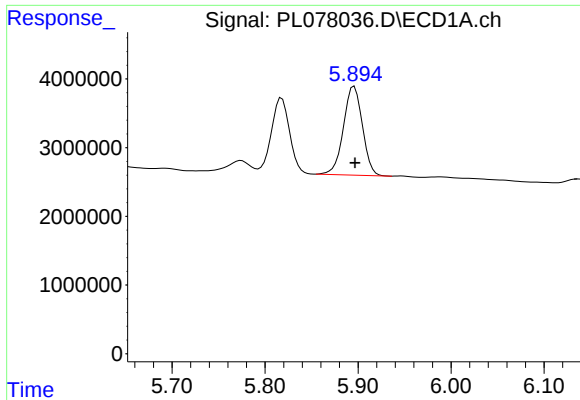

#26 Chlordane-4


R.T.: 5.896 min
Delta R.T.: 0.000 min
Response: 18312942
Conc: 51.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

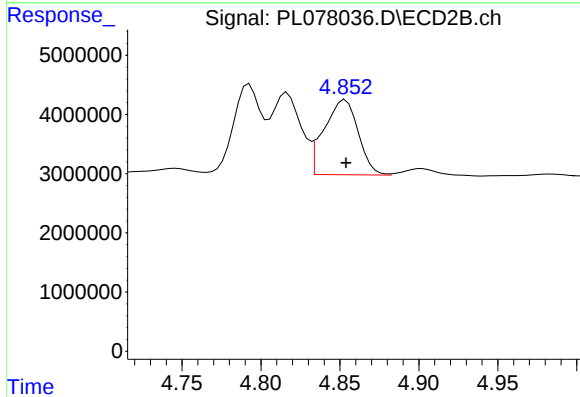


#26 Chlordane-4

R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 19054252
Conc: 58.94 ng/ml

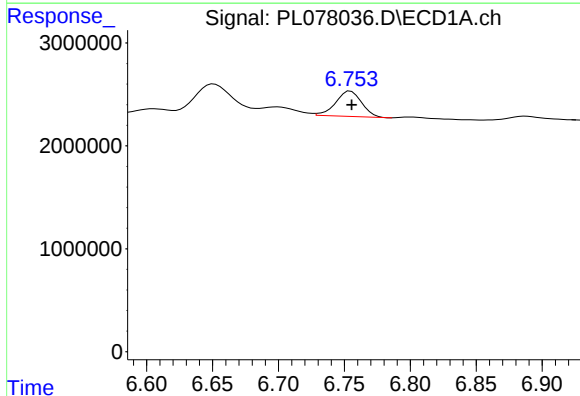


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 3365606
Conc: 56.94 ng/ml

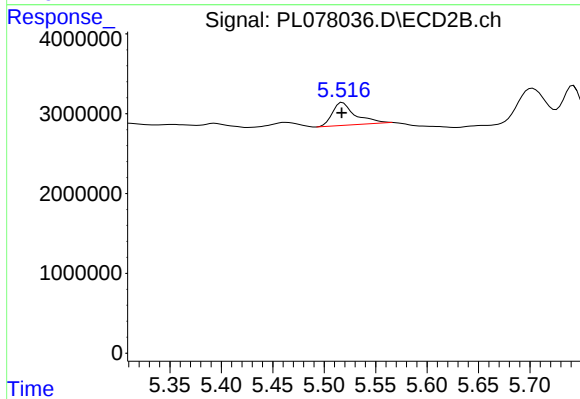

#27 Chlordane-5


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 4431346
Conc: 53.91 ng/ml

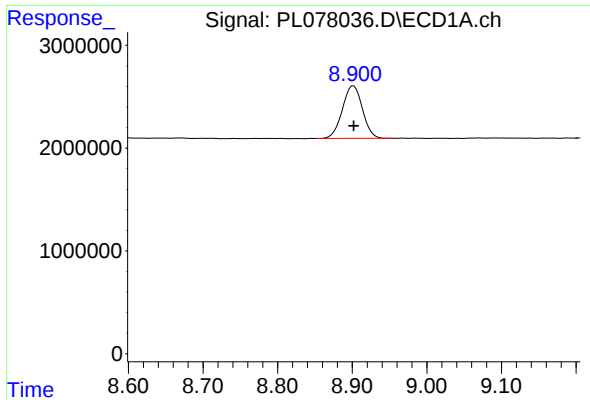

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 9534207
Conc: 6.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

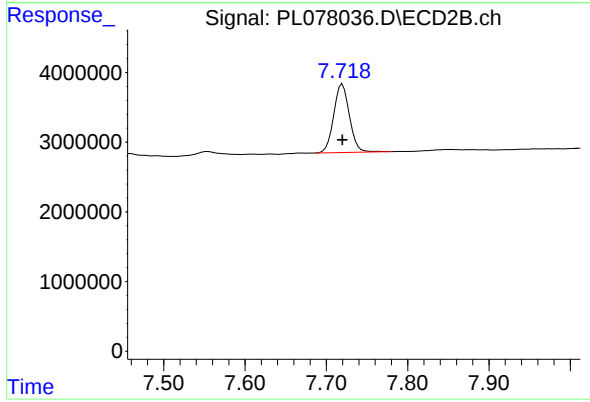

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: 0.000 min
Response: 13210845
Conc: 6.23 ng/ml