

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 17:30
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL100322CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 19:42:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 16:41:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	96857942	171.5E6	51.981	50.570
28)	SA Decachlor...	8.902	7.719	81596076	109.4E6	51.027	49.184
Target Compounds							
23)	Chlordane-1	4.574	3.599	39255466	52461685	535.182	512.474
24)	Chlordane-2	5.107	4.169	41066859	55770266	509.043	500.255
25)	Chlordane-3	5.819	4.793	155.1E6	160.5E6	521.160	499.826
26)	Chlordane-4	5.898	4.854	186.2E6	167.2E6	518.715	499.178
27)	Chlordane-5	6.756	5.518	31673597	42706722	523.083	515.517



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 17:30
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL100322CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 19:42:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 16:41:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

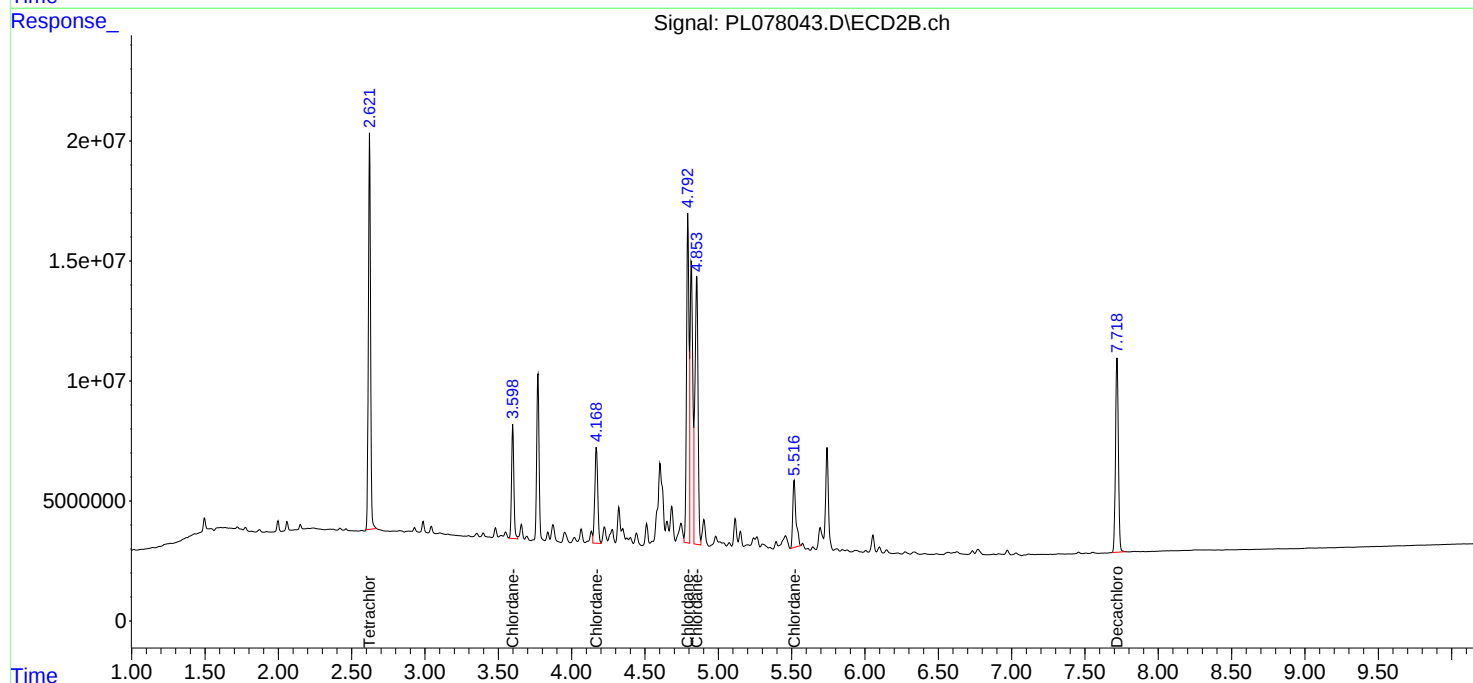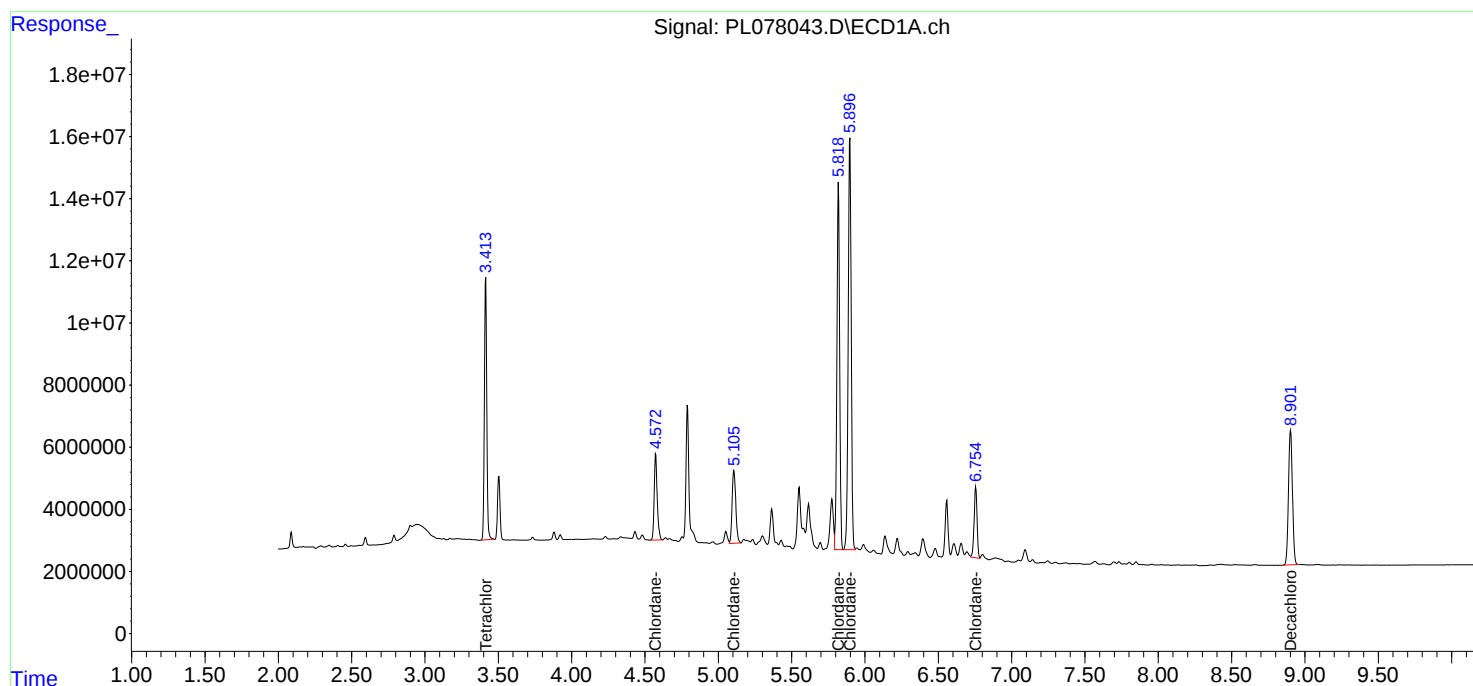


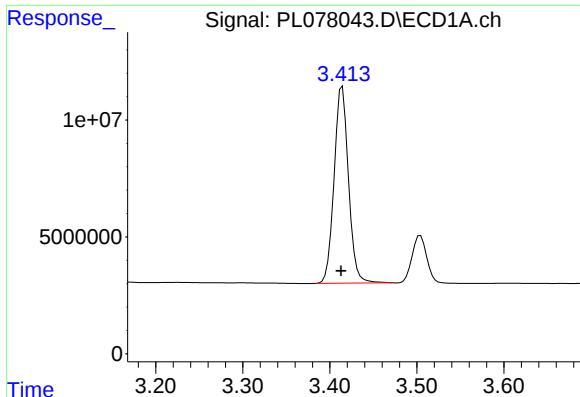

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.001 min
Response: 96857942
Conc: 51.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100322CHLOR

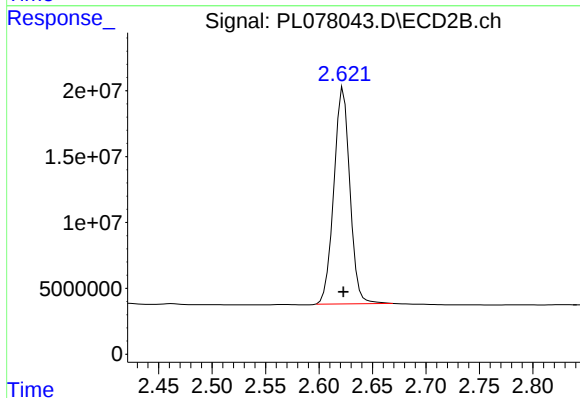


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 171465821
Conc: 50.57 ng/ml

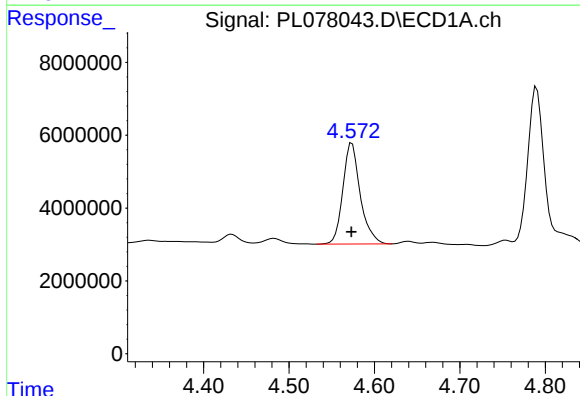


#23 Chlordane-1

R.T.: 4.574 min
Delta R.T.: 0.000 min
Response: 39255466
Conc: 535.18 ng/ml

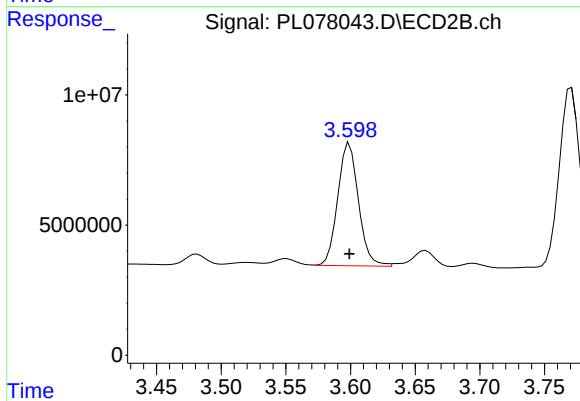

#23 Chlordane-1


R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 52461685
Conc: 512.47 ng/ml

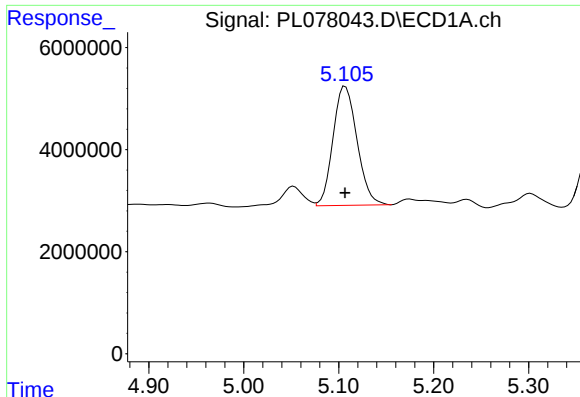

#24 Chlordane-2


R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 41066859
Conc: 509.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100322CHLOR

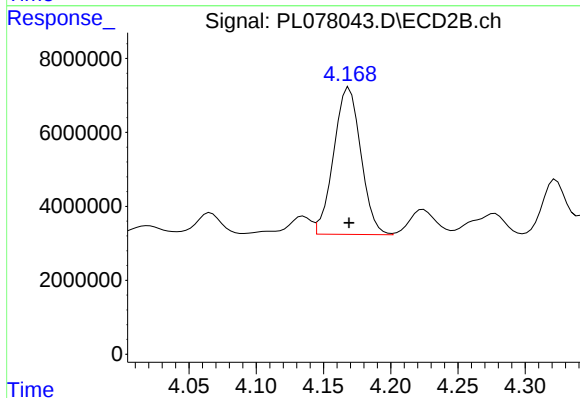


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 55770266
Conc: 500.25 ng/ml

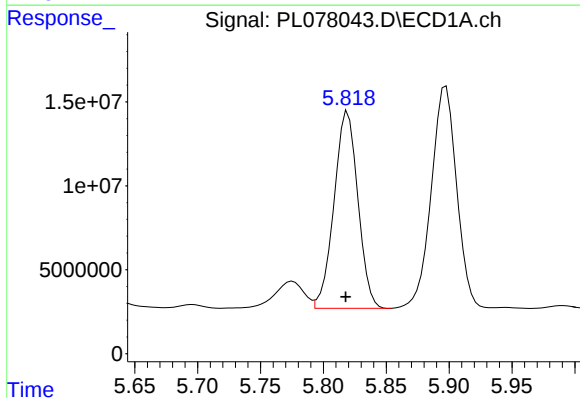


#25 Chlordane-3

R.T.: 5.819 min
Delta R.T.: 0.002 min
Response: 155116008
Conc: 521.16 ng/ml

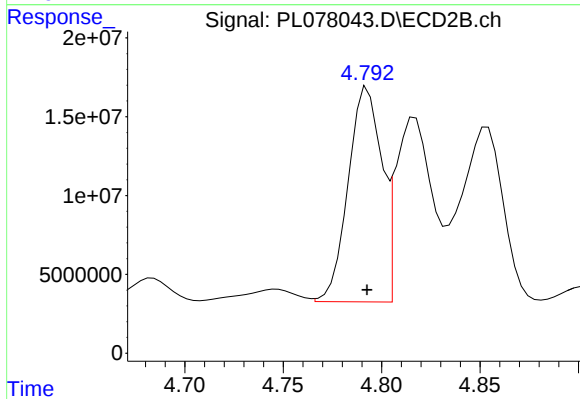

#25 Chlordane-3


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 160460181
Conc: 499.83 ng/ml

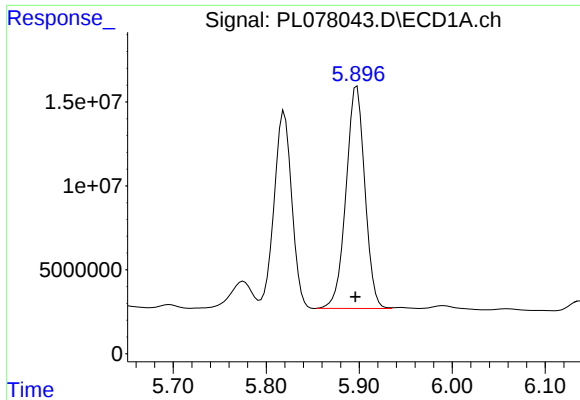

#26 Chlordane-4


R.T.: 5.898 min
Delta R.T.: 0.002 min
Response: 186206612
Conc: 518.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100322CHLOR

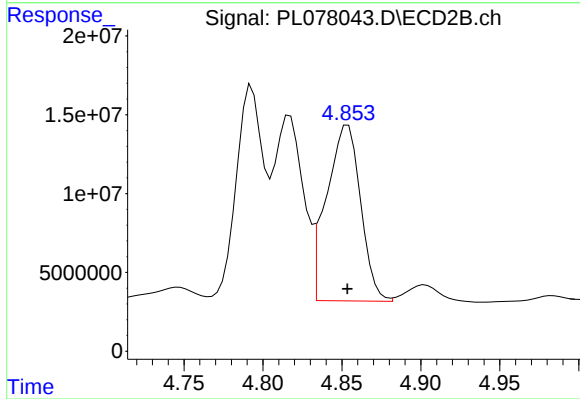


#26 Chlordane-4

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 167214567
Conc: 499.18 ng/ml

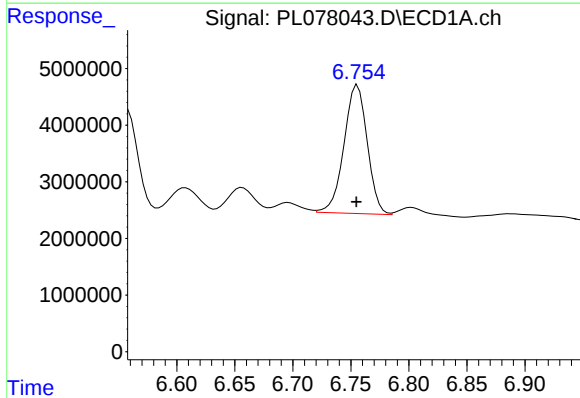


#27 Chlordane-5

R.T.: 6.756 min
Delta R.T.: 0.001 min
Response: 31673597
Conc: 523.08 ng/ml

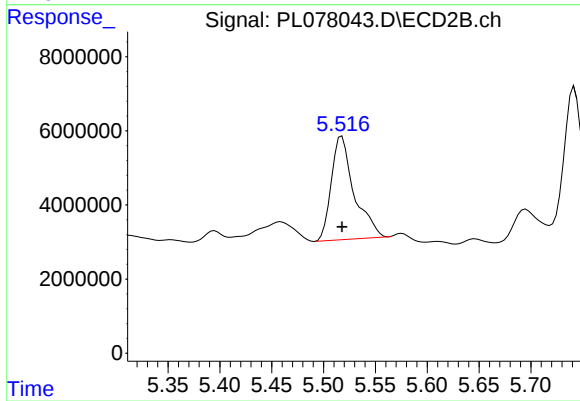

#27 Chlordane-5


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 42706722
Conc: 515.52 ng/ml

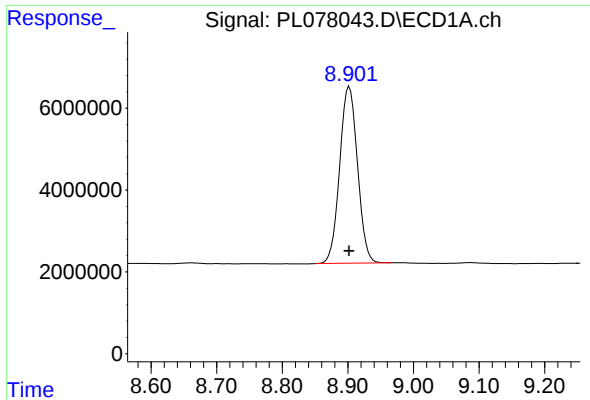

#28 Decachlorobiphenyl

R.T.: 8.902 min
Delta R.T.: 0.000 min
Response: 81596076
Conc: 51.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100322CHLOR

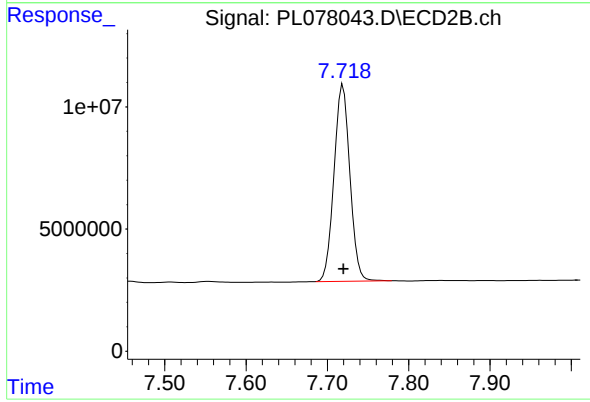

#28 Decachlorobiphenyl

R.T.: 7.719 min
Delta R.T.: 0.000 min
Response: 109435293
Conc: 49.18 ng/ml