

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 21:12
 Operator : AR\AJ
 Sample : N4907-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-222

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/04/2022
 Supervised By :Ankita Jodhani 10/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 22:46:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 19:46:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.412	2.622	18149586	33149013	9.841m	11.794m
28) SA Decachlor...	8.900	7.719	18461298	23755161	11.760	10.947

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 21:12
Operator : AR\AJ
Sample : N4907-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-222


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/04/2022
Supervised By : Ankita Jodhani 10/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 22:46:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 19:46:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

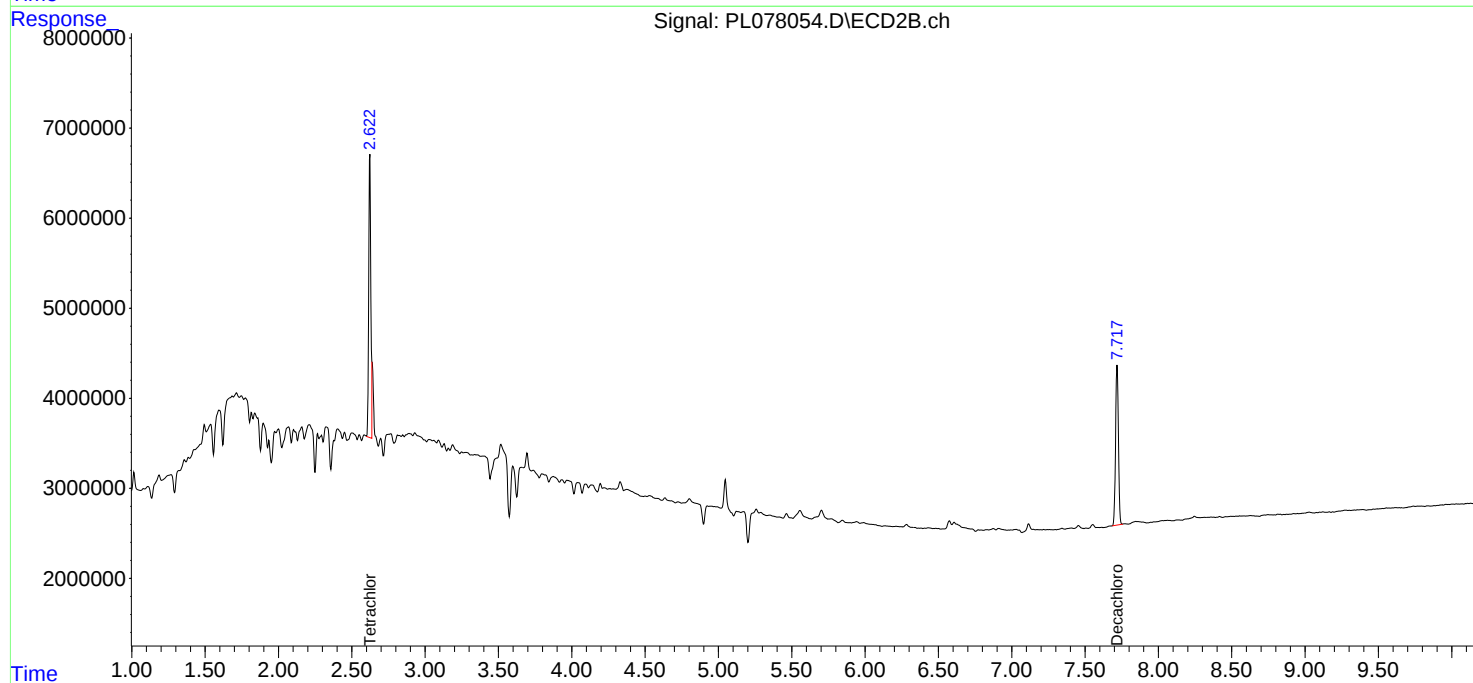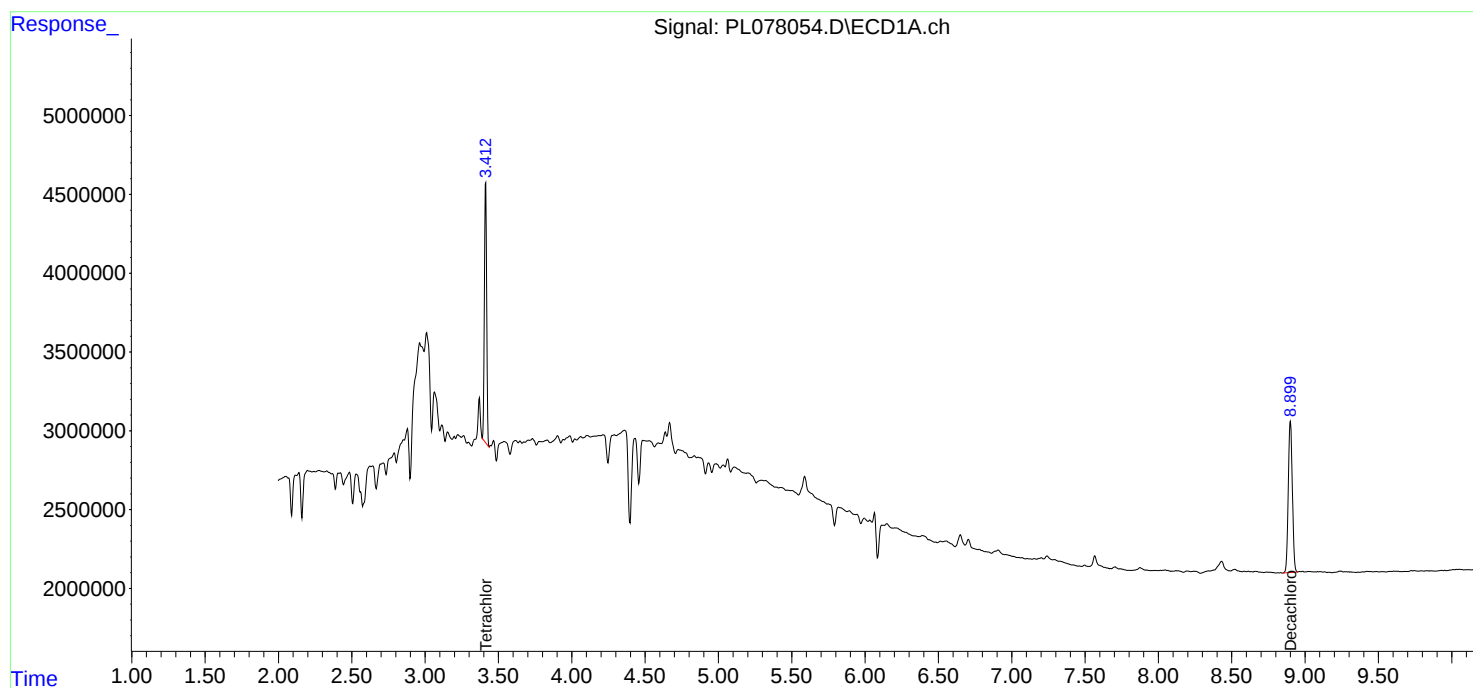

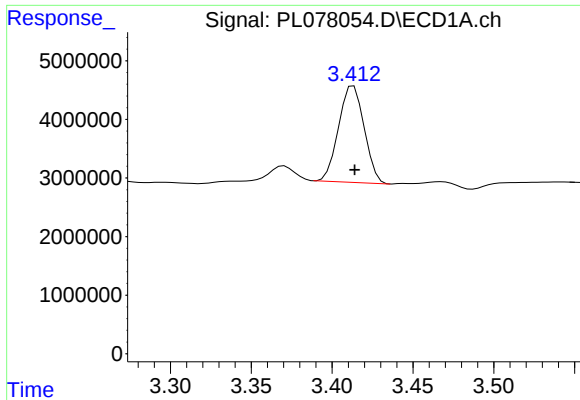


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: -0.002 min
Response: 18149586
Conc: 9.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-222


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/04/2022
Supervised By :Ankita Jodhani 10/04/2022

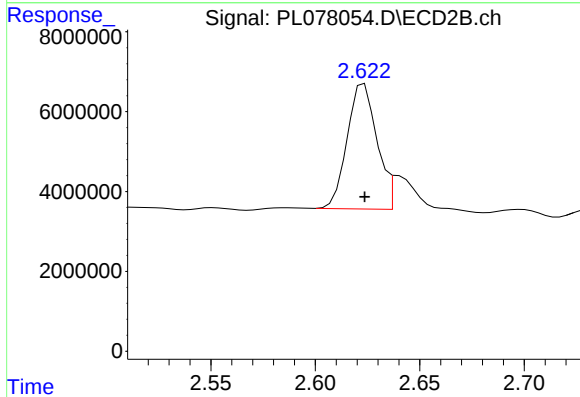


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: -0.002 min
Response: 33149013
Conc: 11.79 ng/ml m

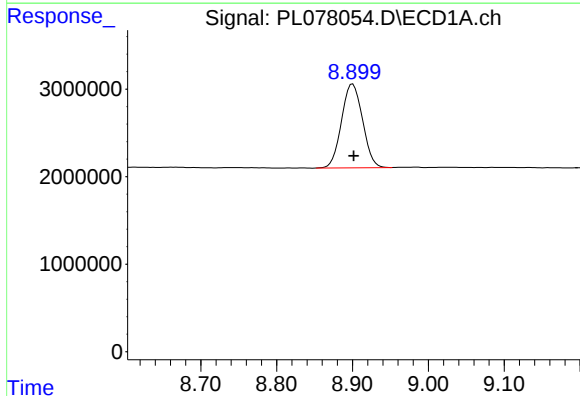

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: -0.002 min
Response: 18461298
Conc: 11.76 ng/ml

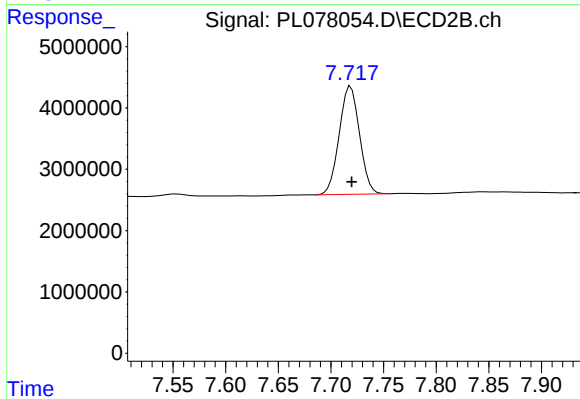

#28 Decachlorobiphenyl

R.T.: 7.719 min
Delta R.T.: -0.001 min
Response: 23755161
Conc: 10.95 ng/ml