

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 21:53
 Operator : AR\AJ
 Sample : N4914-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/04/2022
 Supervised By : Ankita Jodhani 10/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 22:46:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 19:46:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.404	2.632	29670190	104.3E6	16.087m	37.094m#
2)	SA Decachlor...	8.901	7.719	18959672	24087908	12.077	11.100

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 21:53
Operator : AR\AJ
Sample : N4914-03
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
S2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/04/2022
Supervised By : Ankita Jodhani 10/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 22:46:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 19:46:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

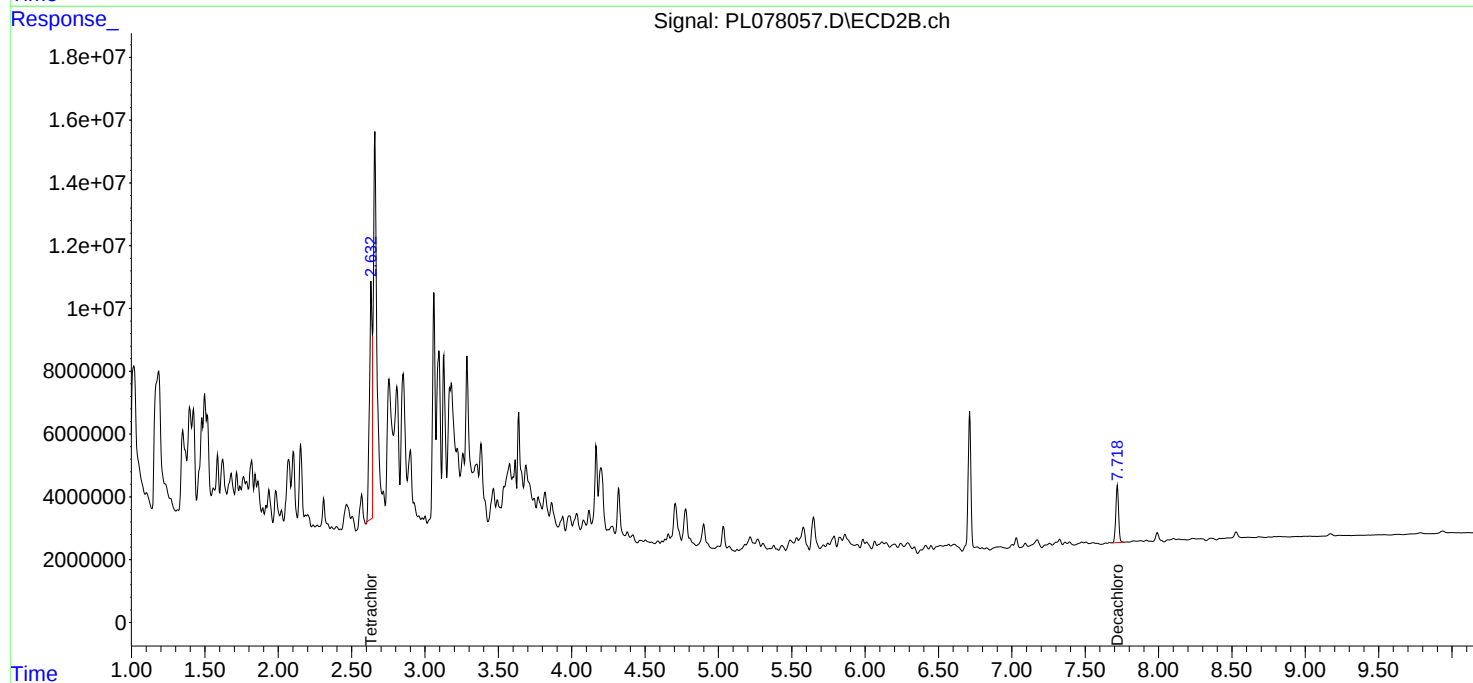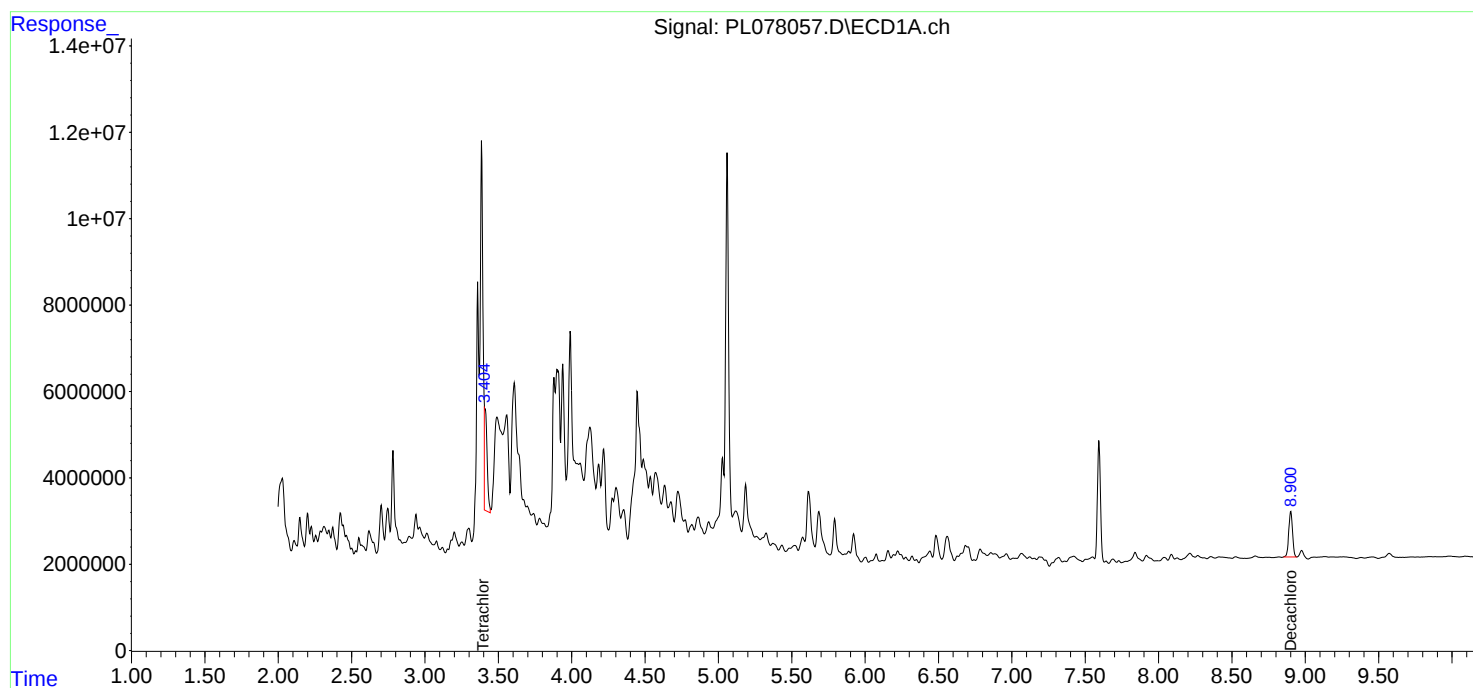

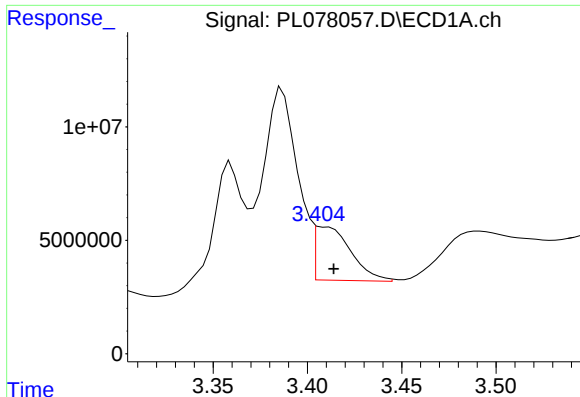


#1 Tetrachloro-m-xylene

R.T.: 3.404 min
Delta R.T.: -0.010 min
Response: 29670190
Conc: 16.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
S2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/04/2022
Supervised By :Ankita Jodhani 10/04/2022

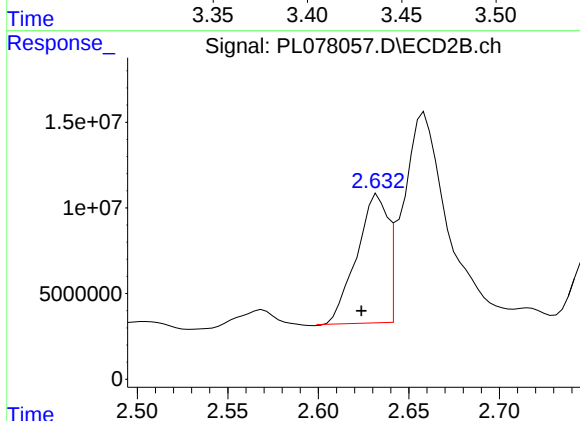


#1 Tetrachloro-m-xylene

R.T.: 2.632 min
Delta R.T.: 0.008 min
Response: 104259247
Conc: 37.09 ng/ml m

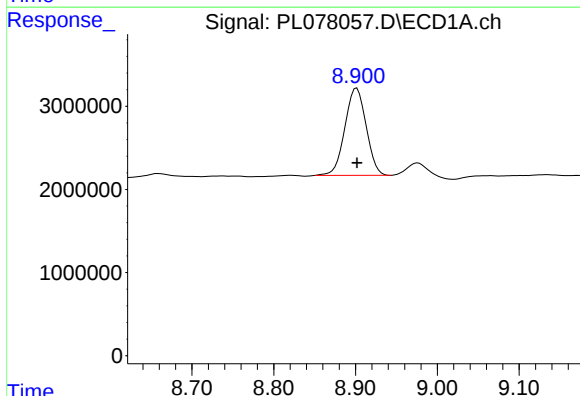

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.000 min
Response: 18959672
Conc: 12.08 ng/ml

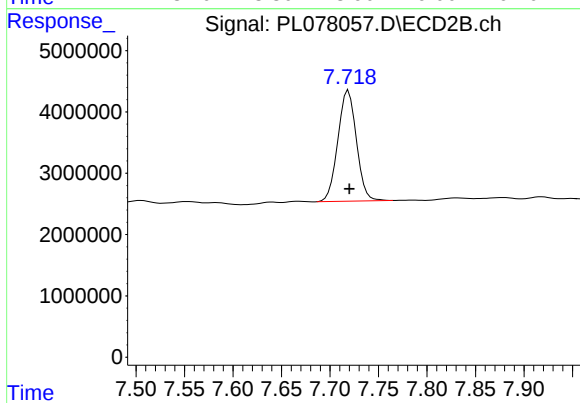

#28 Decachlorobiphenyl

R.T.: 7.719 min
Delta R.T.: 0.000 min
Response: 24087908
Conc: 11.10 ng/ml