

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
 Data File : PL078061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2022 23:02
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 06:22:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 19:46:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	102.8E6	180.2E6	55.737	64.108
28)	SA Decachlor...	8.901	7.720	87712247	117.0E6	55.871	53.928
Target Compounds							
23)	Chlordane-1	4.573	3.600	42280279	55910083	576.420	546.160
24)	Chlordane-2	5.107	4.169	44229127	59538467	548.241	534.055
25)	Chlordane-3	5.819	4.793	169.2E6	170.7E6	568.547	531.756
26)	Chlordane-4	5.897	4.854	201.9E6	179.5E6	562.382	535.707
27)	Chlordane-5	6.755	5.518	34492486	46035682	569.636	555.701



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100322\
Data File : PL078061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2022 23:02
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 06:22:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 19:46:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

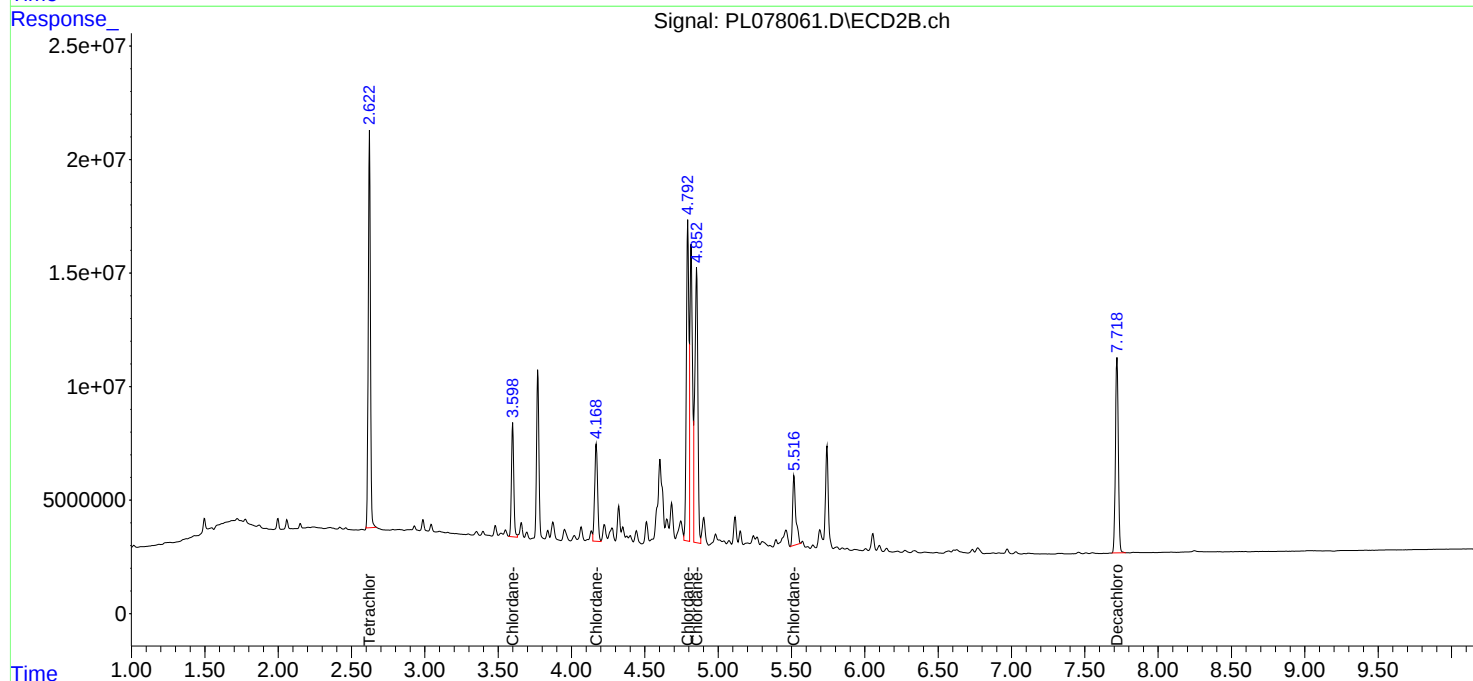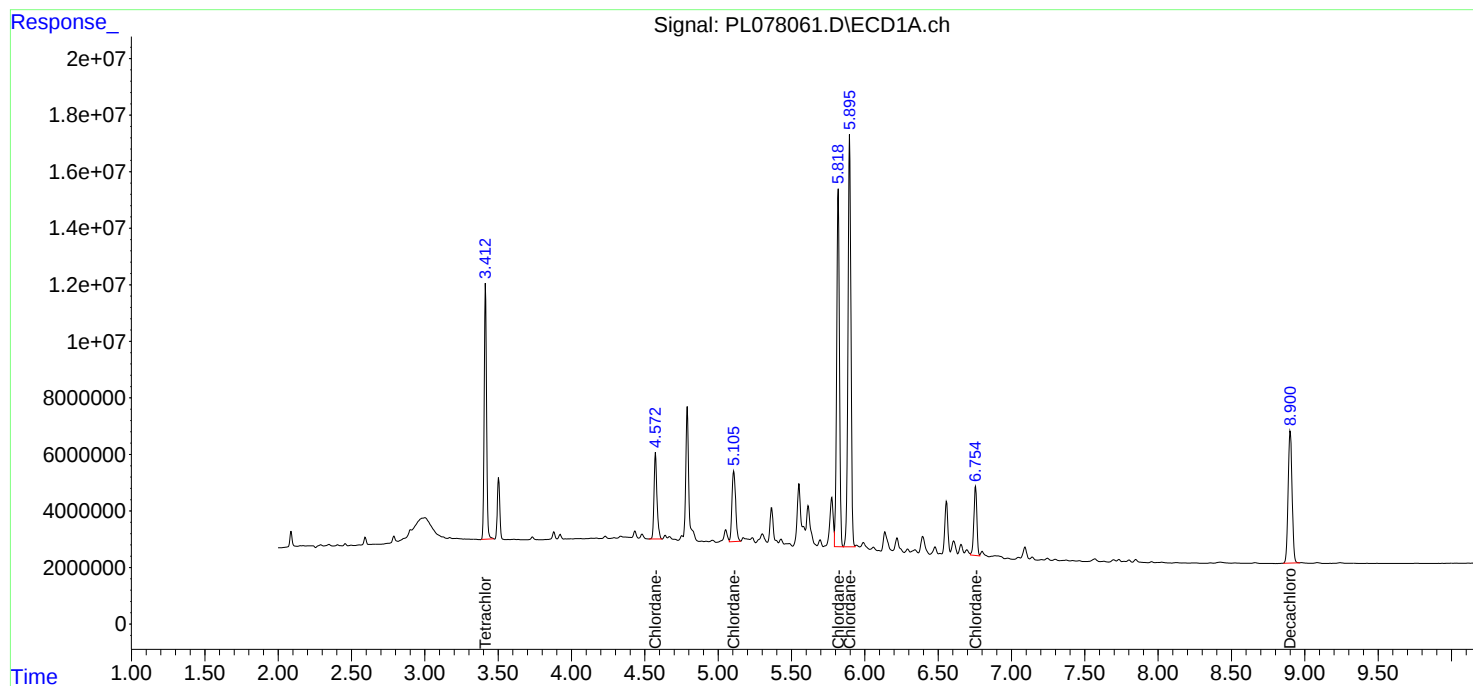


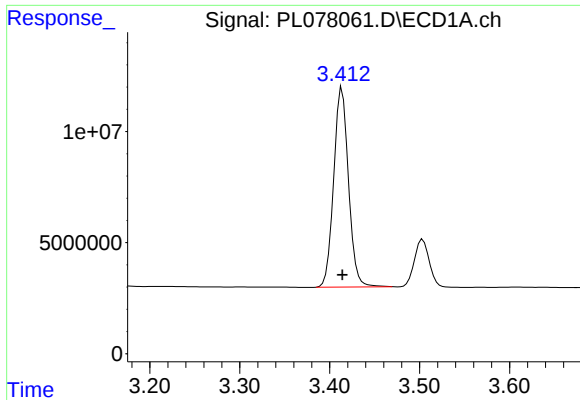

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.000 min
Response: 102796940
Conc: 55.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

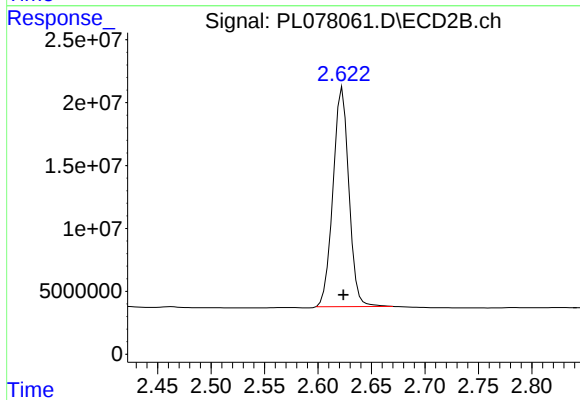


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 180185561
Conc: 64.11 ng/ml

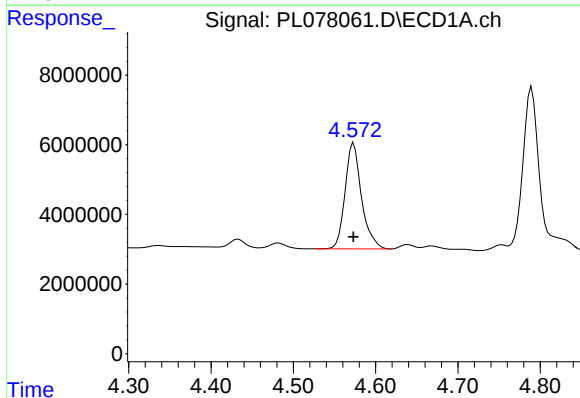


#23 Chlordane-1

R.T.: 4.573 min
Delta R.T.: 0.000 min
Response: 42280279
Conc: 576.42 ng/ml

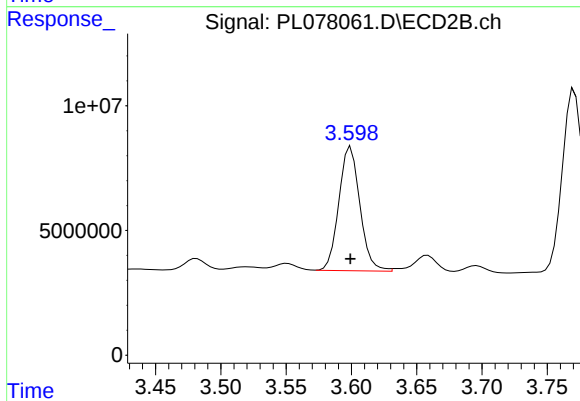

#23 Chlordane-1


R.T.: 3.600 min
Delta R.T.: 0.000 min
Response: 55910083
Conc: 546.16 ng/ml

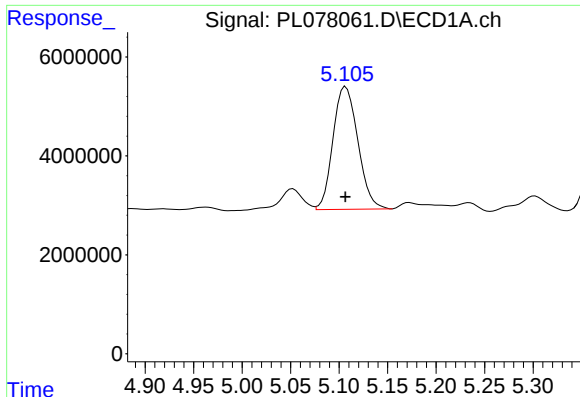

#24 Chlordane-2


R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 44229127
Conc: 548.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

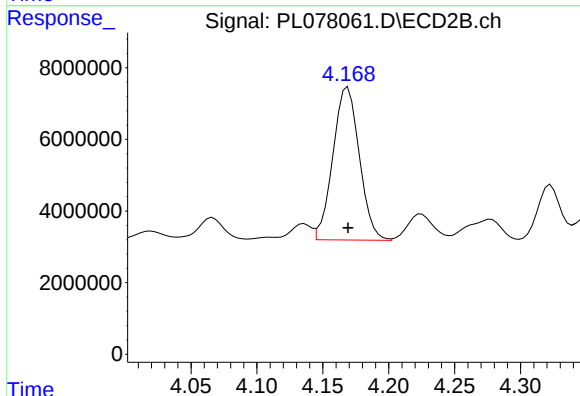


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 59538467
Conc: 534.06 ng/ml

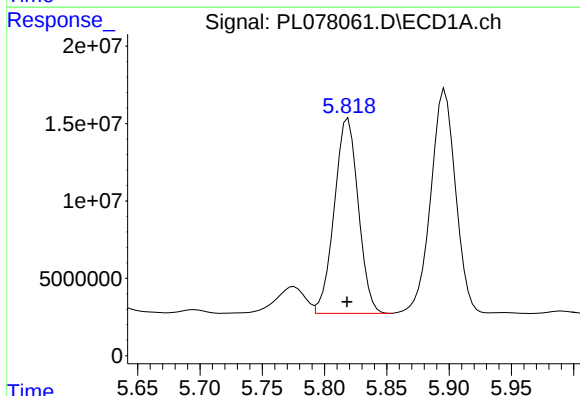


#25 Chlordane-3

R.T.: 5.819 min
Delta R.T.: 0.000 min
Response: 169220145
Conc: 568.55 ng/ml

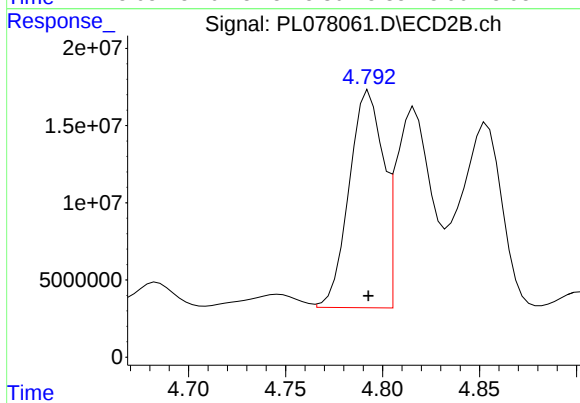

#25 Chlordane-3


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 170710870
Conc: 531.76 ng/ml

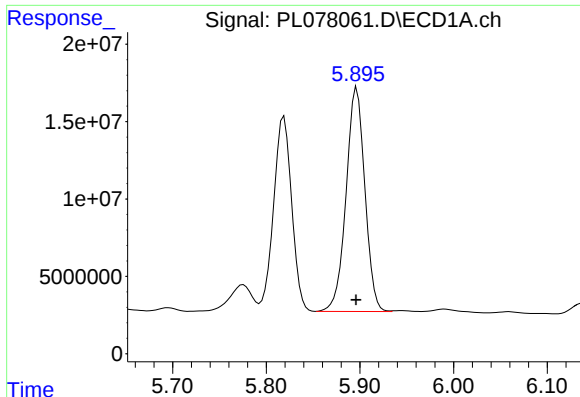

#26 Chlordane-4


R.T.: 5.897 min
Delta R.T.: 0.000 min
Response: 201882136
Conc: 562.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

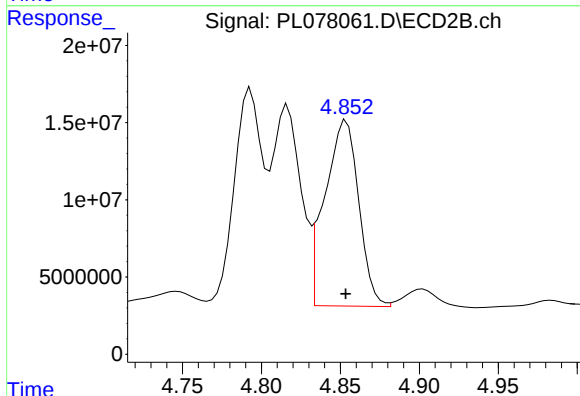


#26 Chlordane-4

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 179451037
Conc: 535.71 ng/ml

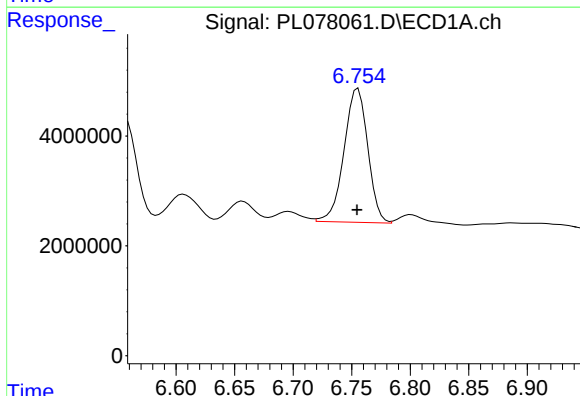


#27 Chlordane-5

R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 34492486
Conc: 569.64 ng/ml

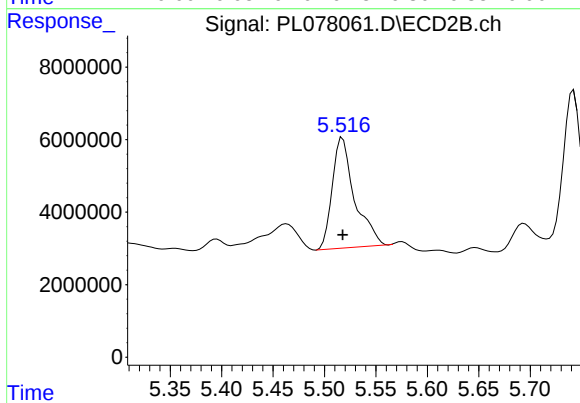

#27 Chlordane-5


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 46035682
Conc: 555.70 ng/ml

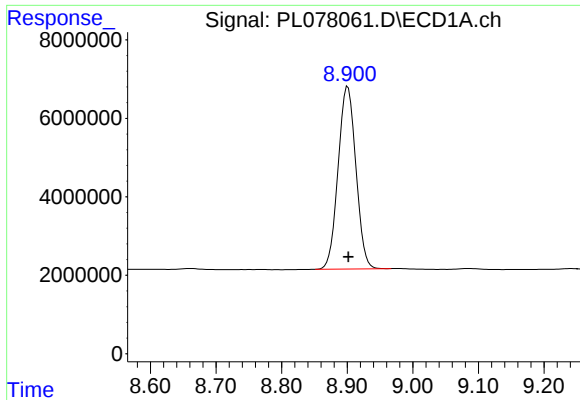

#28 Decachlorobiphenyl

R.T.: 8.901 min
Delta R.T.: 0.000 min
Response: 87712247
Conc: 55.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

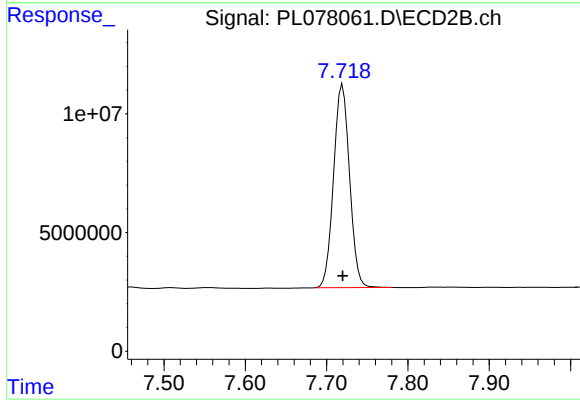

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: 0.000 min
Response: 117028441
Conc: 53.93 ng/ml