

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100323\
 Data File : PL085660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 16:04
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 17:44:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 17:36:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	2.622	298.5E6	117.4E6	101.593	101.322
28)	SA Decachlor...	8.858	7.775	212.9E6	88578756	99.268	98.693
Target Compounds							
23)	Chlordane-1	4.517	3.613	125.4E6	32776329	1021.704	1010.490
24)	Chlordane-2	5.049	4.191	127.0E6	37816417	997.570	987.435
25)	Chlordane-3	5.761	4.820	534.5E6	106.3E6	1025.207	1023.945
26)	Chlordane-4	5.843	4.882	648.8E6	115.9E6	1017.130	1019.846
27)	Chlordane-5	6.689	5.551	100.5E6	29433574	1007.462	1007.347



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100323\
Data File : PL085660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 16:04
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 17:44:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 17:36:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

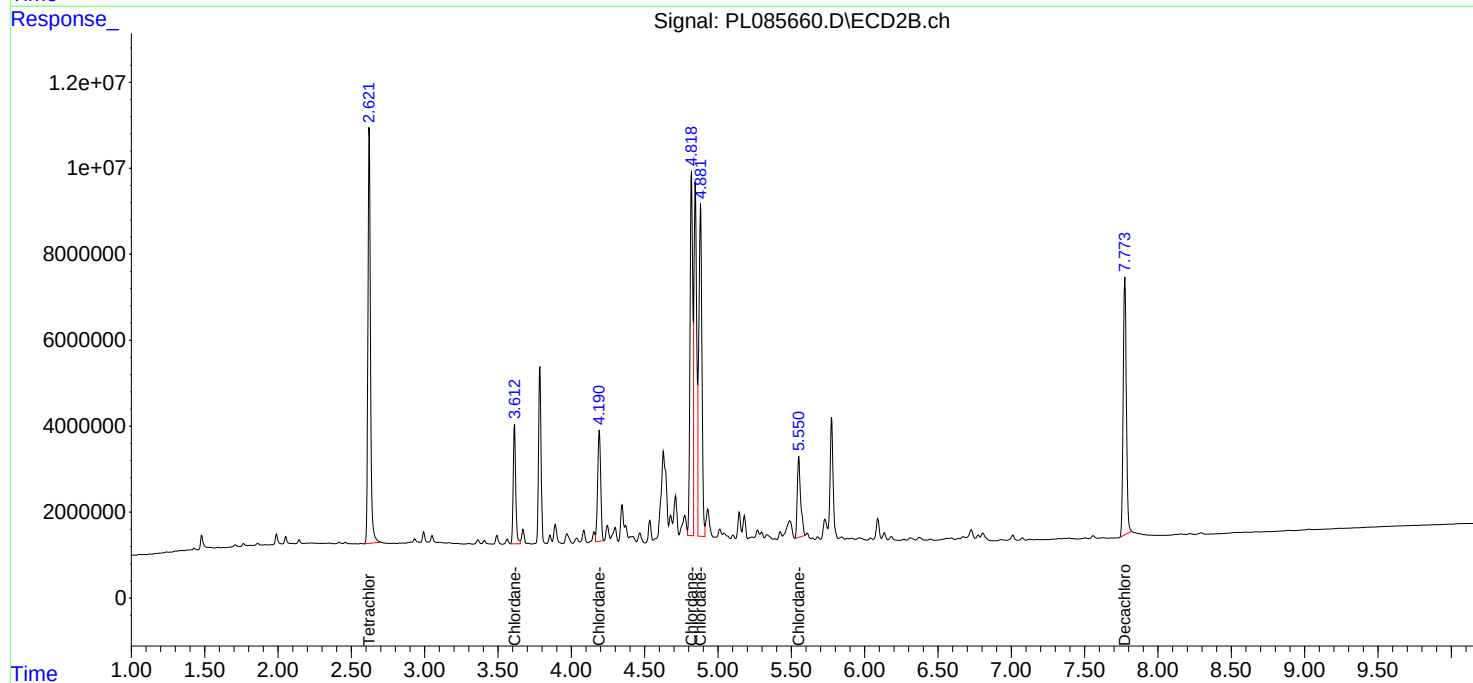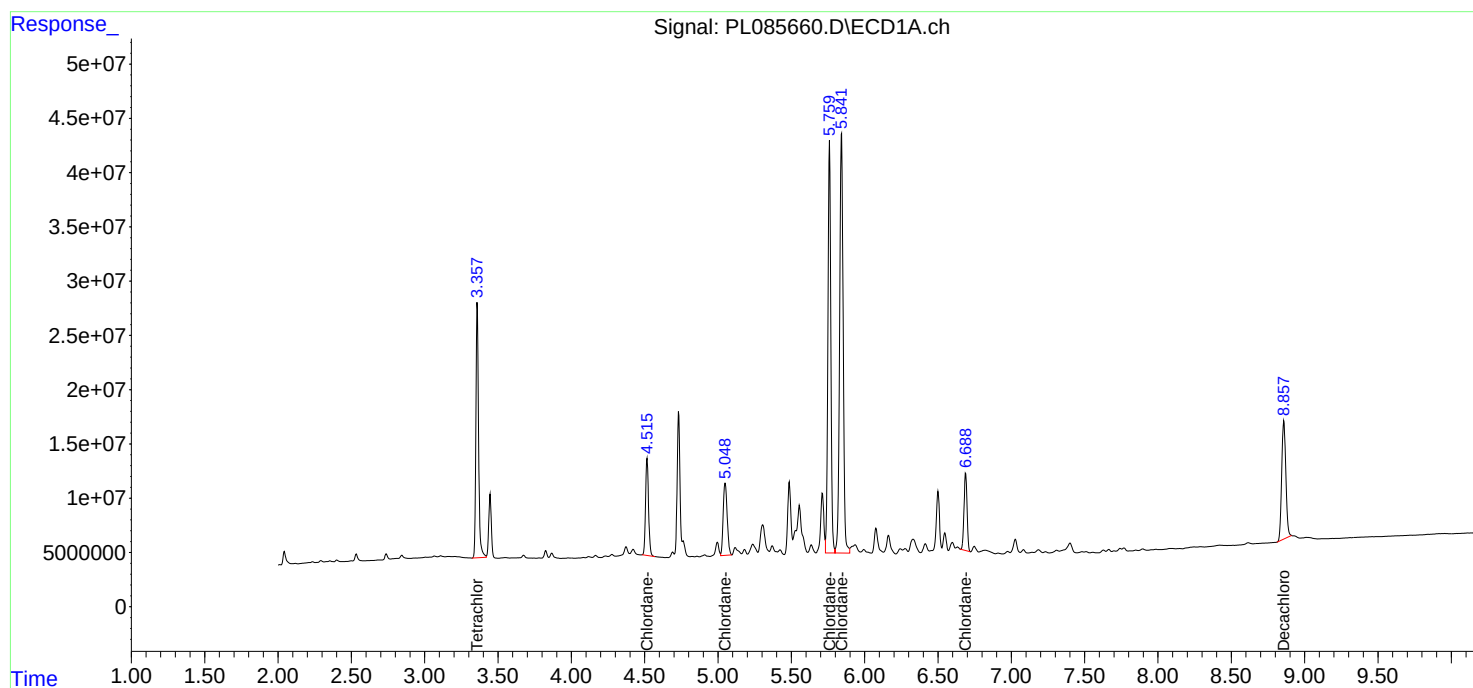


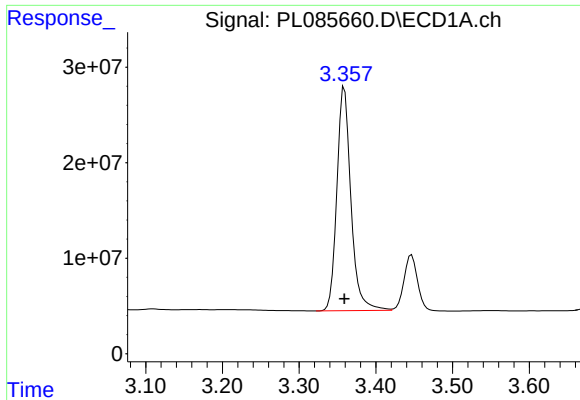

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 298541325
Conc: 101.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

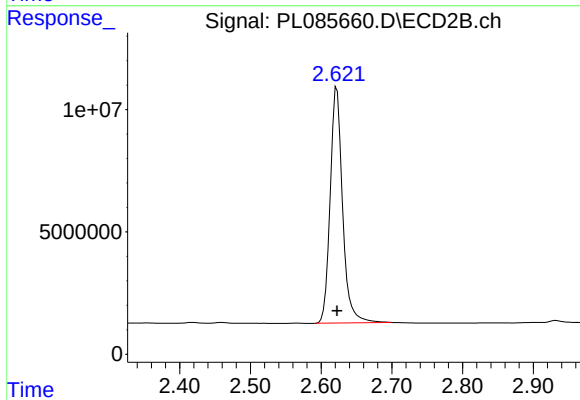


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 117374335
Conc: 101.32 ng/ml

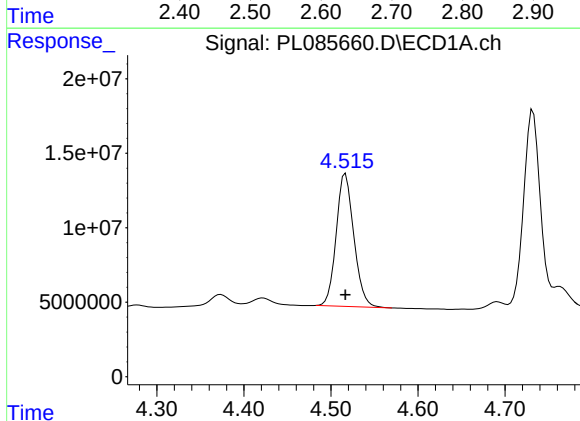


#23 Chlordane-1

R.T.: 4.517 min
Delta R.T.: 0.000 min
Response: 125444600
Conc: 1021.70 ng/ml

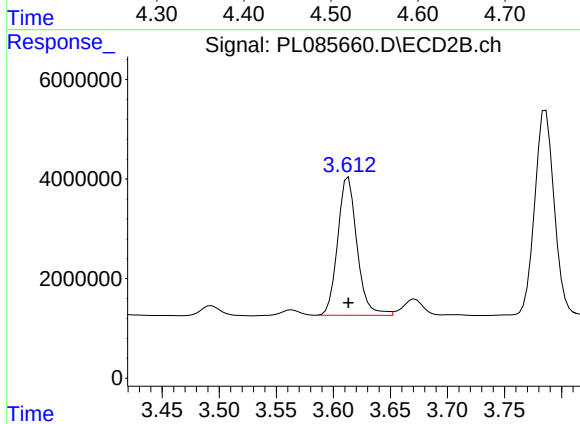

#23 Chlordane-1


R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 32776329
Conc: 1010.49 ng/ml

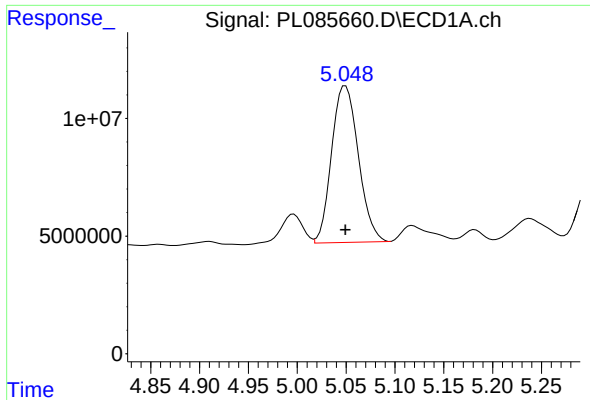

#24 Chlordane-2


R.T.: 5.049 min
Delta R.T.: 0.000 min
Response: 127034821
Conc: 997.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

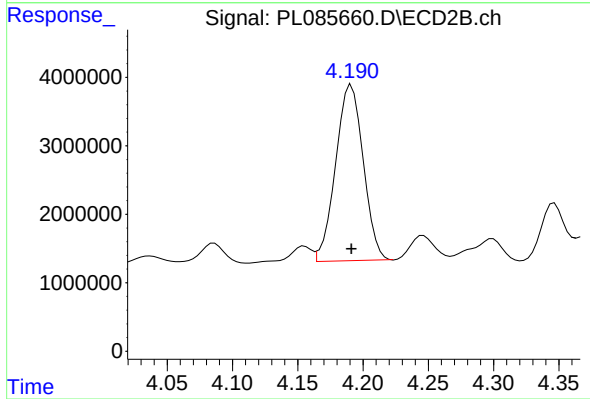


#24 Chlordane-2

R.T.: 4.191 min
Delta R.T.: 0.000 min
Response: 37816417
Conc: 987.44 ng/ml

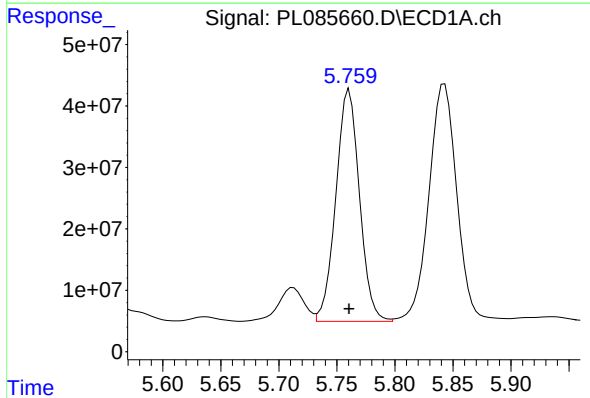


#25 Chlordane-3

R.T.: 5.761 min
Delta R.T.: 0.000 min
Response: 534486772
Conc: 1025.21 ng/ml

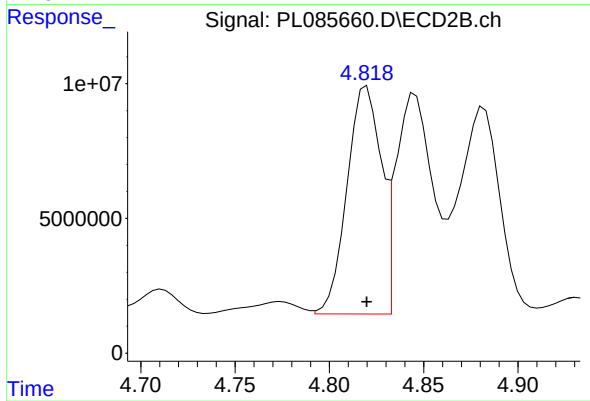

#25 Chlordane-3


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 106270561
Conc: 1023.95 ng/ml

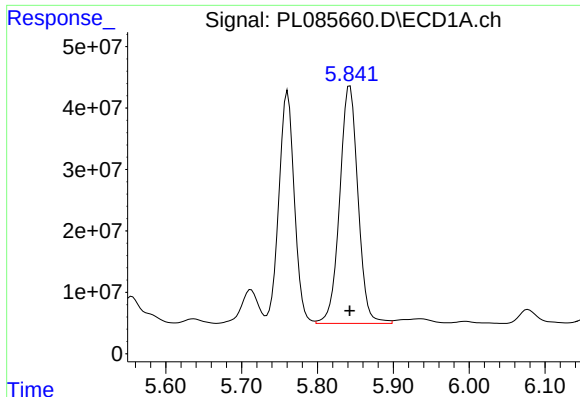

#26 Chlordane-4


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 648837698
Conc: 1017.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

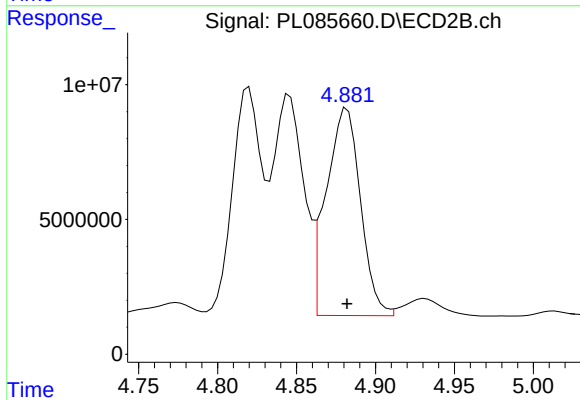


#26 Chlordane-4

R.T.: 4.882 min
Delta R.T.: 0.000 min
Response: 115923797
Conc: 1019.85 ng/ml

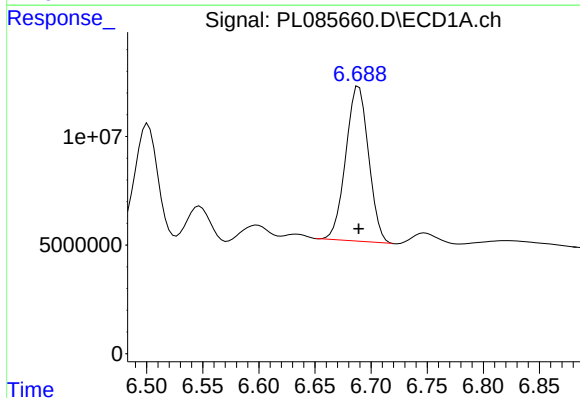


#27 Chlordane-5

R.T.: 6.689 min
Delta R.T.: 0.000 min
Response: 100471902
Conc: 1007.46 ng/ml

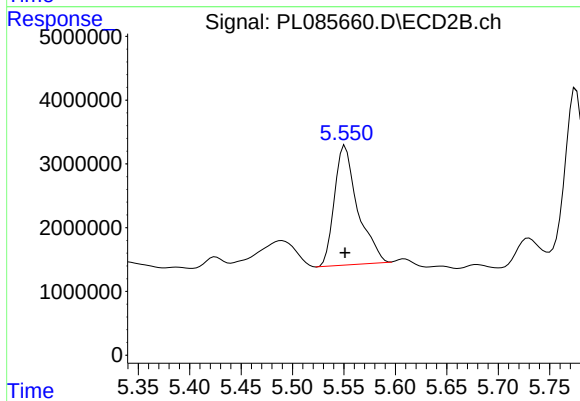

#27 Chlordane-5


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 29433574
Conc: 1007.35 ng/ml

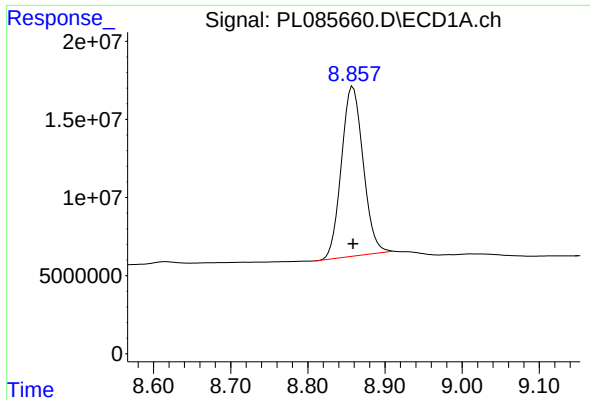

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 212885293
Conc: 99.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

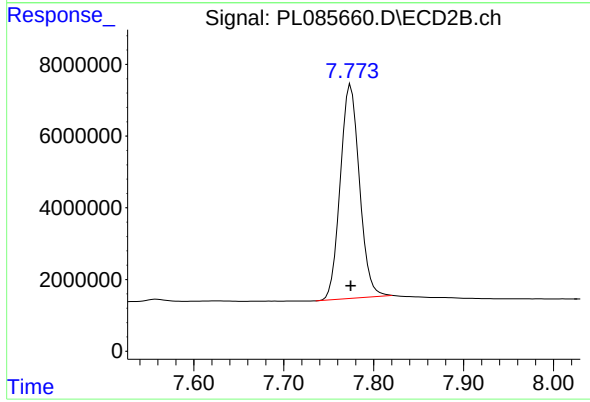

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 88578756
Conc: 98.69 ng/ml