

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100323\
 Data File : PL085661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 16:18
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 17:46:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 17:36:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	2.623	215.5E6	85025854	73.884	73.924
28)	SA Decachlor...	8.859	7.775	155.9E6	65052297	73.461	73.301
Target Compounds							
23)	Chlordane-1	4.518	3.613	90134264	23594221	739.333	734.785
24)	Chlordane-2	5.049	4.191	93185683	27788491	737.742	733.550
25)	Chlordane-3	5.760	4.820	382.3E6	76044805	738.727	738.385
26)	Chlordane-4	5.843	4.881	468.3E6	83077335	739.309	737.142
27)	Chlordane-5	6.689	5.552	72890559	21369787	737.155	737.476



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100323\
Data File : PL085661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 16:18
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 17:46:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 17:36:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

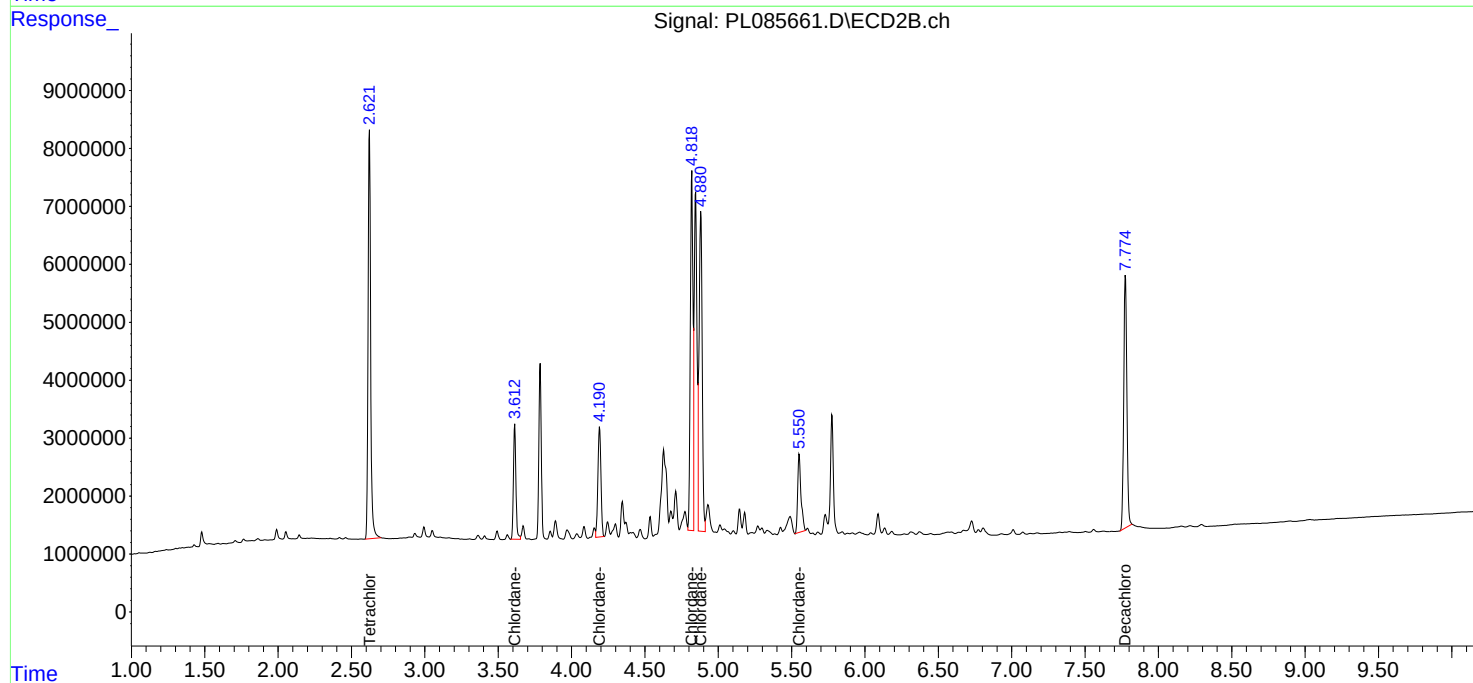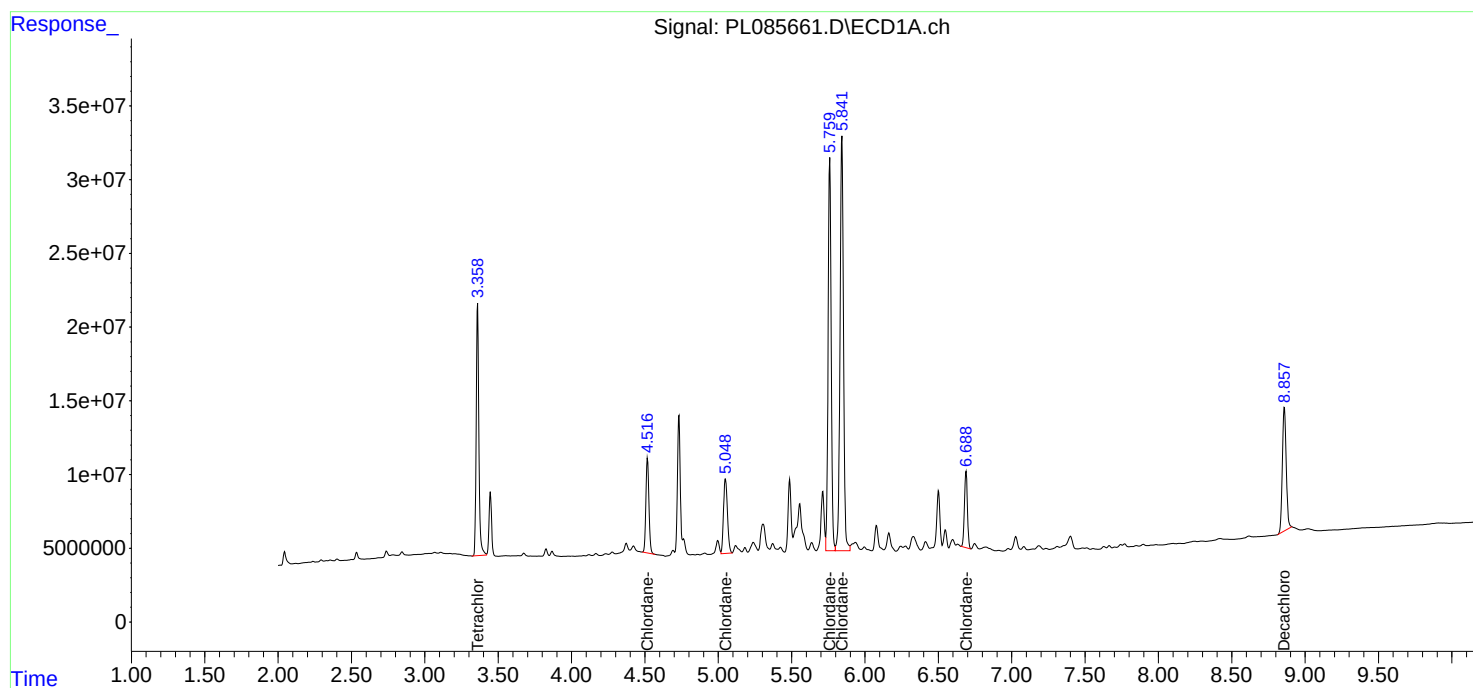


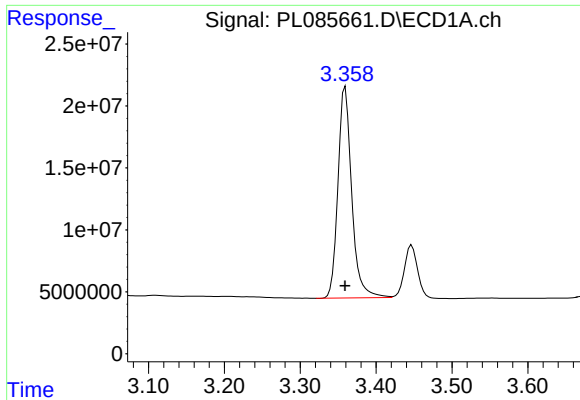

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 215510836
Conc: 73.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

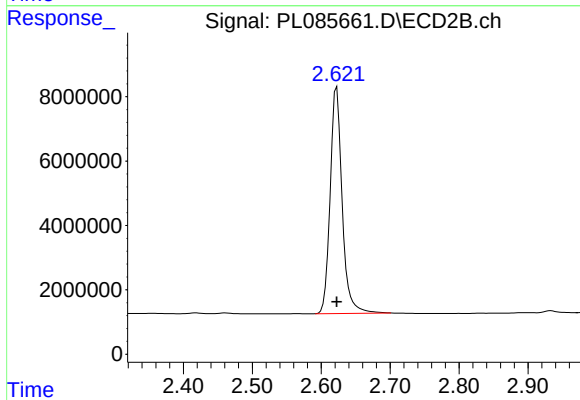


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 85025854
Conc: 73.92 ng/ml

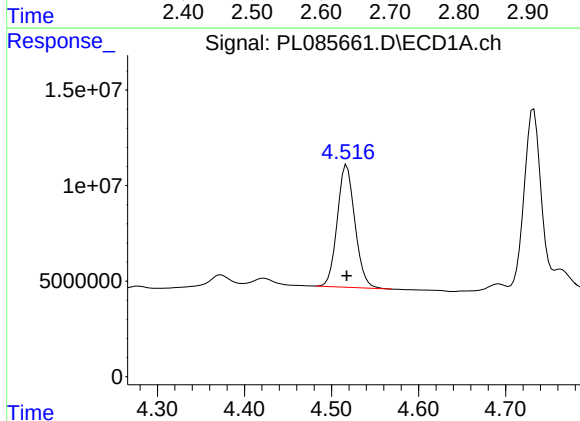


#23 Chlordane-1

R.T.: 4.518 min
Delta R.T.: 0.000 min
Response: 90134264
Conc: 739.33 ng/ml

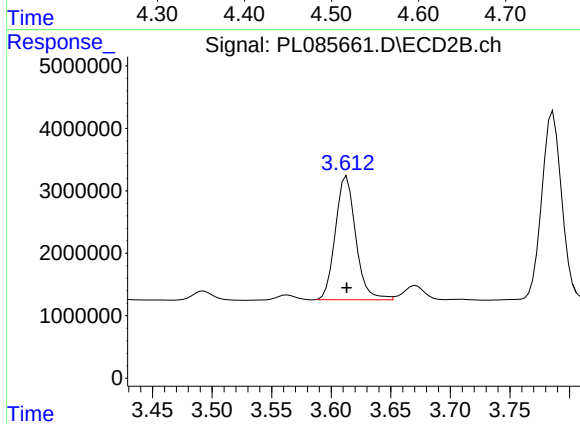

#23 Chlordane-1


R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 23594221
Conc: 734.79 ng/ml

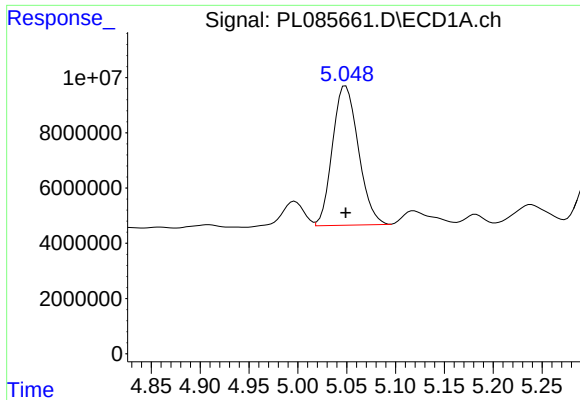

#24 Chlordane-2


R.T.: 5.049 min
Delta R.T.: 0.000 min
Response: 93185683
Conc: 737.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

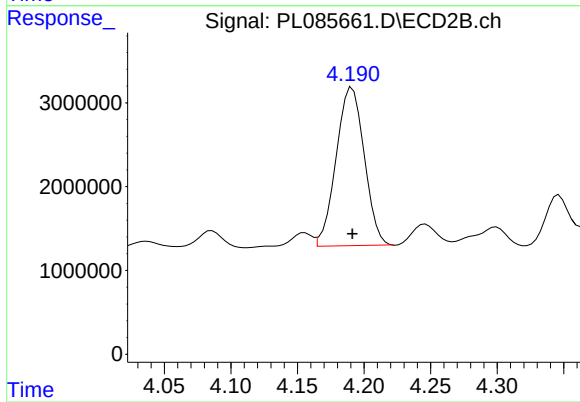


#24 Chlordane-2

R.T.: 4.191 min
Delta R.T.: 0.000 min
Response: 27788491
Conc: 733.55 ng/ml

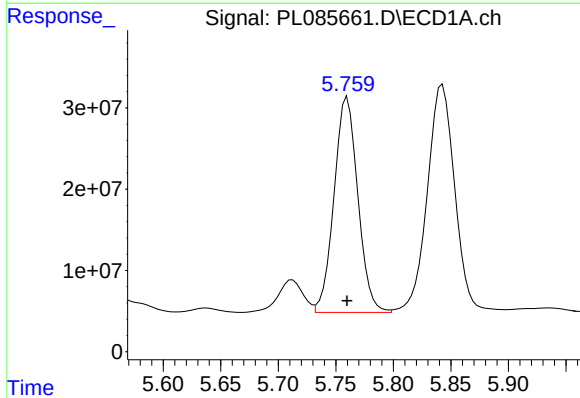


#25 Chlordane-3

R.T.: 5.760 min
Delta R.T.: 0.000 min
Response: 382259121
Conc: 738.73 ng/ml

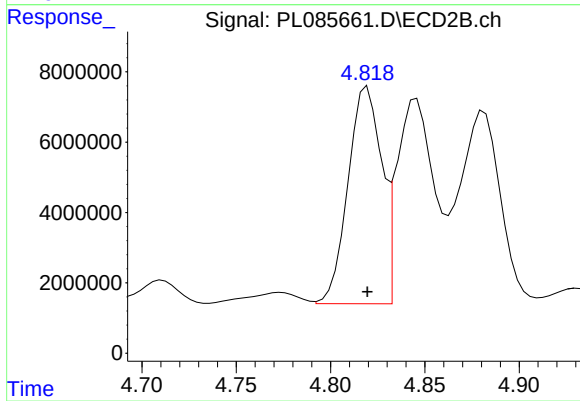

#25 Chlordane-3


R.T.: 4.820 min
Delta R.T.: 0.000 min
Response: 76044805
Conc: 738.39 ng/ml

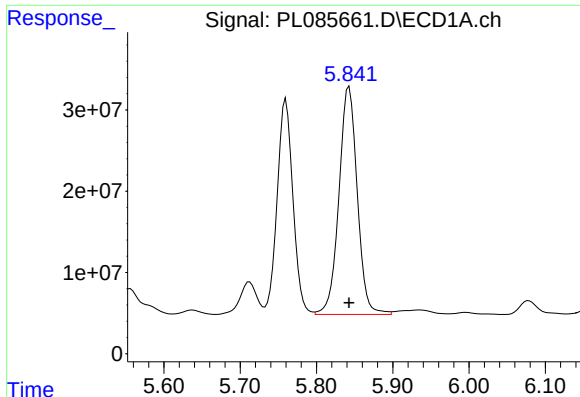

#26 Chlordane-4


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 468275111
Conc: 739.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

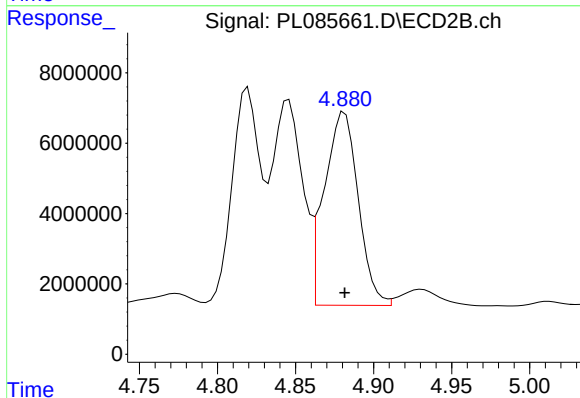


#26 Chlordane-4

R.T.: 4.881 min
Delta R.T.: 0.000 min
Response: 83077335
Conc: 737.14 ng/ml

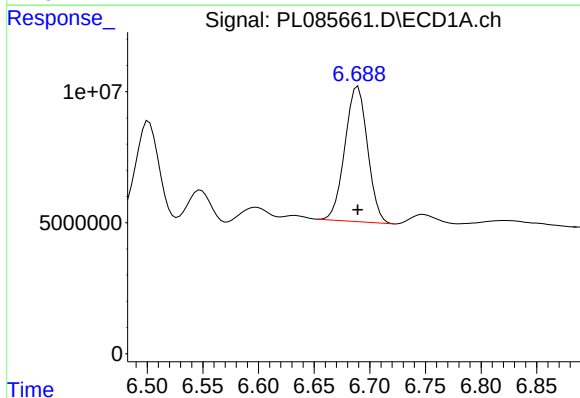


#27 Chlordane-5

R.T.: 6.689 min
Delta R.T.: 0.000 min
Response: 72890559
Conc: 737.15 ng/ml

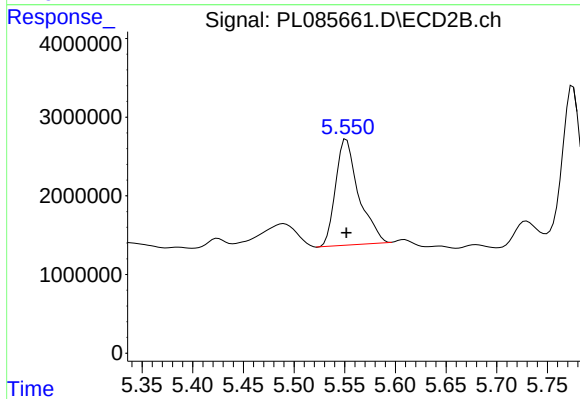

#27 Chlordane-5


R.T.: 5.552 min
Delta R.T.: 0.000 min
Response: 21369787
Conc: 737.48 ng/ml

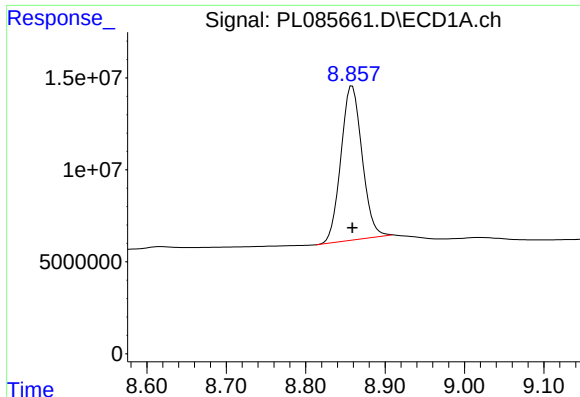

#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 155939594
Conc: 73.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

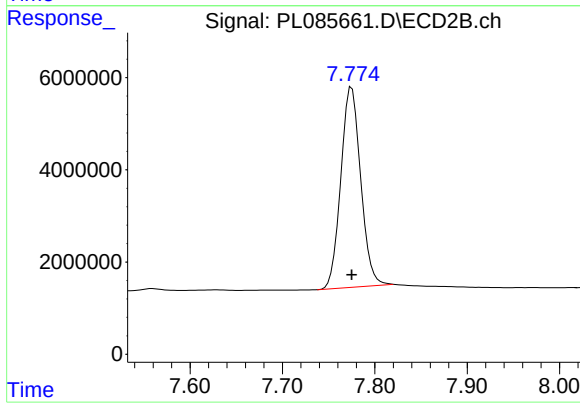

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 65052297
Conc: 73.30 ng/ml