

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100323\
 Data File : PL085662.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 16:32
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 03 17:36:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 03 17:36:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.623	144.6E6	57155874	50.000	50.000
28)	SA Decachlor...	8.858	7.775	108.0E6	45462514	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.516	3.613	60057546	16047897	500.000	500.000
24)	Chlordane-2	5.048	4.191	63826873	19389418	500.000	500.000
25)	Chlordane-3	5.760	4.819	254.1E6	50650126	500.000	500.000
26)	Chlordane-4	5.842	4.881	313.5E6	55706013	500.000	500.000
27)	Chlordane-5	6.689	5.551	49491769	14502102	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100323\
Data File : PL085662.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 16:32
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 03 17:36:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Tue Oct 03 17:36:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

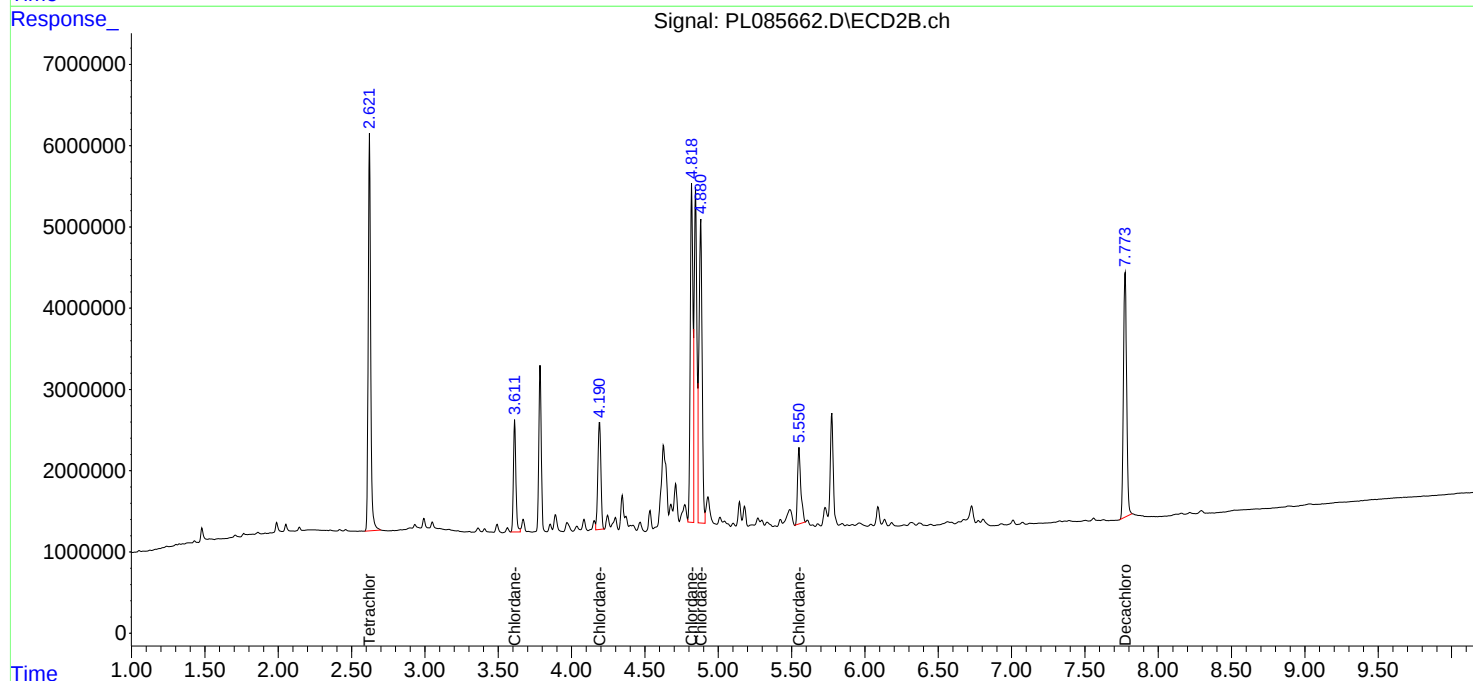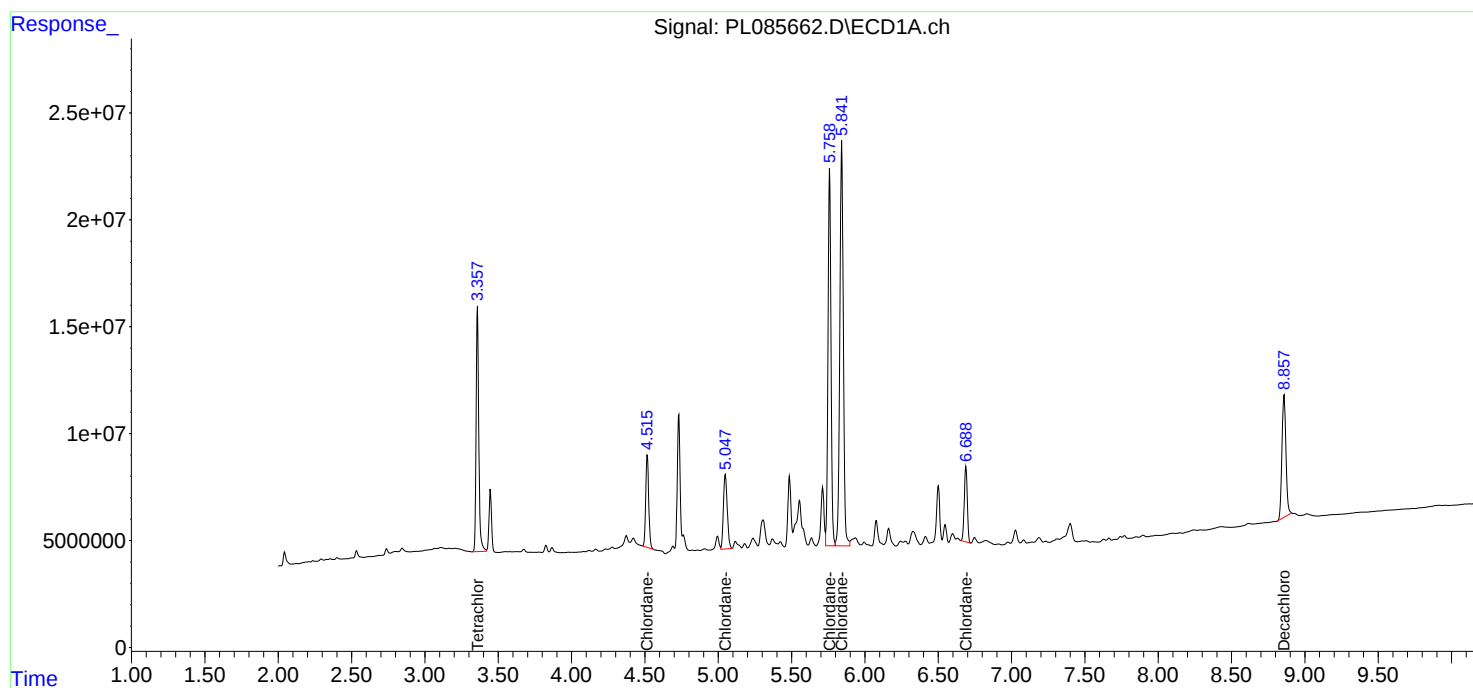


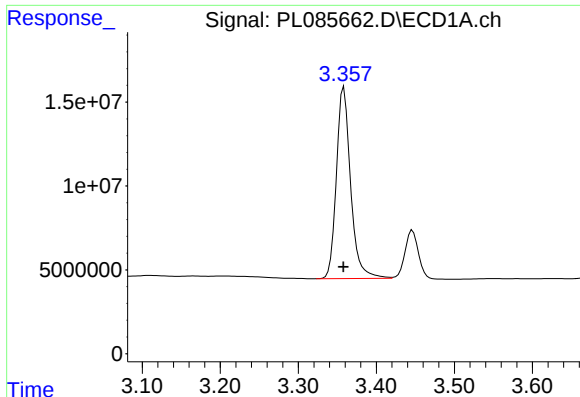

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: 0.000 min
Response: 144589876
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

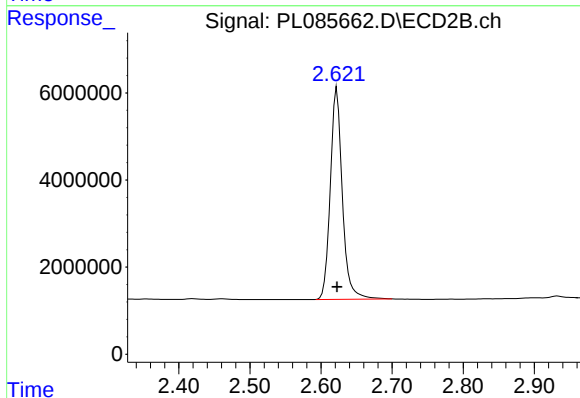


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 57155874
Conc: 50.00 ng/ml

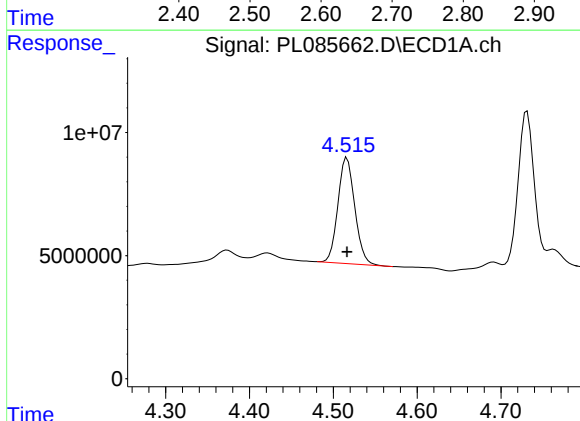


#23 Chlordane-1

R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 60057546
Conc: 500.00 ng/ml

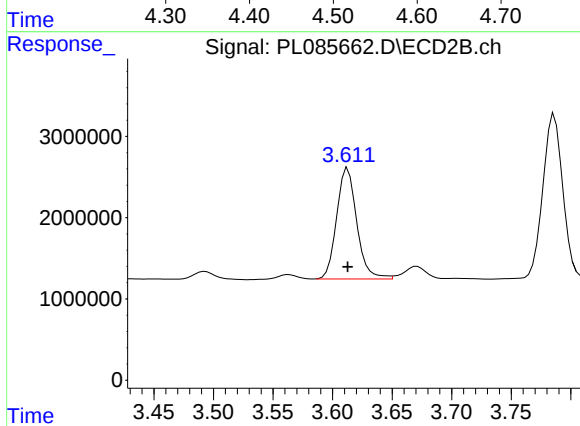

#23 Chlordane-1


R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 16047897
Conc: 500.00 ng/ml

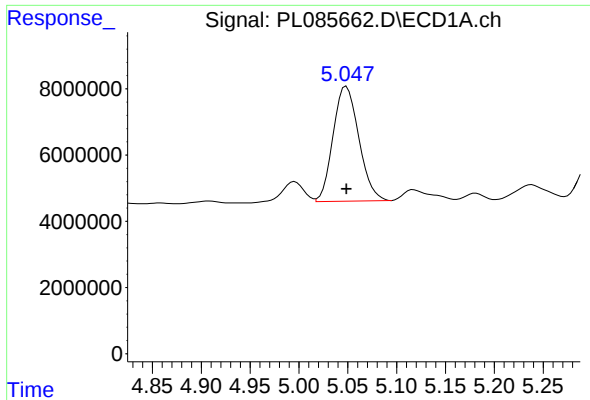

#24 Chlordane-2


R.T.: 5.048 min
Delta R.T.: 0.000 min
Response: 63826873
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

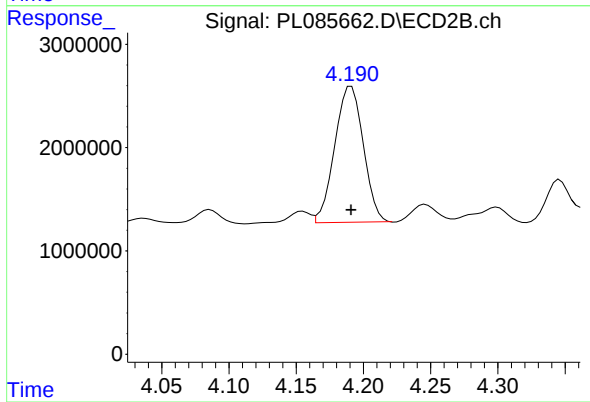


#24 Chlordane-2

R.T.: 4.191 min
Delta R.T.: 0.000 min
Response: 19389418
Conc: 500.00 ng/ml

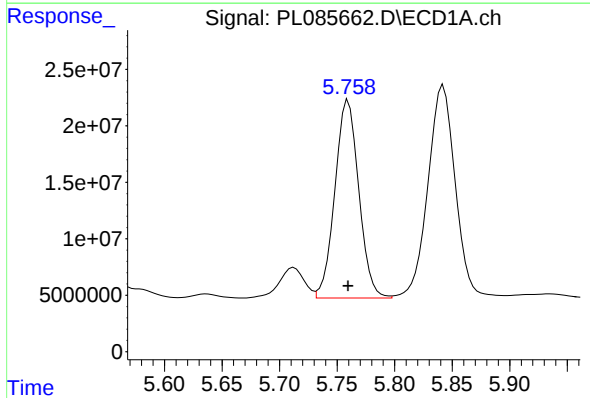


#25 Chlordane-3

R.T.: 5.760 min
Delta R.T.: 0.000 min
Response: 254101932
Conc: 500.00 ng/ml

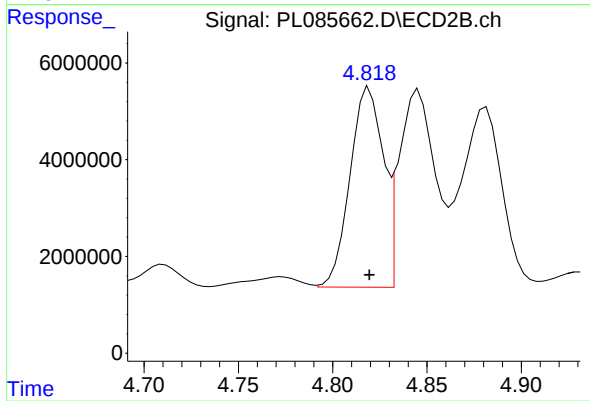

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 50650126
Conc: 500.00 ng/ml

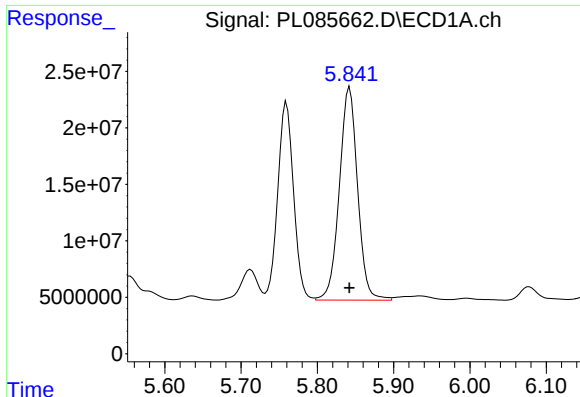

#26 Chlordane-4


R.T.: 5.842 min
Delta R.T.: 0.000 min
Response: 313491683
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

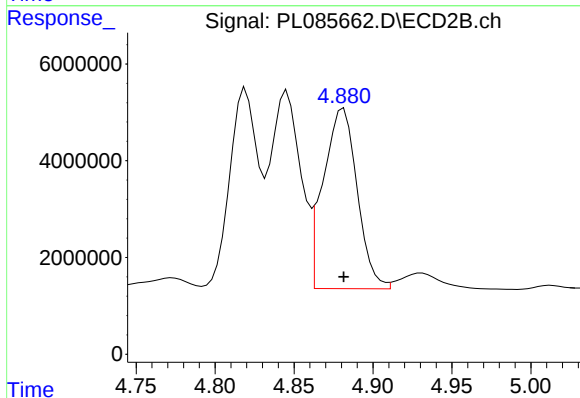


#26 Chlordane-4

R.T.: 4.881 min
Delta R.T.: 0.000 min
Response: 55706013
Conc: 500.00 ng/ml

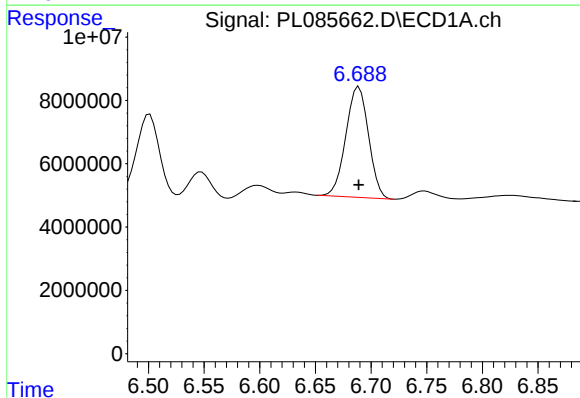


#27 Chlordane-5

R.T.: 6.689 min
Delta R.T.: 0.000 min
Response: 49491769
Conc: 500.00 ng/ml

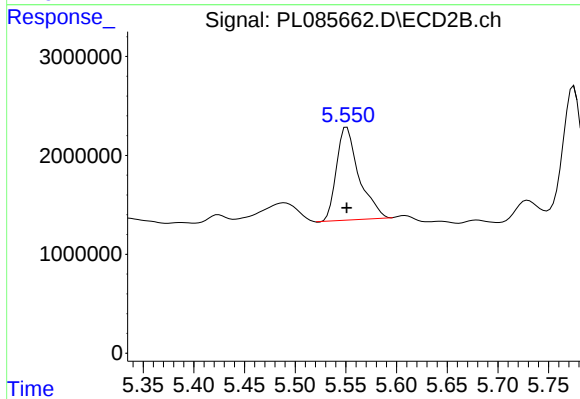

#27 Chlordane-5


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 14502102
Conc: 500.00 ng/ml

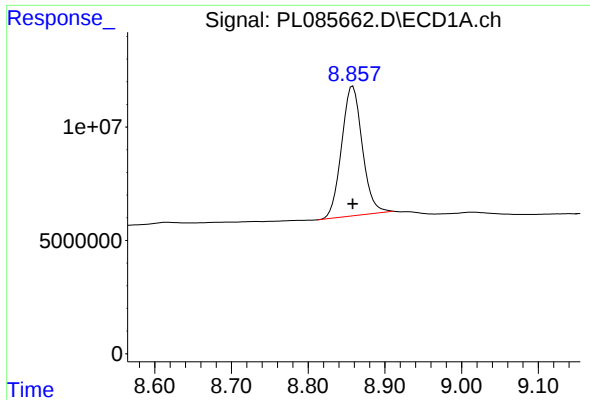

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 108012759
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

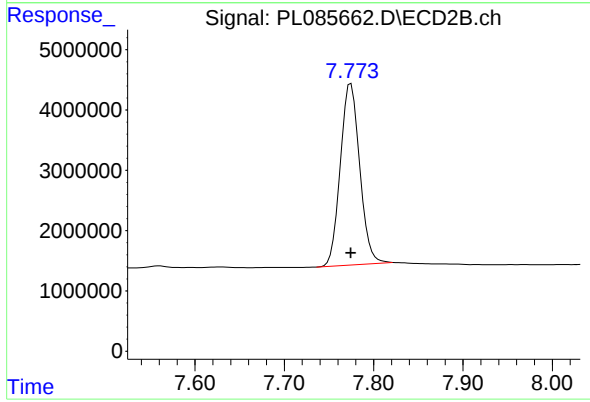

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 45462514
Conc: 50.00 ng/ml