

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100323\
 Data File : PL085671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2023 18:50
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL100323

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 05:27:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:26:18 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	2.622	143.0E6	57223851	48.929	49.926
28)	SA Decachlor...	8.857	7.775	108.0E6	44857010	48.424	48.031
Target Compounds							
23)	Chlordane-1	4.516	3.613	60653391	15795982	504.544	484.556
24)	Chlordane-2	5.048	4.191	63803110	19284429	490.627	495.568
25)	Chlordane-3	5.759	4.819	253.9E6	51557273	497.571	510.227
26)	Chlordane-4	5.842	4.882	313.6E6	56356549	494.367	486.738
27)	Chlordane-5	6.688	5.551	49706668	13540348	484.524	485.815



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100323\
Data File : PL085671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2023 18:50
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL100323

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 05:27:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:26:18 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

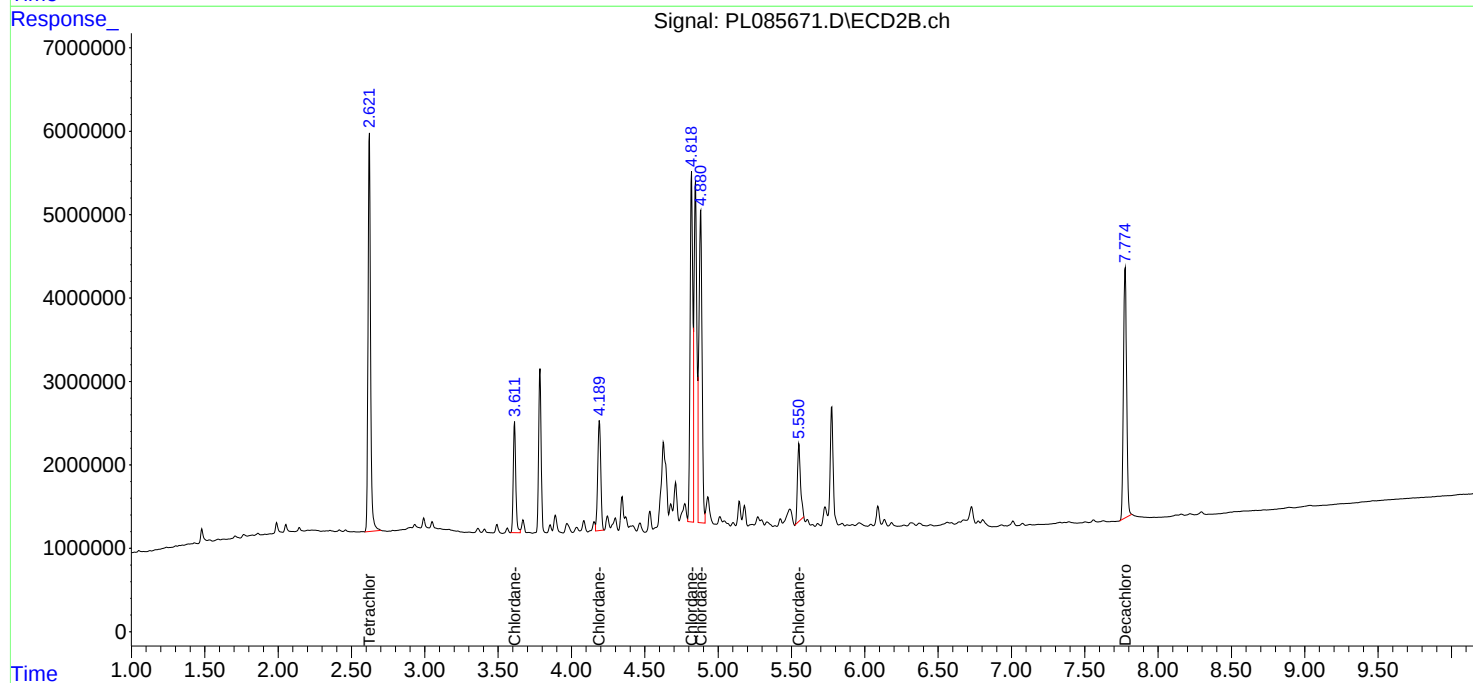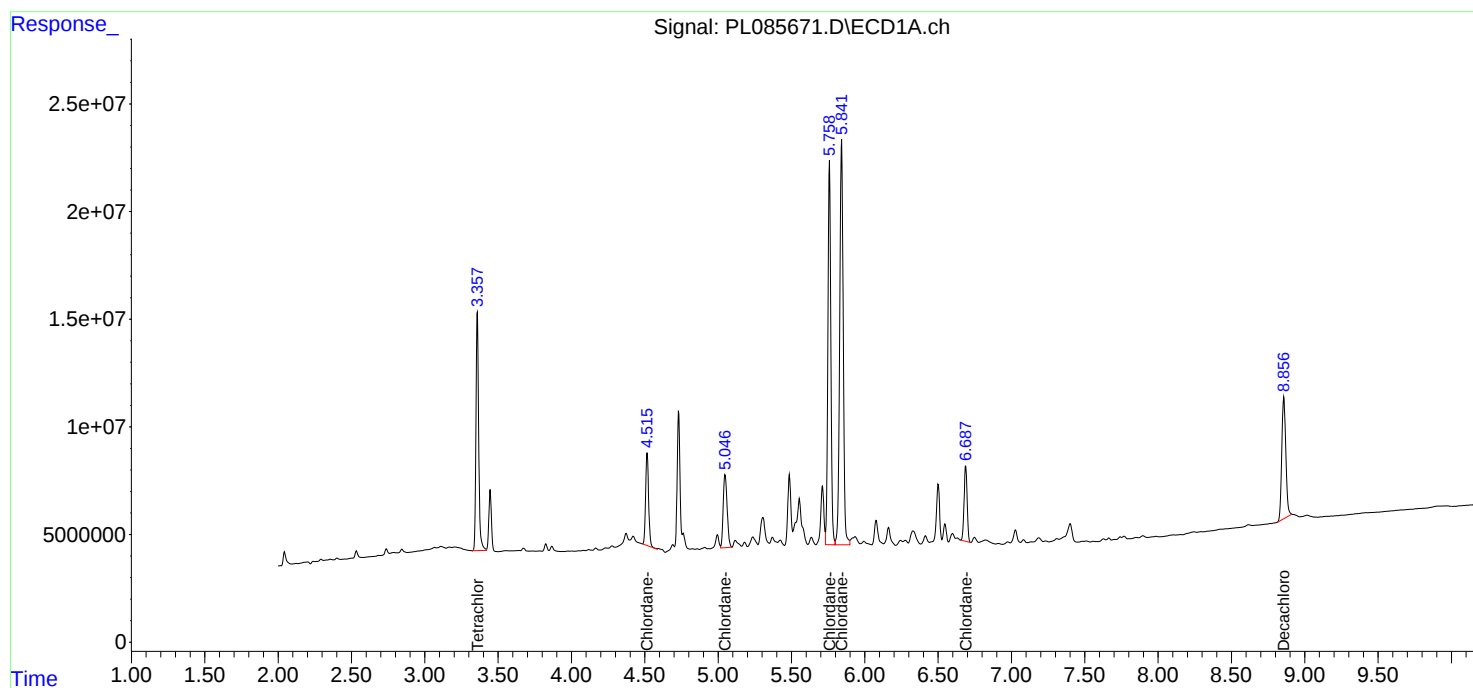


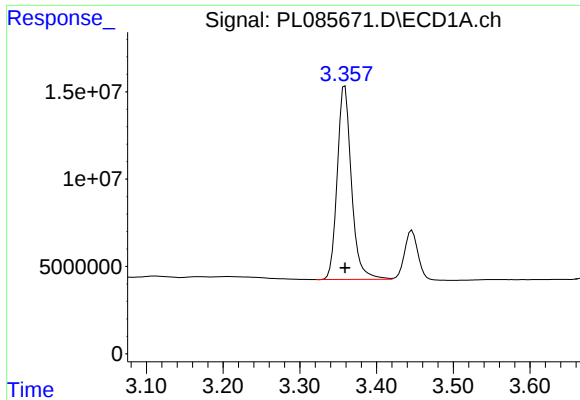

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: 0.000 min
Response: 143049401
Conc: 48.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100323

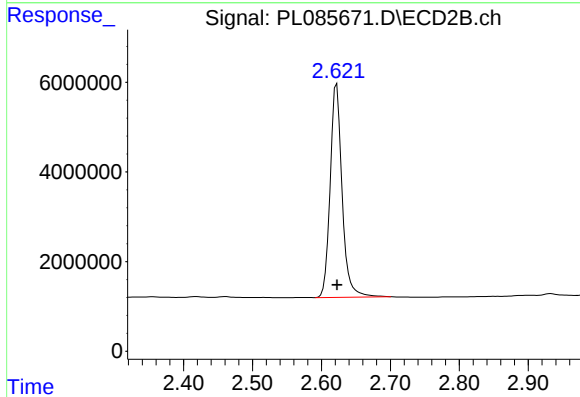


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 57223851
Conc: 49.93 ng/ml

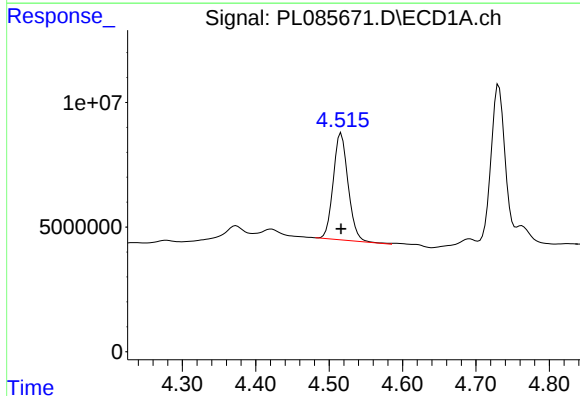


#23 Chlordane-1

R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 60653391
Conc: 504.54 ng/ml

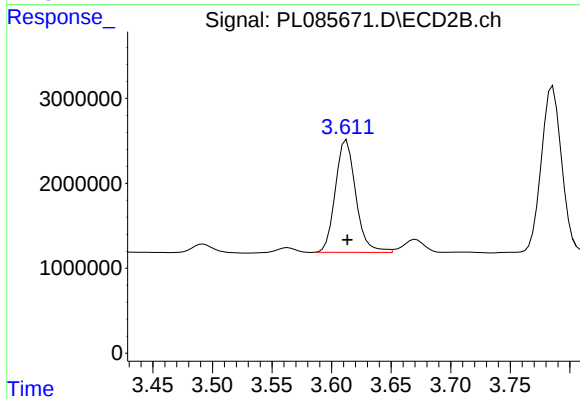

#23 Chlordane-1


R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 15795982
Conc: 484.56 ng/ml

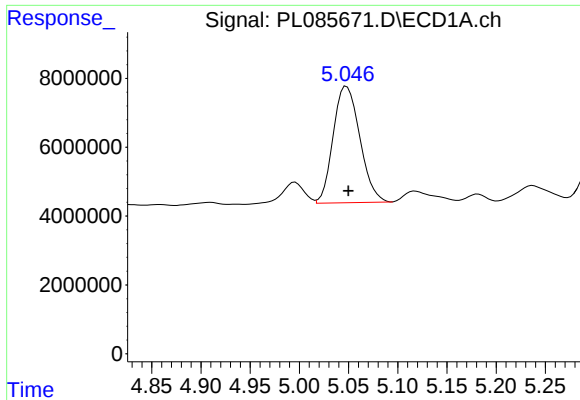

#24 Chlordane-2


R.T.: 5.048 min
Delta R.T.: -0.002 min
Response: 63803110
Conc: 490.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100323

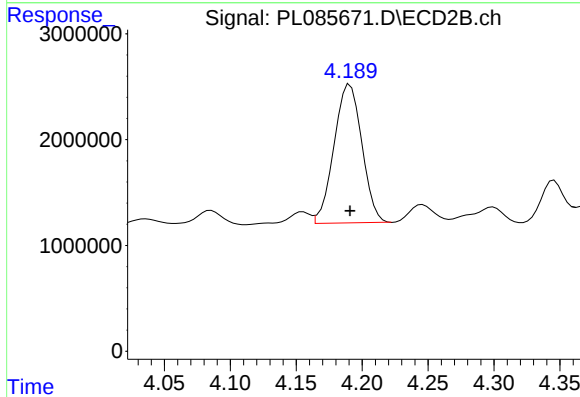


#24 Chlordane-2

R.T.: 4.191 min
Delta R.T.: 0.000 min
Response: 19284429
Conc: 495.57 ng/ml

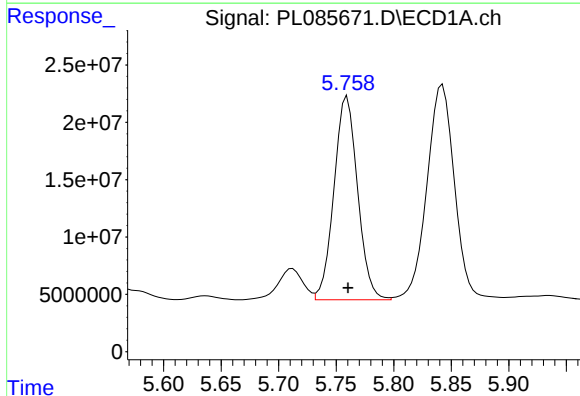


#25 Chlordane-3

R.T.: 5.759 min
Delta R.T.: -0.001 min
Response: 253861323
Conc: 497.57 ng/ml

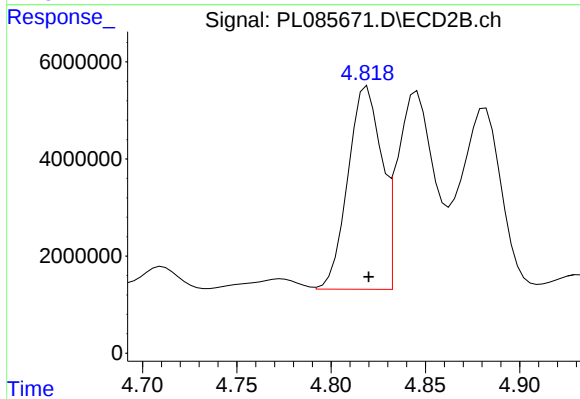

#25 Chlordane-3


R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 51557273
Conc: 510.23 ng/ml

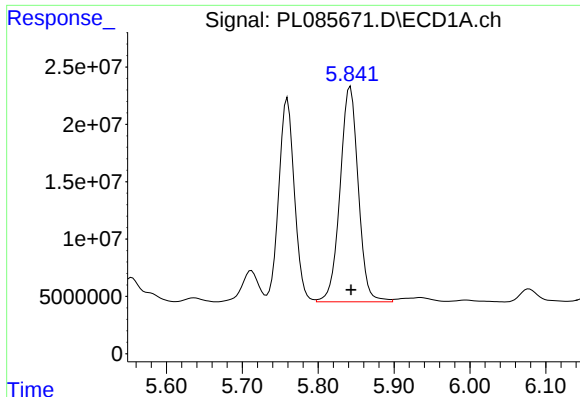

#26 Chlordane-4


R.T.: 5.842 min
Delta R.T.: 0.000 min
Response: 313646898
Conc: 494.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100323

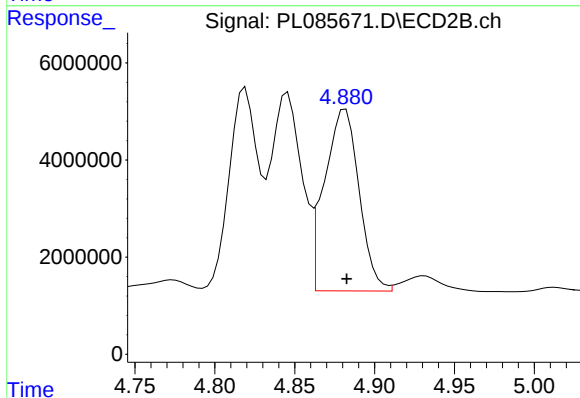


#26 Chlordane-4

R.T.: 4.882 min
Delta R.T.: 0.000 min
Response: 56356549
Conc: 486.74 ng/ml

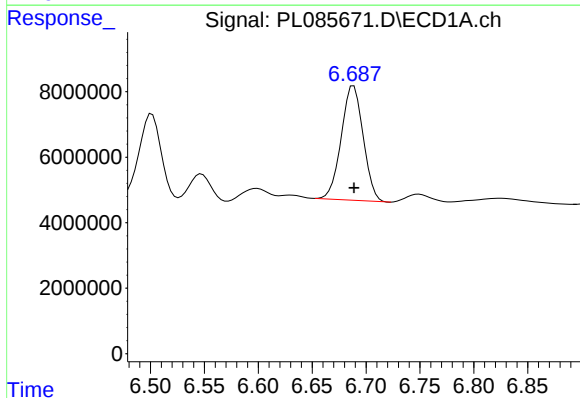


#27 Chlordane-5

R.T.: 6.688 min
Delta R.T.: 0.000 min
Response: 49706668
Conc: 484.52 ng/ml

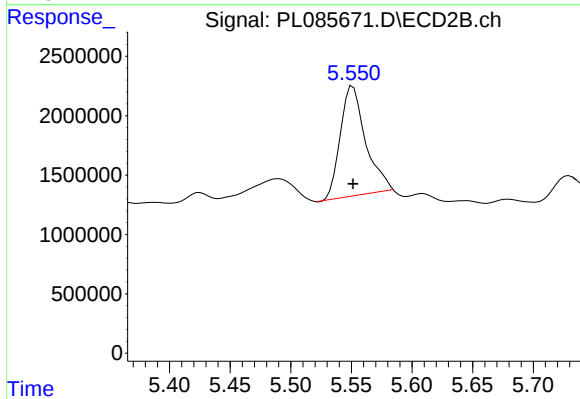

#27 Chlordane-5


R.T.: 5.551 min
Delta R.T.: 0.000 min
Response: 13540348
Conc: 485.82 ng/ml

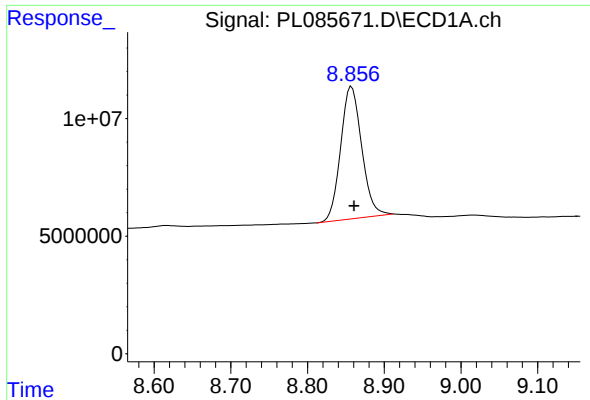

#28 Decachlorobiphenyl

R.T.: 8.857 min
Delta R.T.: -0.003 min
Response: 107988280
Conc: 48.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL100323

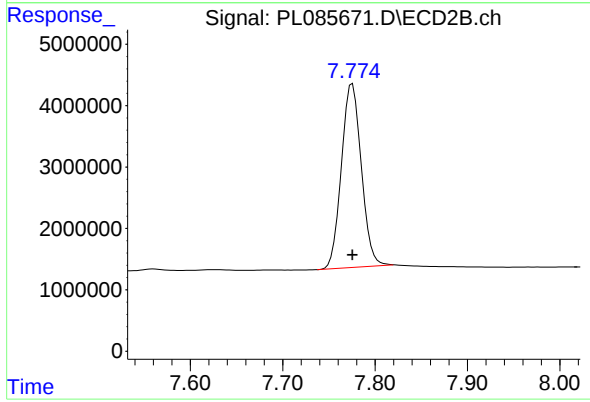

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 44857010
Conc: 48.03 ng/ml