

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100325\
 Data File : PL097507.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2025 02:38
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 01:20:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.642	0.000	65331879	0	11.368	N.D. #
9) A	Endosulfan I	6.062f	0.000	28965663	0	5.590	N.D. #
13) MA	Dieldrin	0.000	5.422	0	38081548	N.D.	4.657 #
14) MA	Endrin	0.000	5.709	0	167.9E6	N.D.	22.357 #
15) B	Endosulfa...	6.739	5.996	1444225	8027261	0.294	1.129 #
18) B	Endrin al...	6.879	0.000	9231058	0	2.994	N.D. #
27)	Chlordane-5	6.802f	5.996	14356947	8027261	85.645	26.924 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100325\
Data File : PL097507.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2025 02:38
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 01:20:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

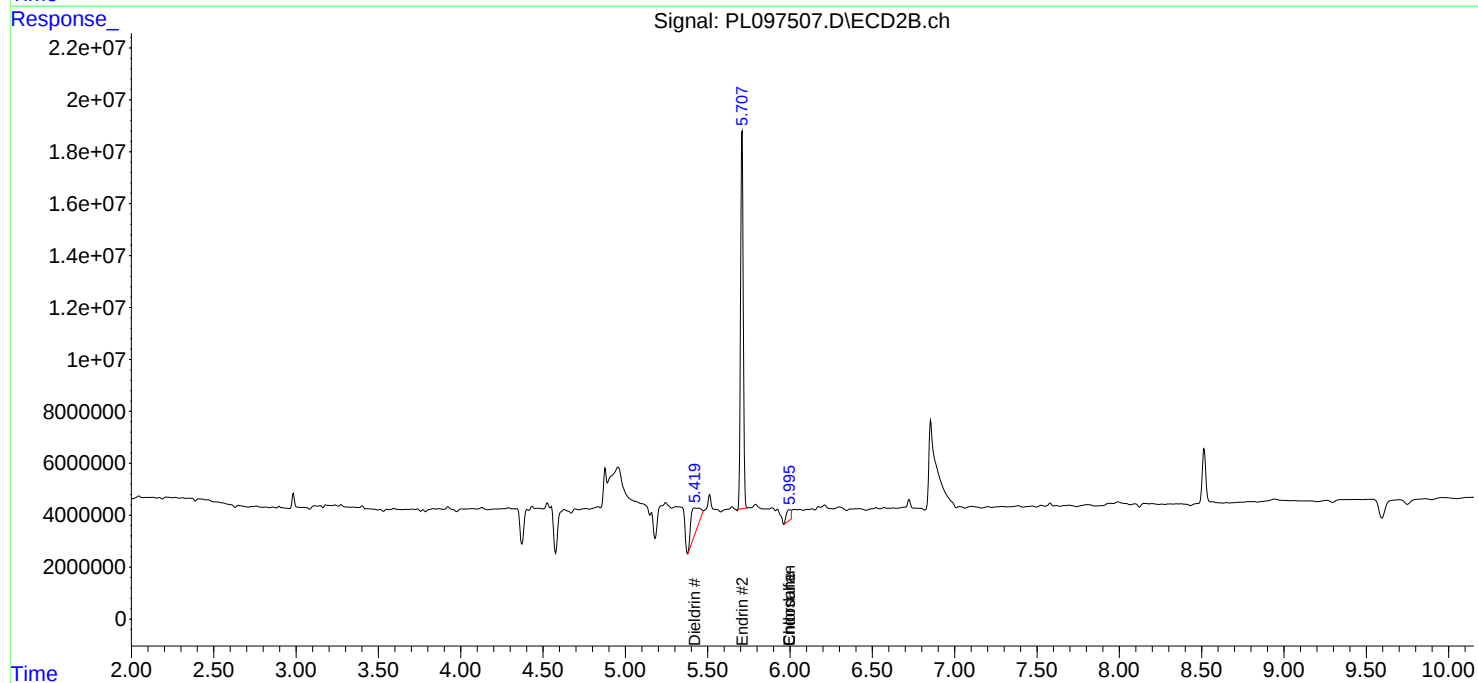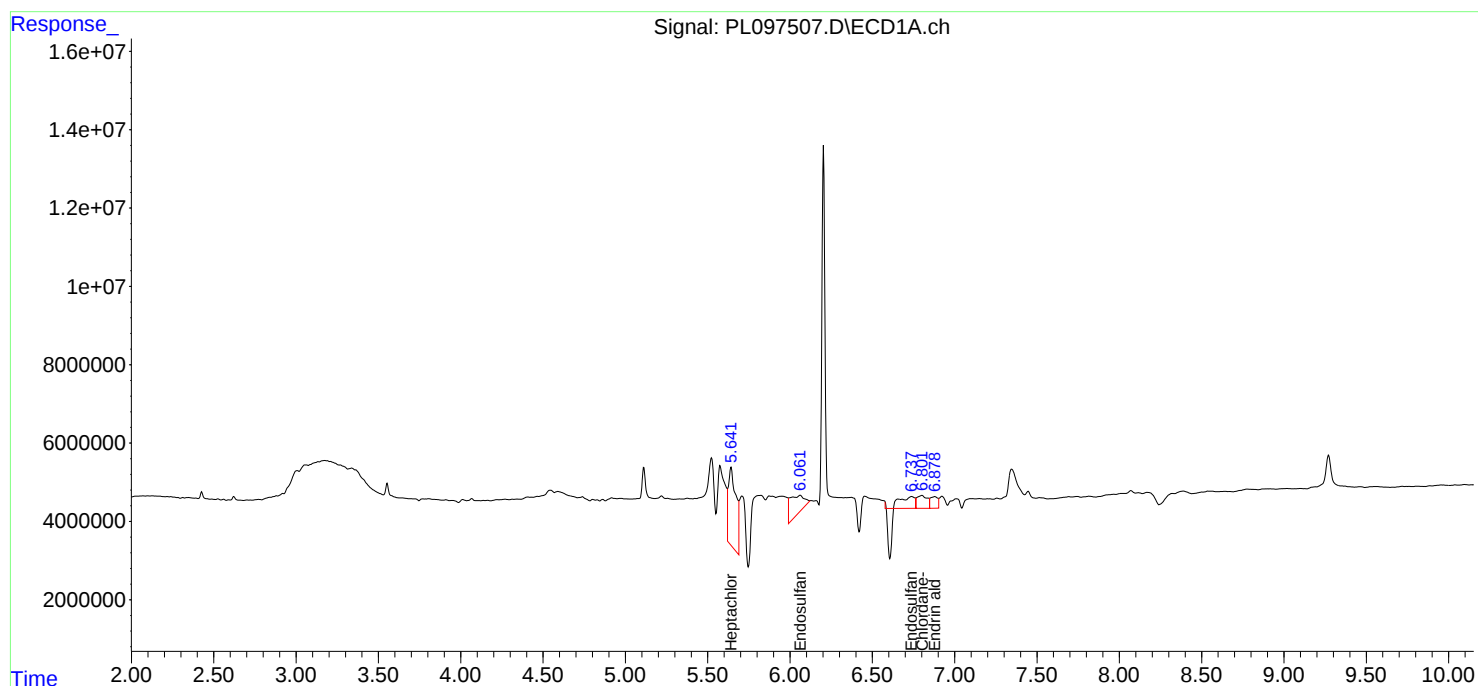


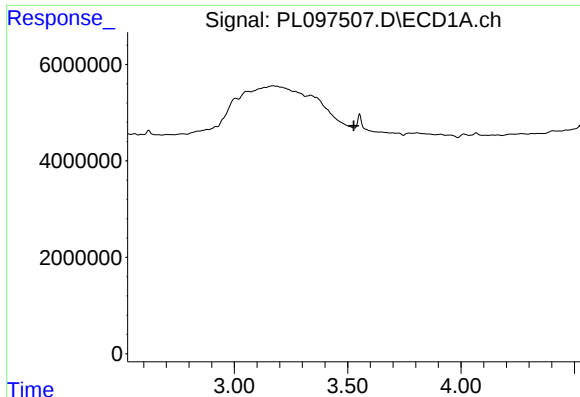

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.527 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

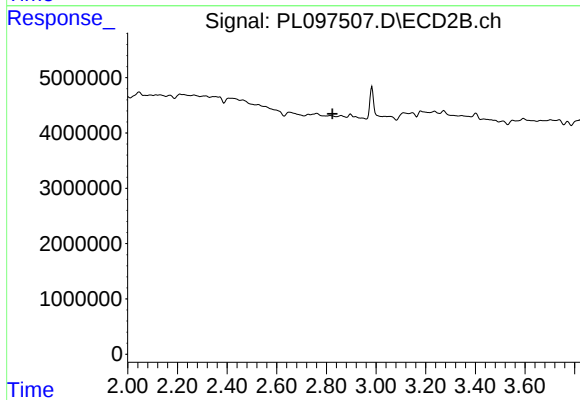


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.823 min
Response: 0
Conc: N.D.

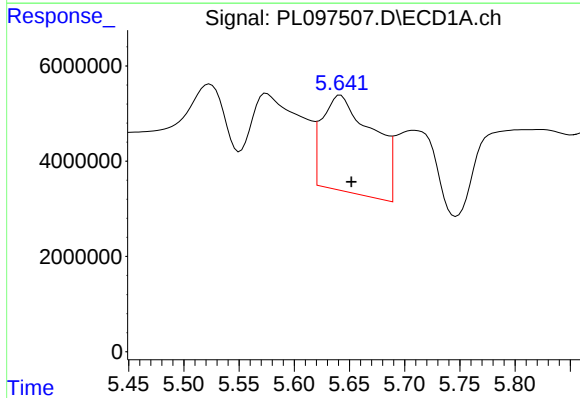


#8 Heptachlor epoxide

R.T.: 5.642 min
Delta R.T.: -0.010 min
Response: 65331879
Conc: 11.37 ng/ml

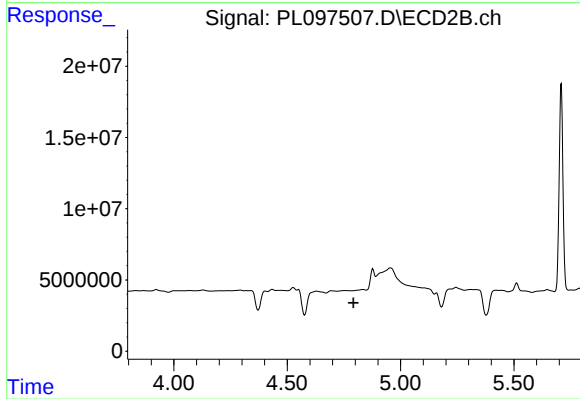

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.793 min
Response: 0
Conc: N.D.

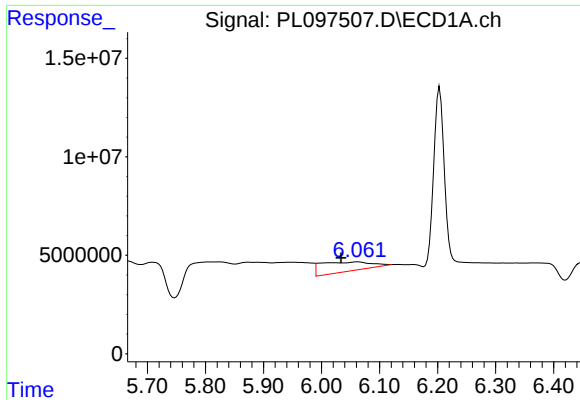

#9 Endosulfan I


R.T.: 6.062 min
Delta R.T.: 0.029 min
Response: 28965663
Conc: 5.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

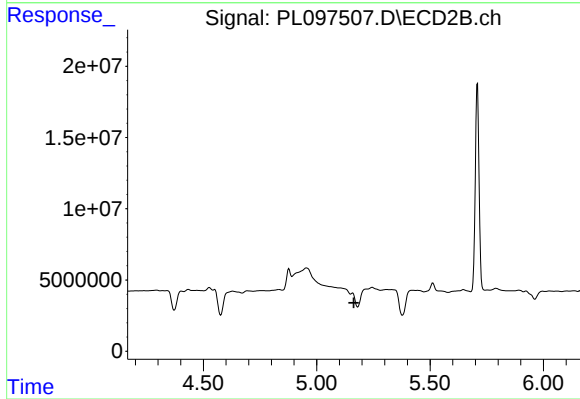


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.163 min
Response: 0
Conc: N.D.

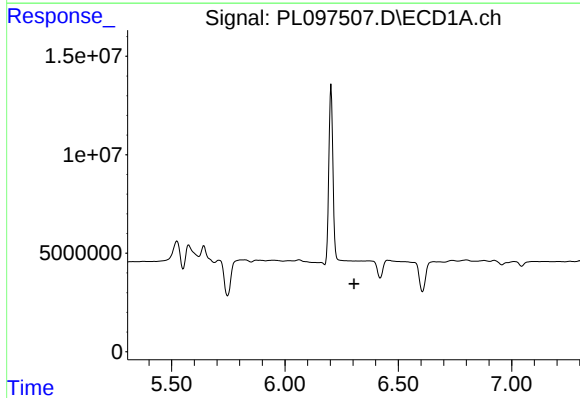


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

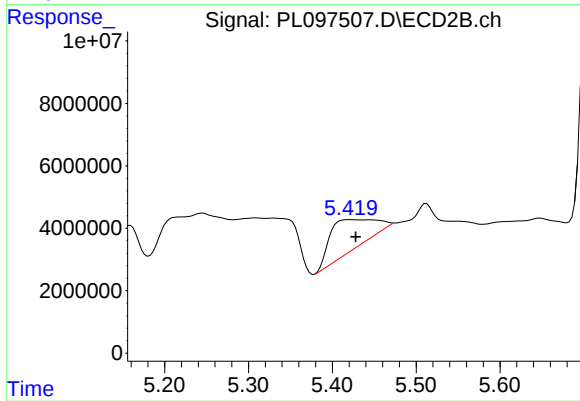

#13 Dieldrin


R.T.: 5.422 min
Delta R.T.: -0.006 min
Response: 38081548
Conc: 4.66 ng/ml

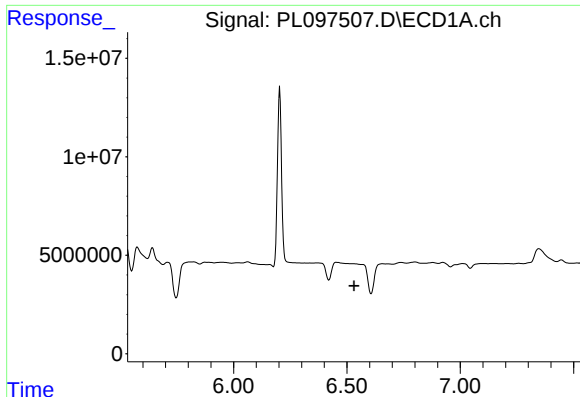

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

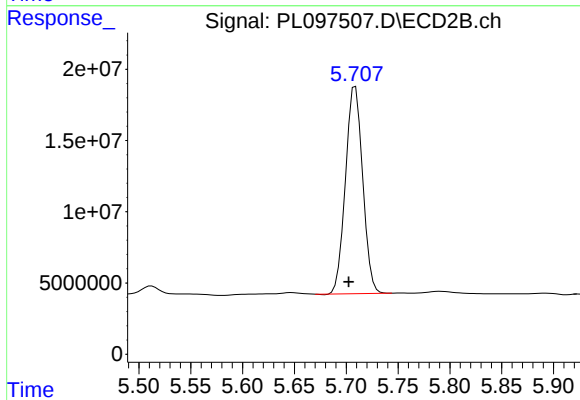


#14 Endrin

R.T.: 5.709 min
Delta R.T.: 0.006 min
Response: 167913484
Conc: 22.36 ng/ml

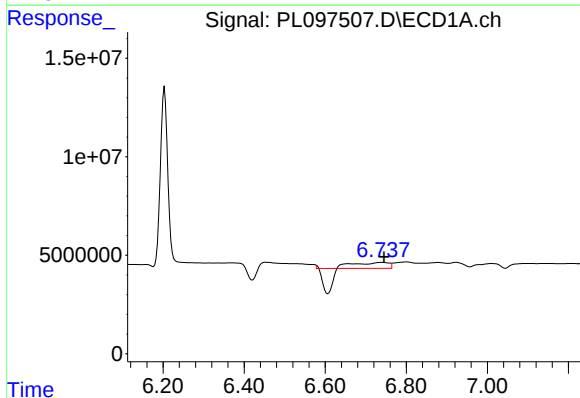


#15 Endosulfan II

R.T.: 6.739 min
Delta R.T.: -0.007 min
Response: 1444225
Conc: 0.29 ng/ml

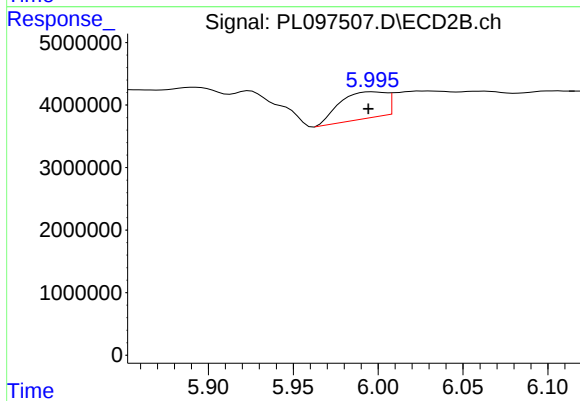

#15 Endosulfan II


R.T.: 5.996 min
Delta R.T.: 0.002 min
Response: 8027261
Conc: 1.13 ng/ml

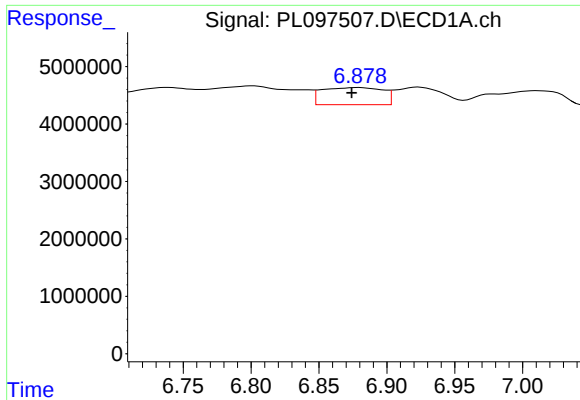

#18 Endrin aldehyde


R.T.: 6.879 min
Delta R.T.: 0.005 min
Response: 9231058
Conc: 2.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

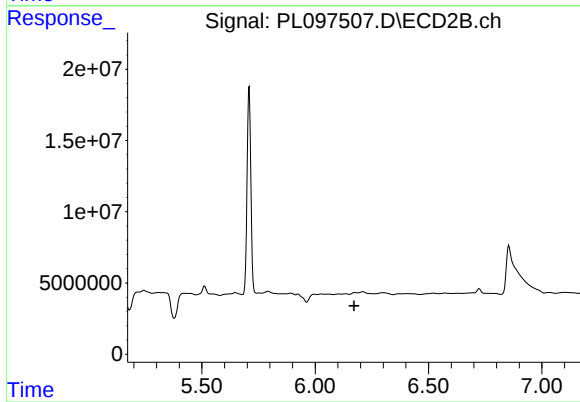


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.172 min
Response: 0
Conc: N.D.

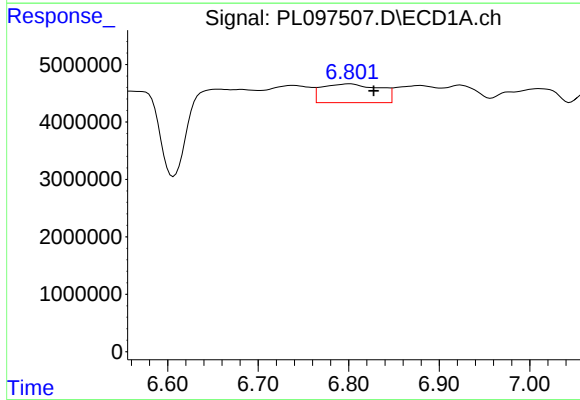


#27 Chlordane-5

R.T.: 6.802 min
Delta R.T.: -0.026 min
Response: 14356947
Conc: 85.64 ng/ml

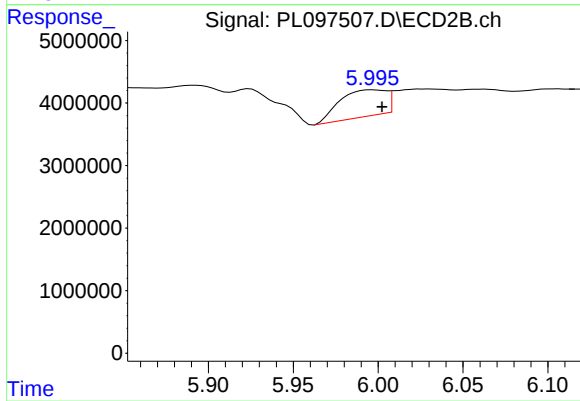

#27 Chlordane-5


R.T.: 5.996 min
Delta R.T.: -0.006 min
Response: 8027261
Conc: 26.92 ng/ml

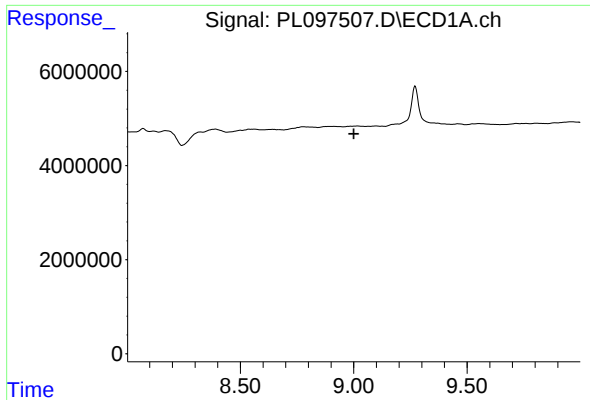

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.001 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

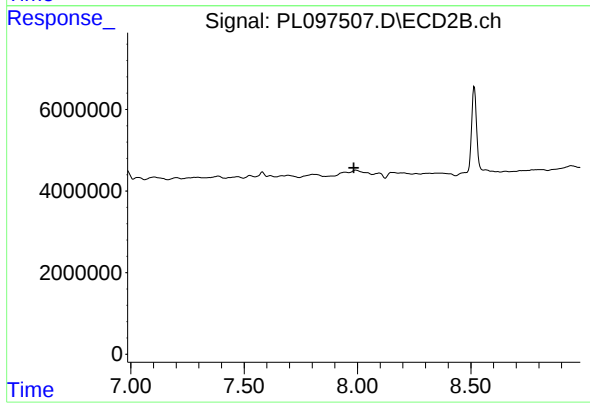

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.984 min
Response: 0
Conc: N.D.