

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100325\
 Data File : PL097514.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2025 04:27
 Operator : AR\AJ
 Sample : Q3269-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EG1-TP2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 01:21:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.526	2.824	87617595	90226798	19.354	13.722 #
28)	SA Decachlor...	8.995	7.981	38379857	66877913	11.729	11.750
Target Compounds							
9)	A Endosulfan I	0.000	5.182f	0	7314024	N.D.	0.952 #
10)	B gamma-Chl...	0.000	5.041	0	13793976	N.D.	1.579 #
20)	A Methoxychlor	0.000	6.697f	0	4427961	N.D.	1.175 #
25)	Chlordane-3	0.000	5.041	0	13793976	N.D.	15.426 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100325\
Data File : PL097514.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2025 04:27
Operator : AR\AJ
Sample : Q3269-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EG1-TP2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 01:21:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

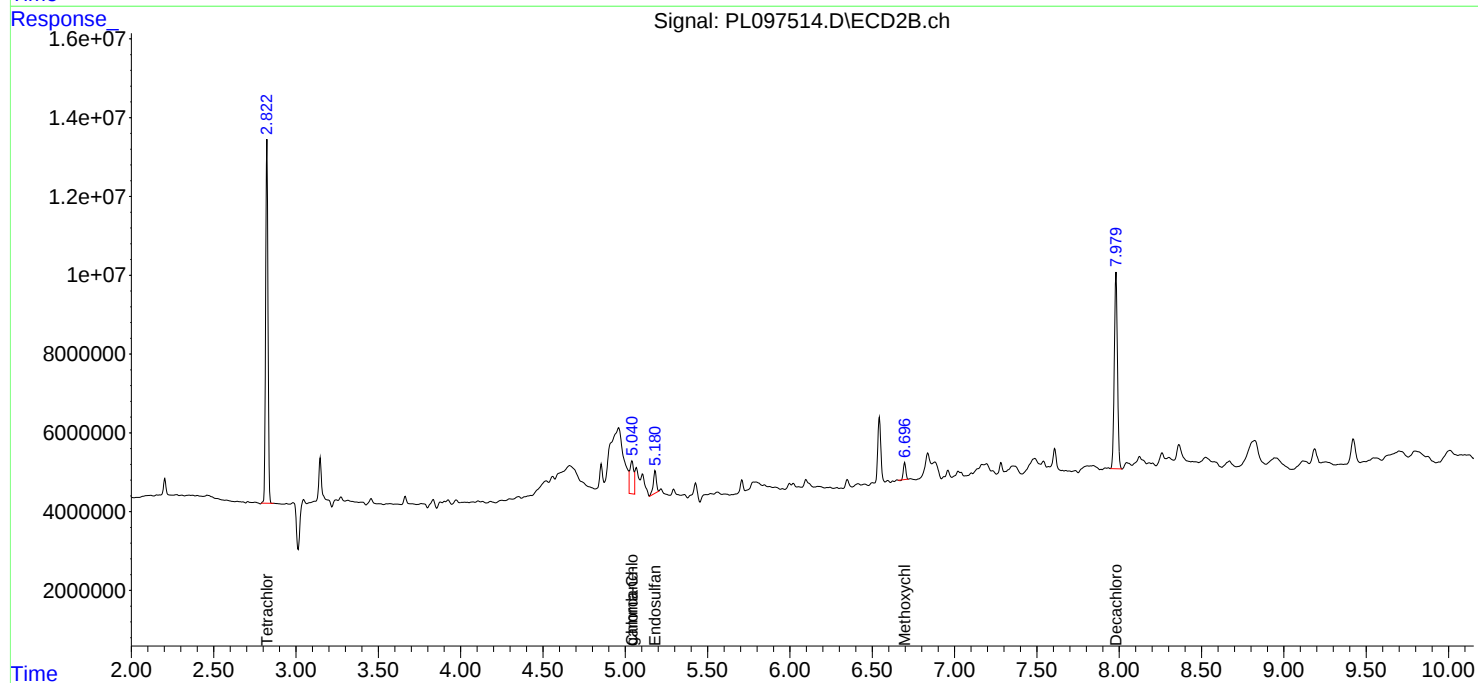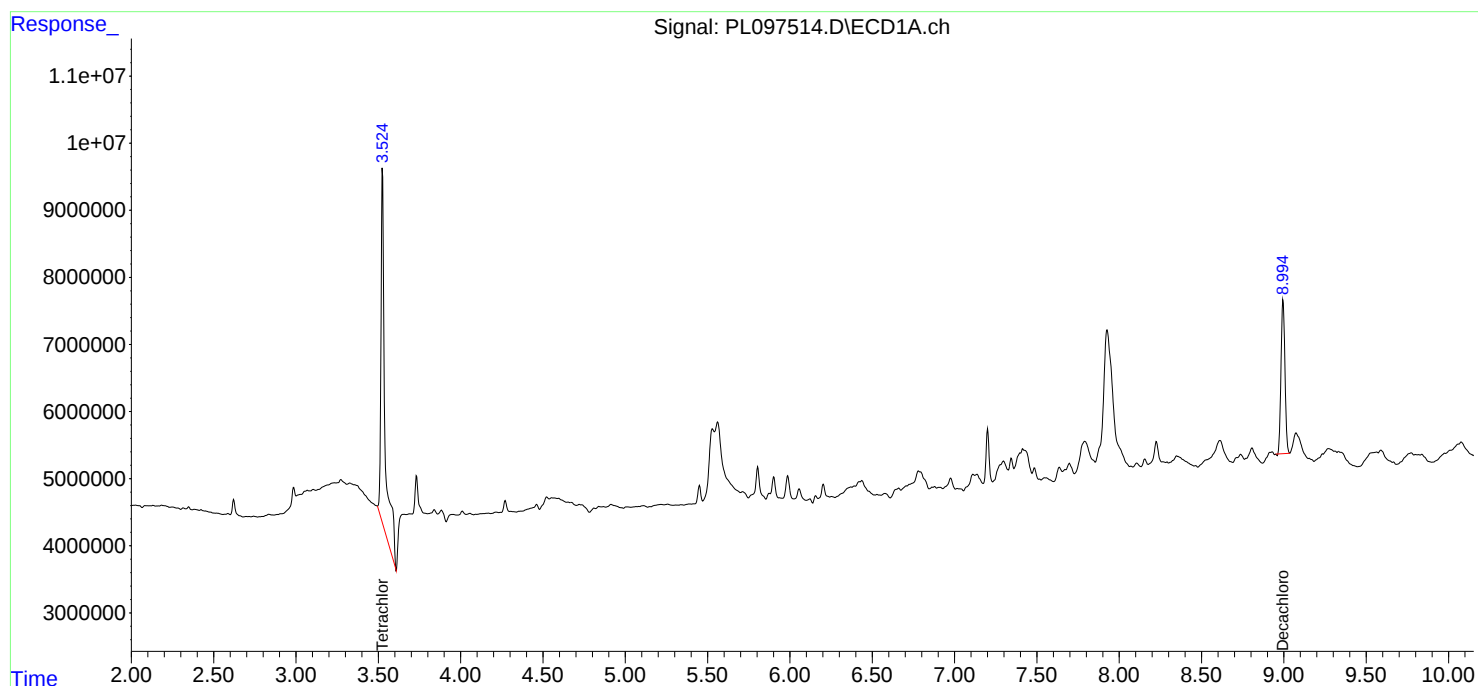


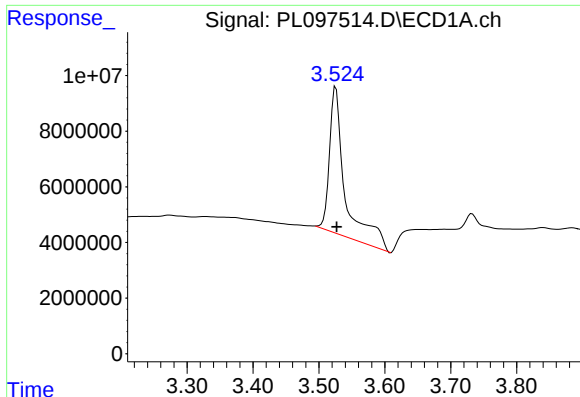

#1 Tetrachloro-m-xylene


R.T.: 3.526 min
Delta R.T.: -0.001 min
Response: 87617595
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
EG1-TP2

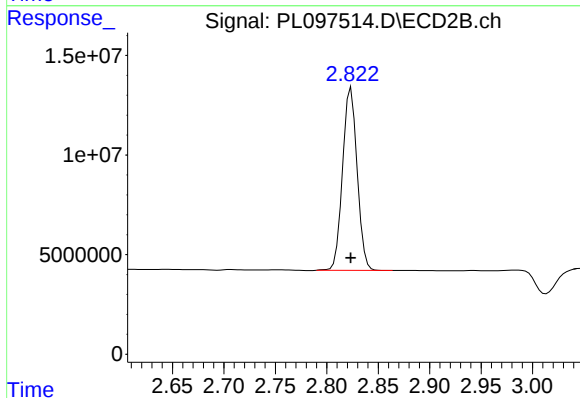


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 90226798
Conc: 13.72 ng/ml

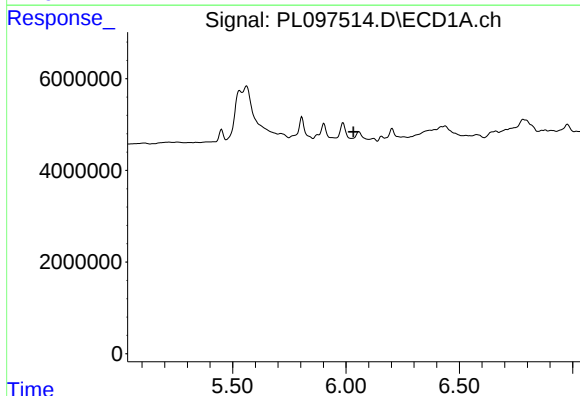


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

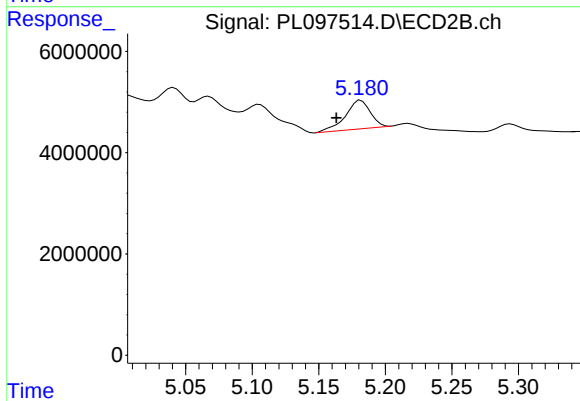

#9 Endosulfan I


R.T.: 5.182 min
Delta R.T.: 0.019 min
Response: 7314024
Conc: 0.95 ng/ml

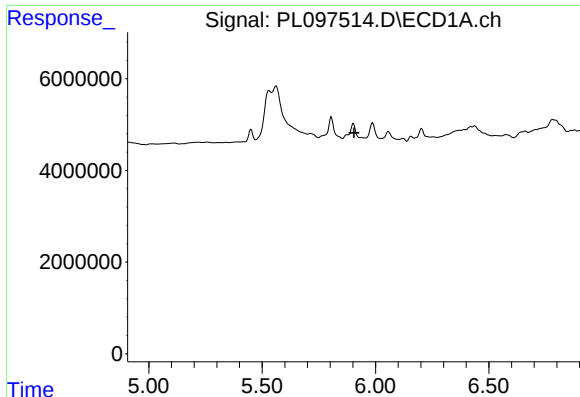

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EG1-TP2

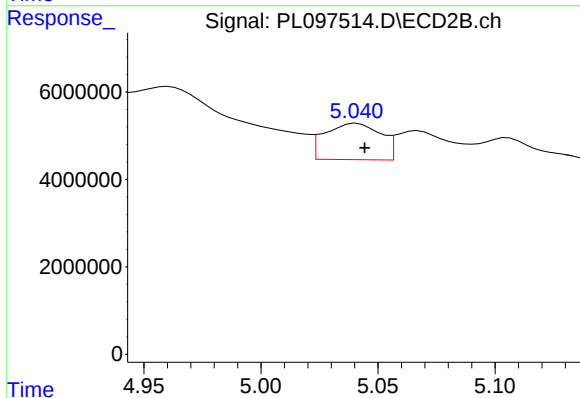


#10 gamma-Chlordane

R.T.: 5.041 min
Delta R.T.: -0.003 min
Response: 13793976
Conc: 1.58 ng/ml

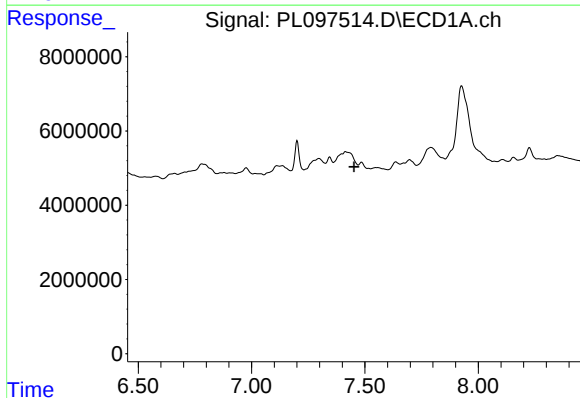


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.452 min
Response: 0
Conc: N.D.

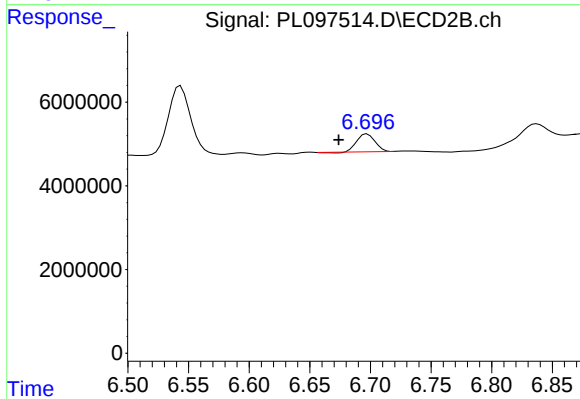

#20 Methoxychlor


R.T.: 6.697 min
Delta R.T.: 0.023 min
Response: 4427961
Conc: 1.17 ng/ml

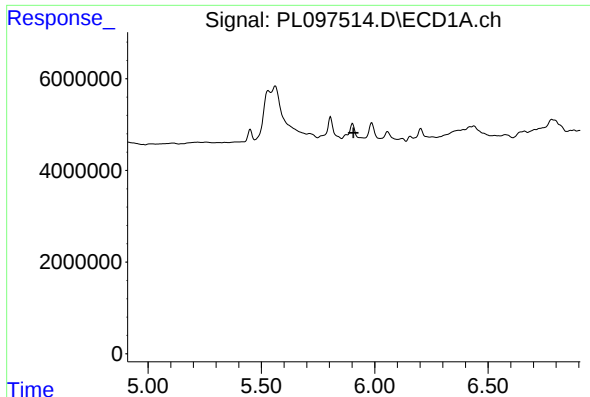

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.907 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EG1-TP2

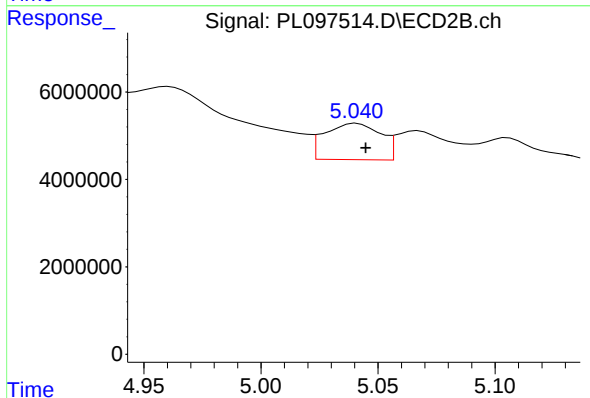


#25 Chlordane-3

R.T.: 5.041 min
Delta R.T.: -0.004 min
Response: 13793976
Conc: 15.43 ng/ml

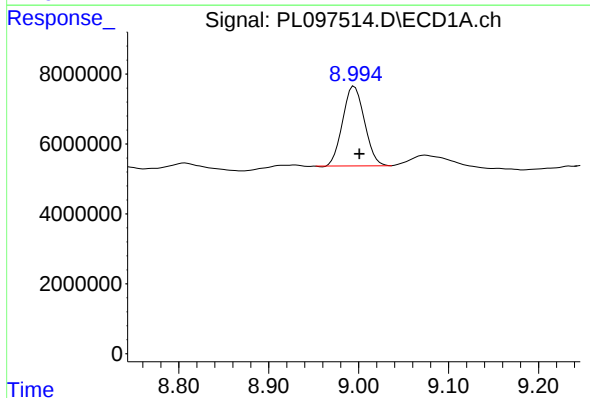

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.006 min
Response: 38379857
Conc: 11.73 ng/ml

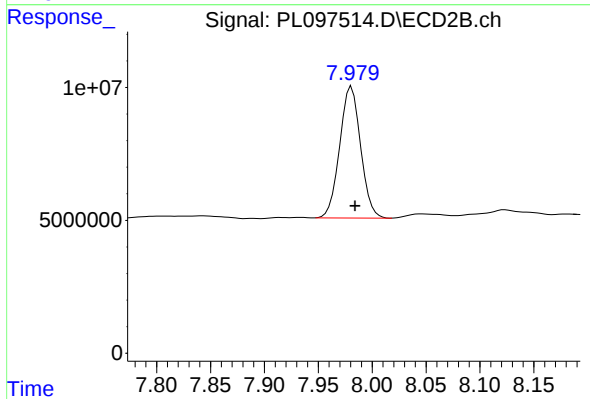

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.003 min
Response: 66877913
Conc: 11.75 ng/ml