

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100325\
 Data File : PL097520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2025 07:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 01:22:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.824	105.7E6	147.8E6	23.349	22.479
28)	SA Decachlor...	8.997	7.981	86389298	129.5E6	26.401	22.749
Target Compounds							
13)	MA Dieldrin	0.000	5.424	0 20758213	N.D.	2.539	#
14)	MA Endrin	0.000	5.709	0 57395530	N.D.	7.642	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100325\
Data File : PL097520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2025 07:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 01:22:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

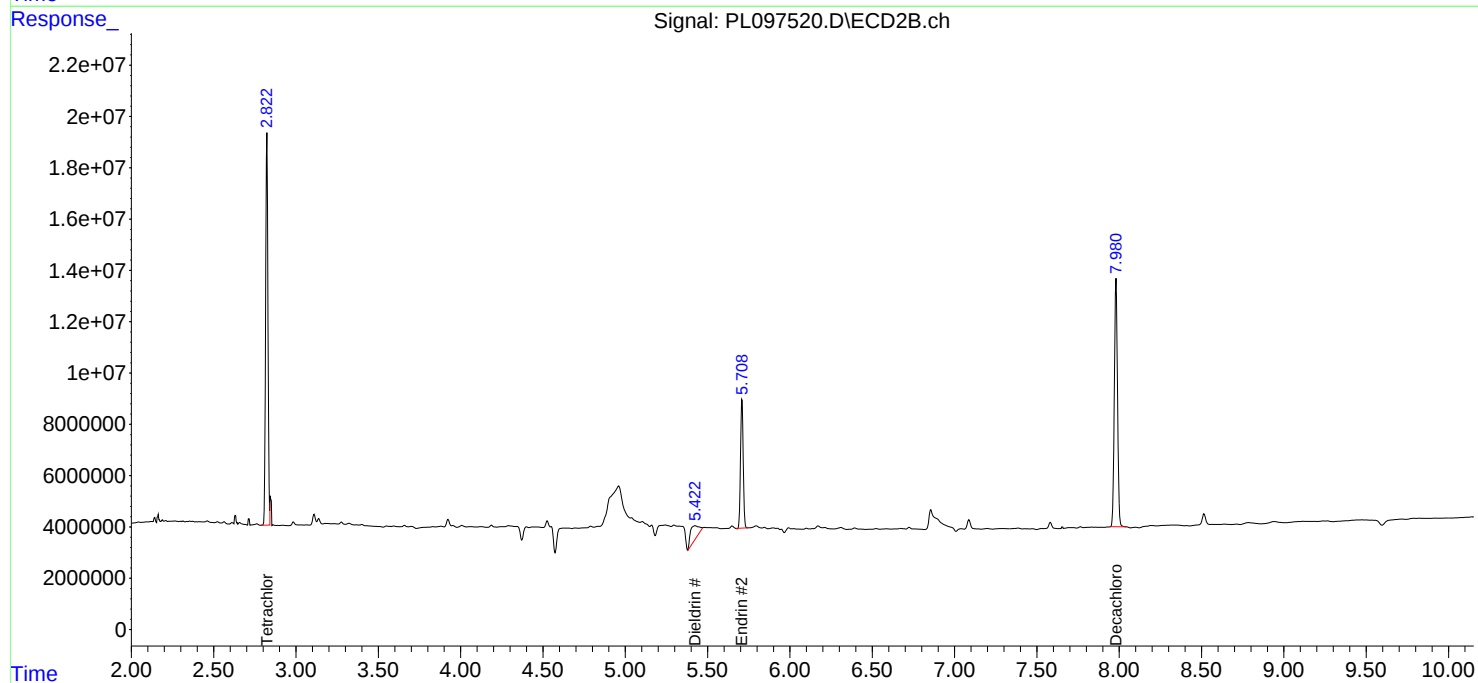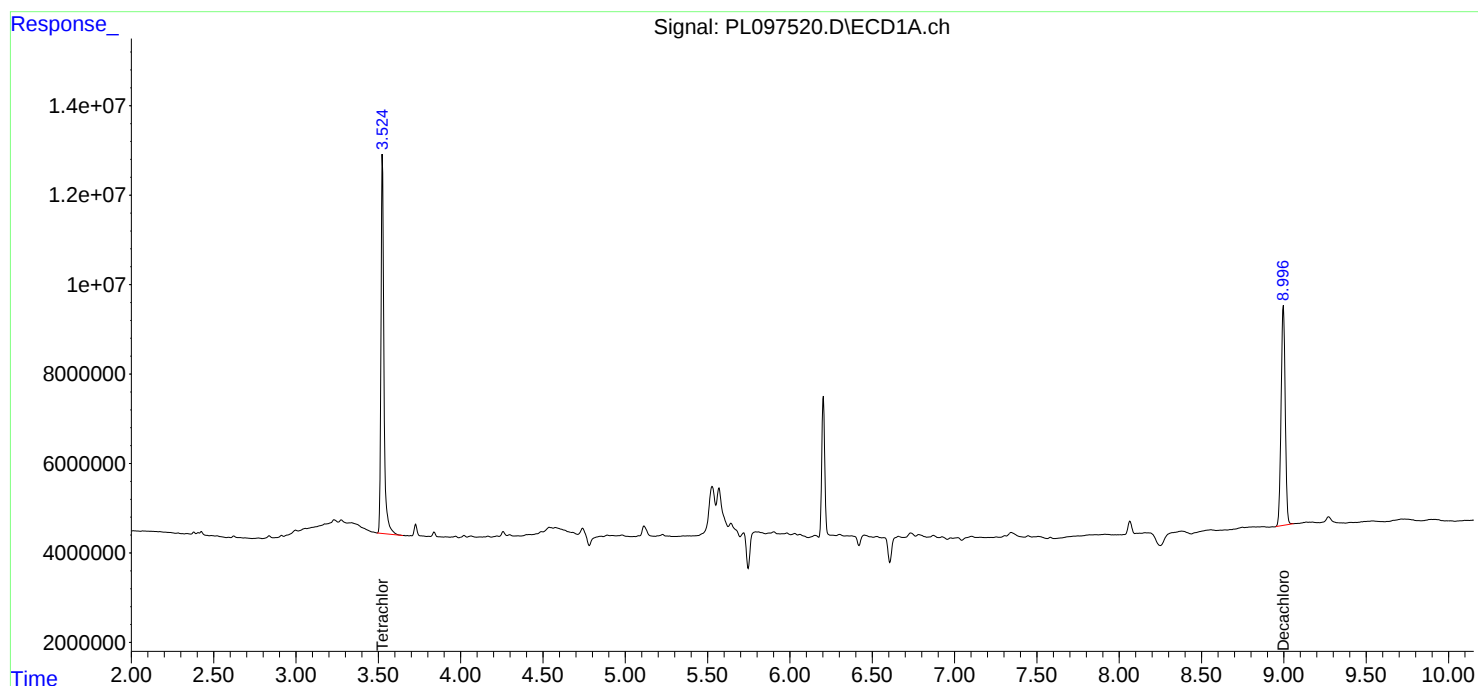


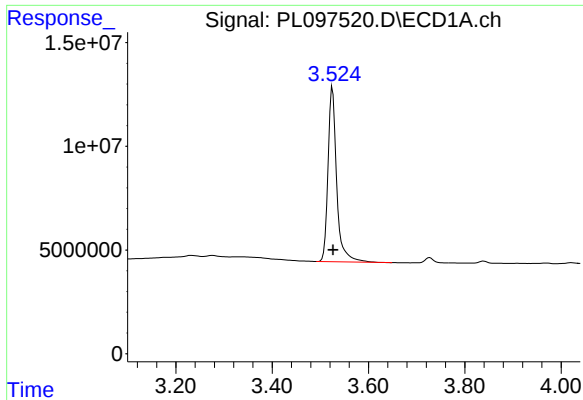

#1 Tetrachloro-m-xylene


R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 105704029
Conc: 23.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

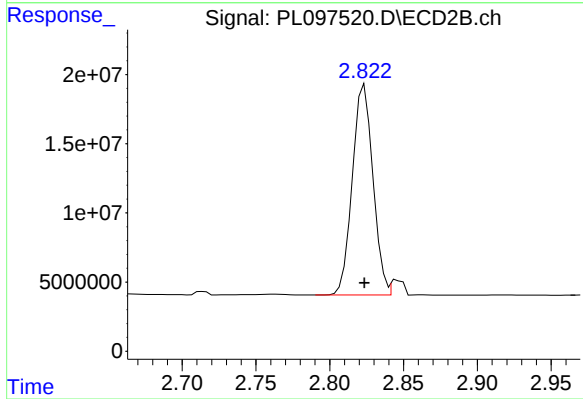


#1 Tetrachloro-m-xylene

R.T.: 2.824 min
Delta R.T.: 0.000 min
Response: 147810564
Conc: 22.48 ng/ml

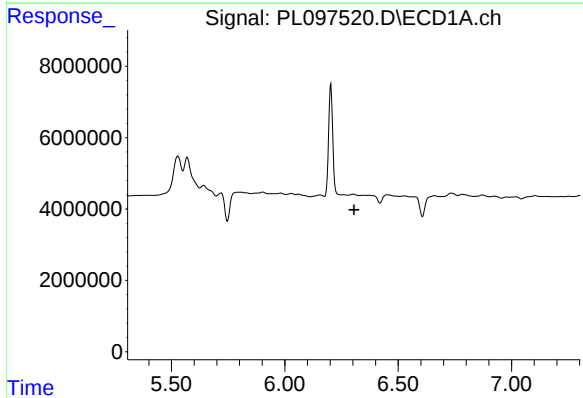


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.306 min
Response: 0
Conc: N.D.

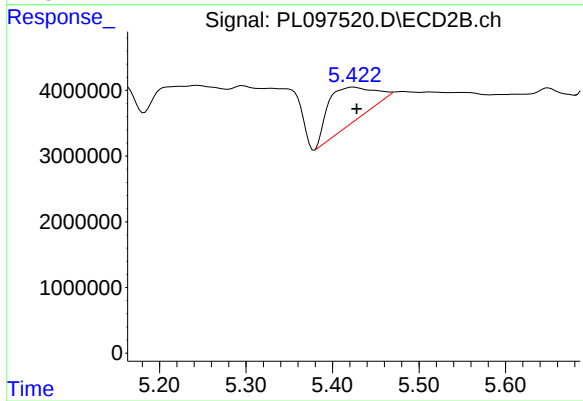

#13 Dieldrin


R.T.: 5.424 min
Delta R.T.: -0.004 min
Response: 20758213
Conc: 2.54 ng/ml

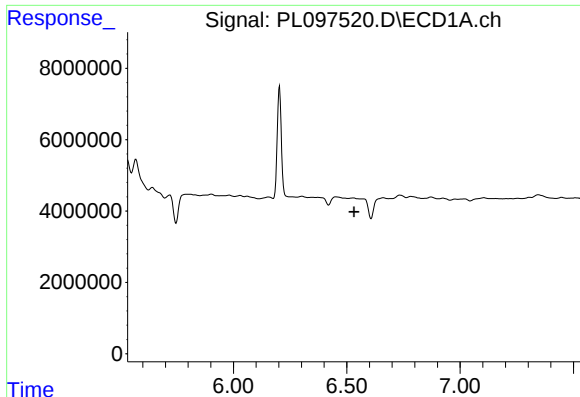

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

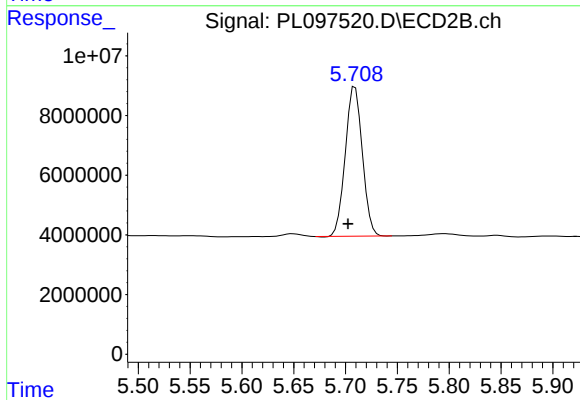


#14 Endrin

R.T.: 5.709 min
Delta R.T.: 0.007 min
Response: 57395530
Conc: 7.64 ng/ml

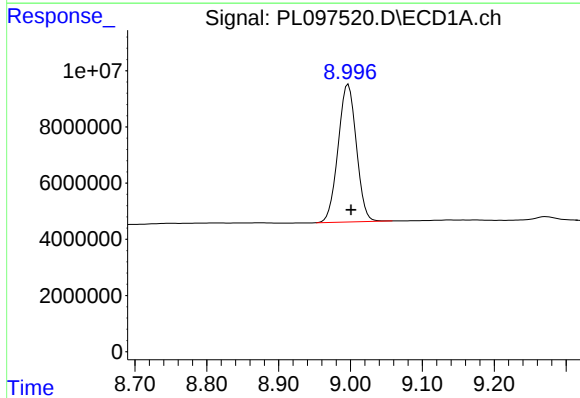

#28 Decachlorobiphenyl

R.T.: 8.997 min
Delta R.T.: -0.004 min
Response: 86389298
Conc: 26.40 ng/ml

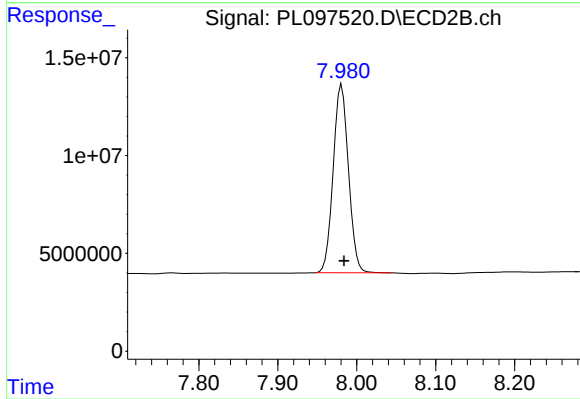

#28 Decachlorobiphenyl

R.T.: 7.981 min
Delta R.T.: -0.003 min
Response: 129477444
Conc: 22.75 ng/ml