

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100325\
 Data File : PL097515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2025 04:40
 Operator : AR\AJ
 Sample : Q3270-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SG-1-TEST-PIT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/06/2025
 Supervised By :mohammad ahmed 10/07/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 01:21:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:40:25 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.525	2.823	62621682	91938898	13.832m	13.982
28)	SA Decachlor...	8.996	7.980	37599634	60656111	11.491	10.657

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100325\
Data File : PL097515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2025 04:40
Operator : AR\AJ
Sample : Q3270-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SG-1-TEST-PIT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/06/2025
Supervised By :mohammad ahmed 10/07/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 01:21:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092025.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:40:25 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

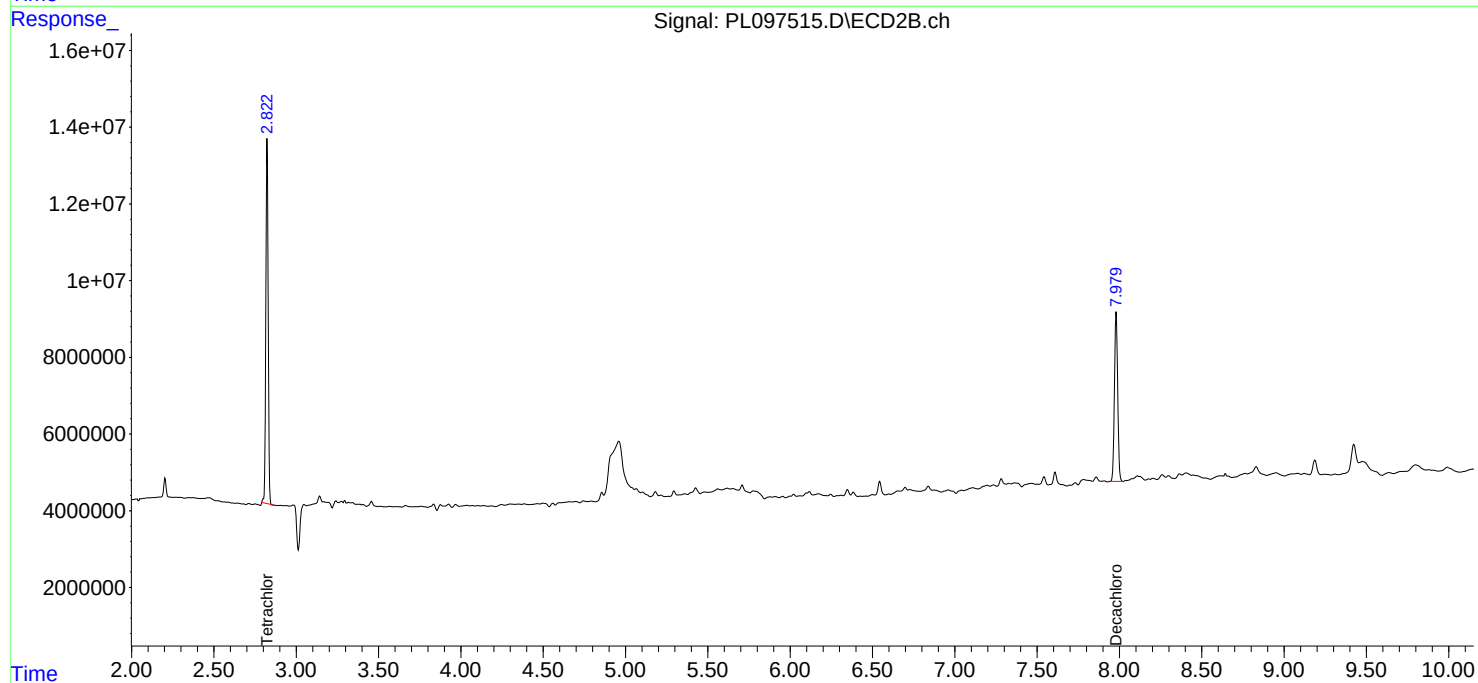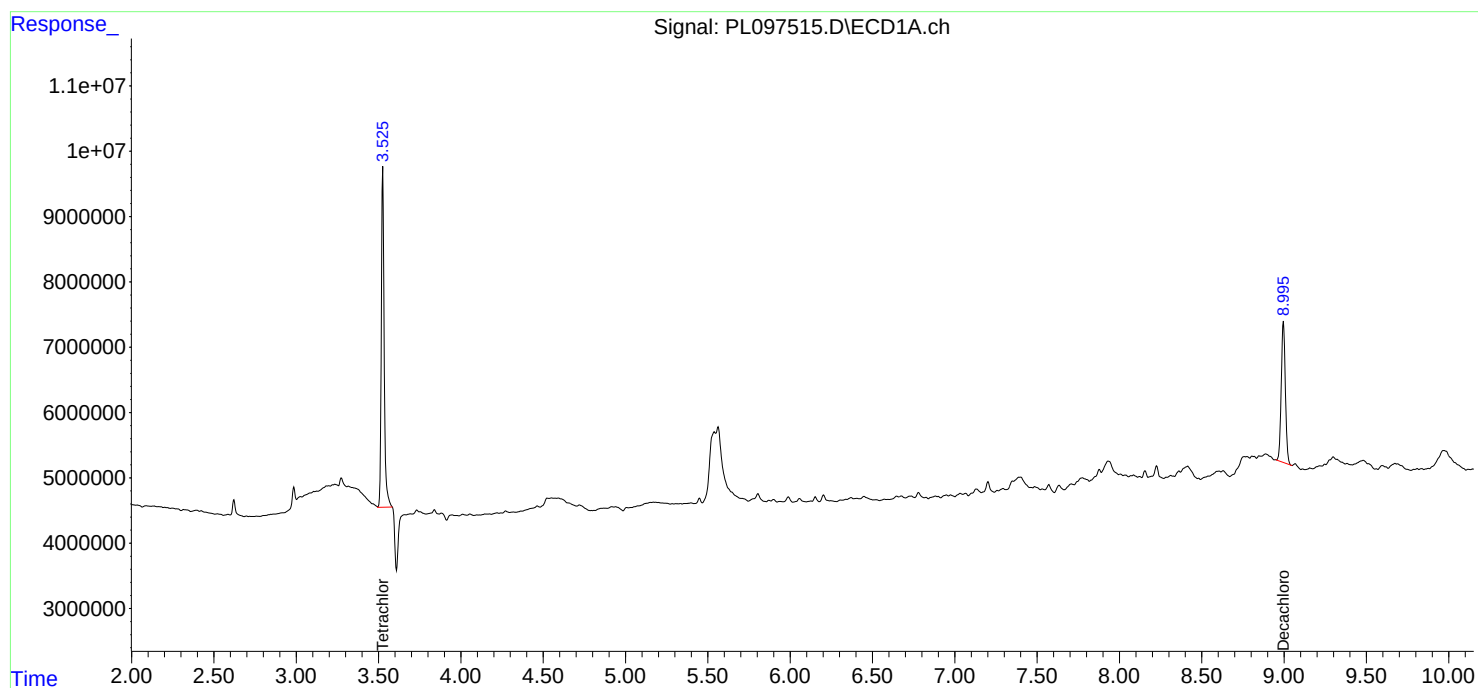

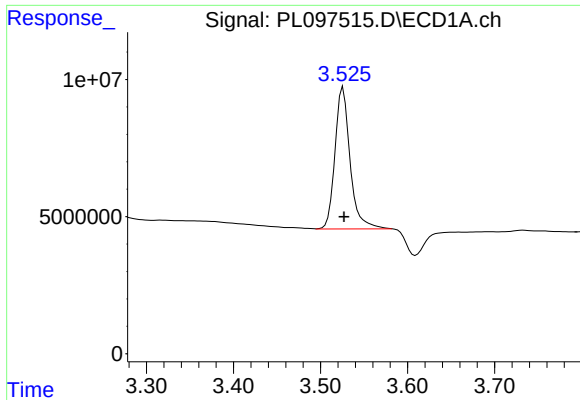


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.002 min
Response: 62621682
Conc: 13.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
SG-1-TEST-PIT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/06/2025
Supervised By :mohammad ahmed 10/07/2025

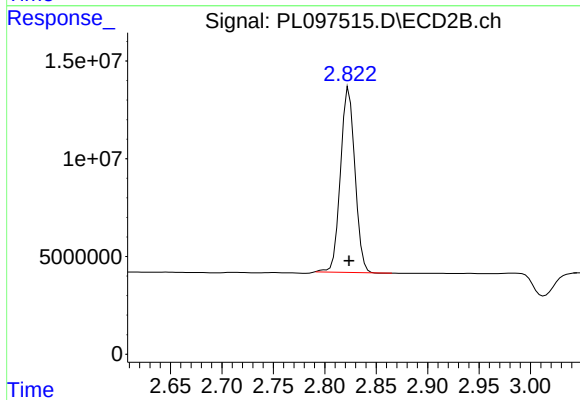


#1 Tetrachloro-m-xylene

R.T.: 2.823 min
Delta R.T.: 0.000 min
Response: 91938898
Conc: 13.98 ng/ml

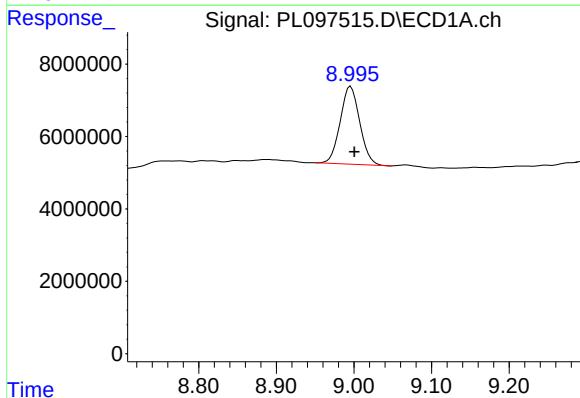

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: -0.005 min
Response: 37599634
Conc: 11.49 ng/ml

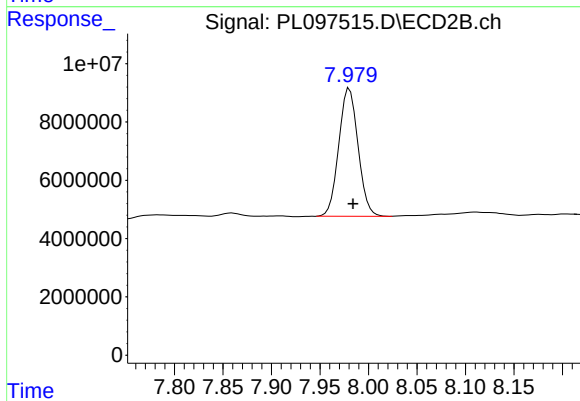

#28 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.004 min
Response: 60656111
Conc: 10.66 ng/ml