

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100418\
 Data File : PL040655.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2018 13:55
 Operator : AJ\SJ
 Sample : PB113491BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 07:10:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 27 01:27:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.209	3.806	154.8E6	58863437	21.151	18.641
28)	SA Decachlor...	7.812	8.730	186.2E6	54565368	19.591	17.230
Target Compounds							
20)	A Methoxychlor	6.501f	0.000	86565806	0	17.921	N.D. #
23)	Chlordane-1	3.964	0.000	30072598	0	85.310	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100418\
Data File : PL040655.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2018 13:55
Operator : AJ\SJ
Sample : PB113491BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 07:10:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092618.M
Quant Title : GC Extractables
QLast Update : Thu Sep 27 01:27:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

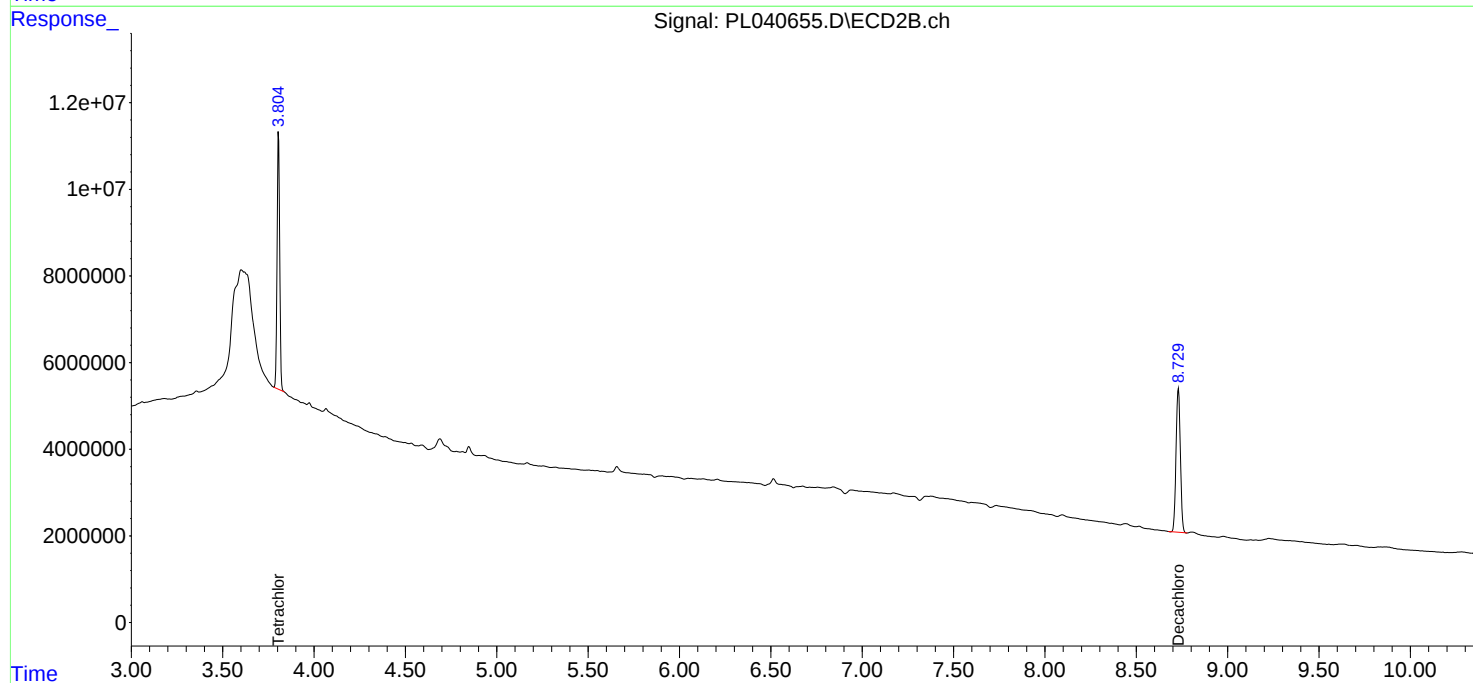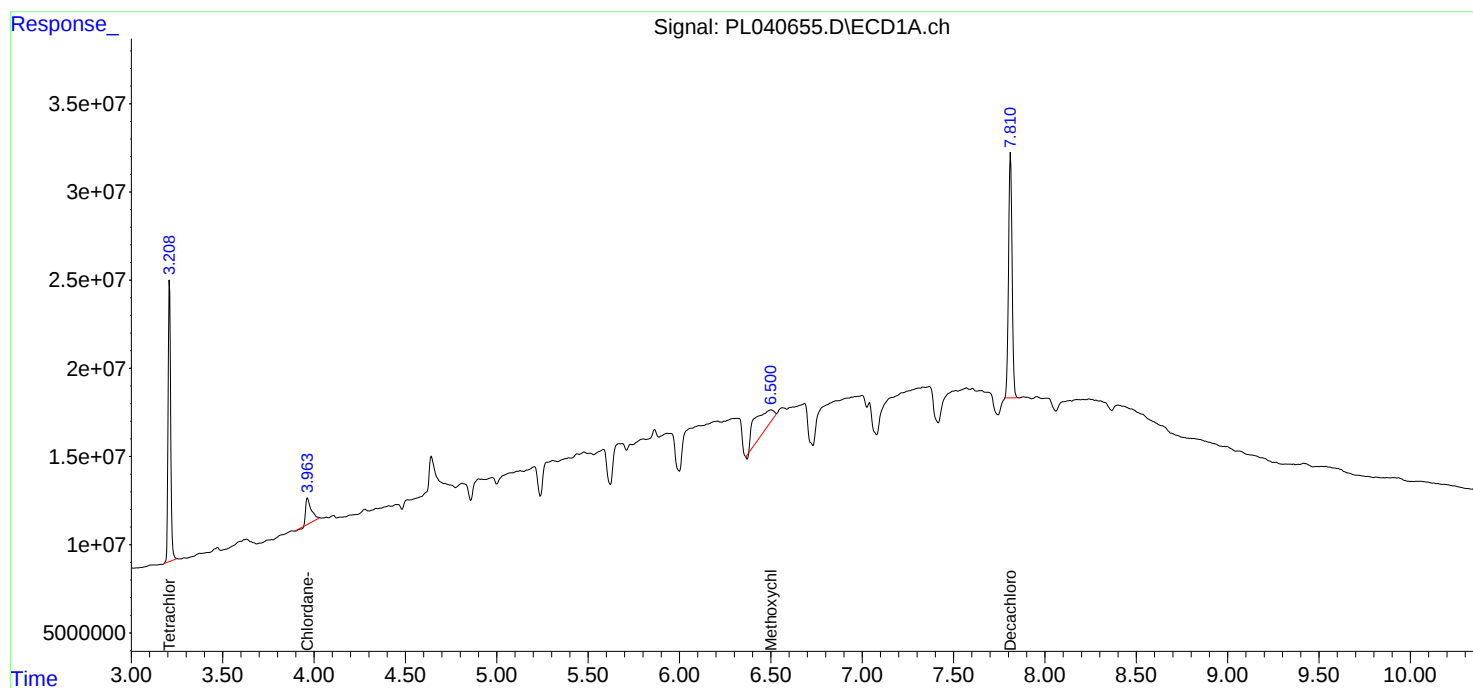


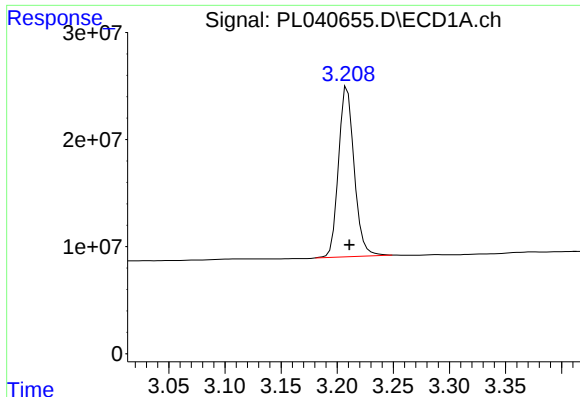

#1 Tetrachloro-m-xylene


R.T.: 3.209 min
Delta R.T.: -0.002 min
Response: 154824361
Conc: 21.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

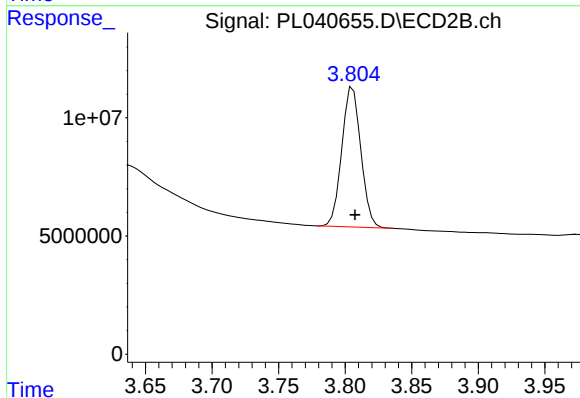


#1 Tetrachloro-m-xylene

R.T.: 3.806 min
Delta R.T.: -0.002 min
Response: 58863437
Conc: 18.64 ng/ml

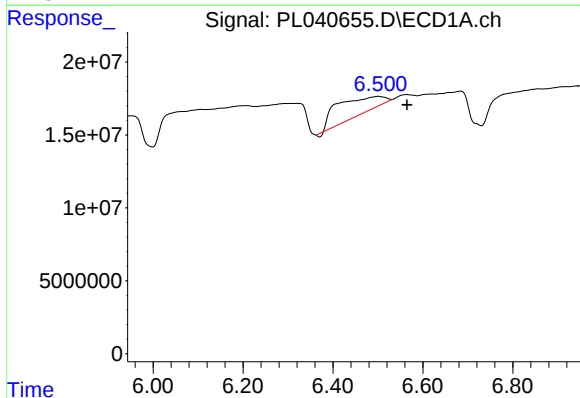


#20 Methoxychlor

R.T.: 6.501 min
Delta R.T.: -0.064 min
Response: 86565806
Conc: 17.92 ng/ml

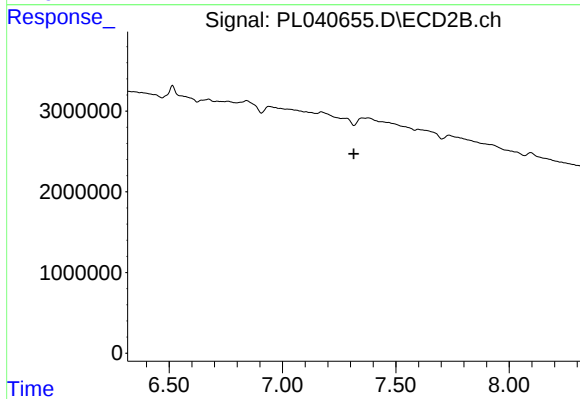

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.314 min
Response: 0
Conc: N.D.

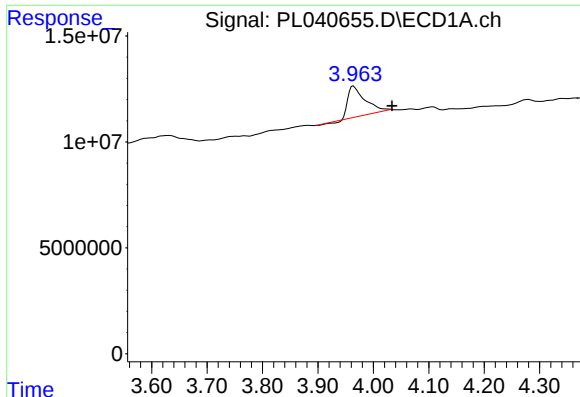

#23 Chlordane-1


R.T.: 3.964 min
Delta R.T.: -0.070 min
Response: 30072598
Conc: 85.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

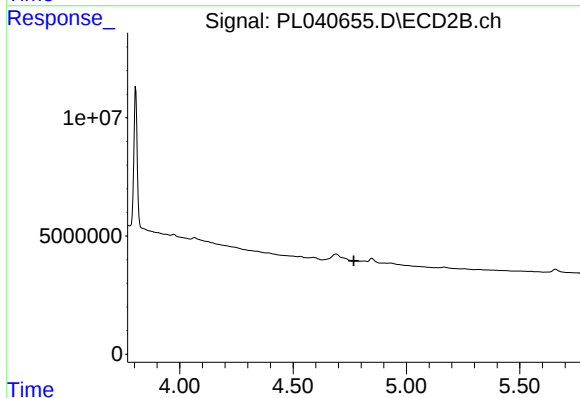


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.768 min
Response: 0
Conc: N.D.

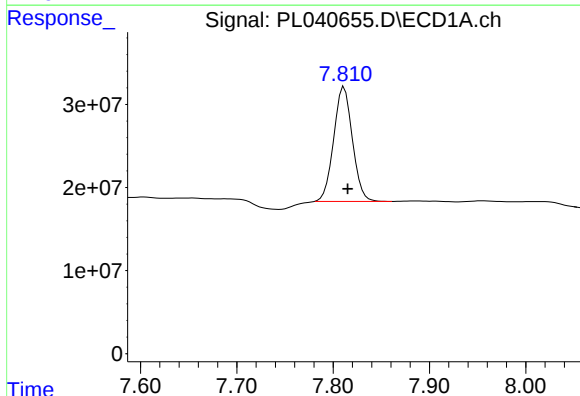

#28 Decachlorobiphenyl

R.T.: 7.812 min
Delta R.T.: -0.003 min
Response: 186230480
Conc: 19.59 ng/ml

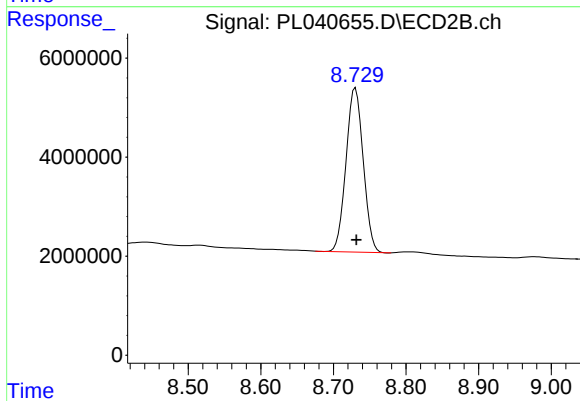

#28 Decachlorobiphenyl

R.T.: 8.730 min
Delta R.T.: -0.001 min
Response: 54565368
Conc: 17.23 ng/ml