

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100419\
 Data File : PL053088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2019 16:51
 Operator : SG\AJ
 Sample : K5156-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSEG-GAS

Manual Integrations
 APPROVED

Ankita
 10/7/2019 1:56:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 22:56:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.047	152.4E6	40446920	15.321m	15.063m
28)	SA Decachlor...	8.340	9.125	166.7E6	53178558	16.645	18.127

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100419\
Data File : PL053088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2019 16:51
Operator : SG\AJ
Sample : K5156-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PSEG-GAS


Manual Integrations
APPROVED

Ankita
10/7/2019 1:56:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 22:56:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

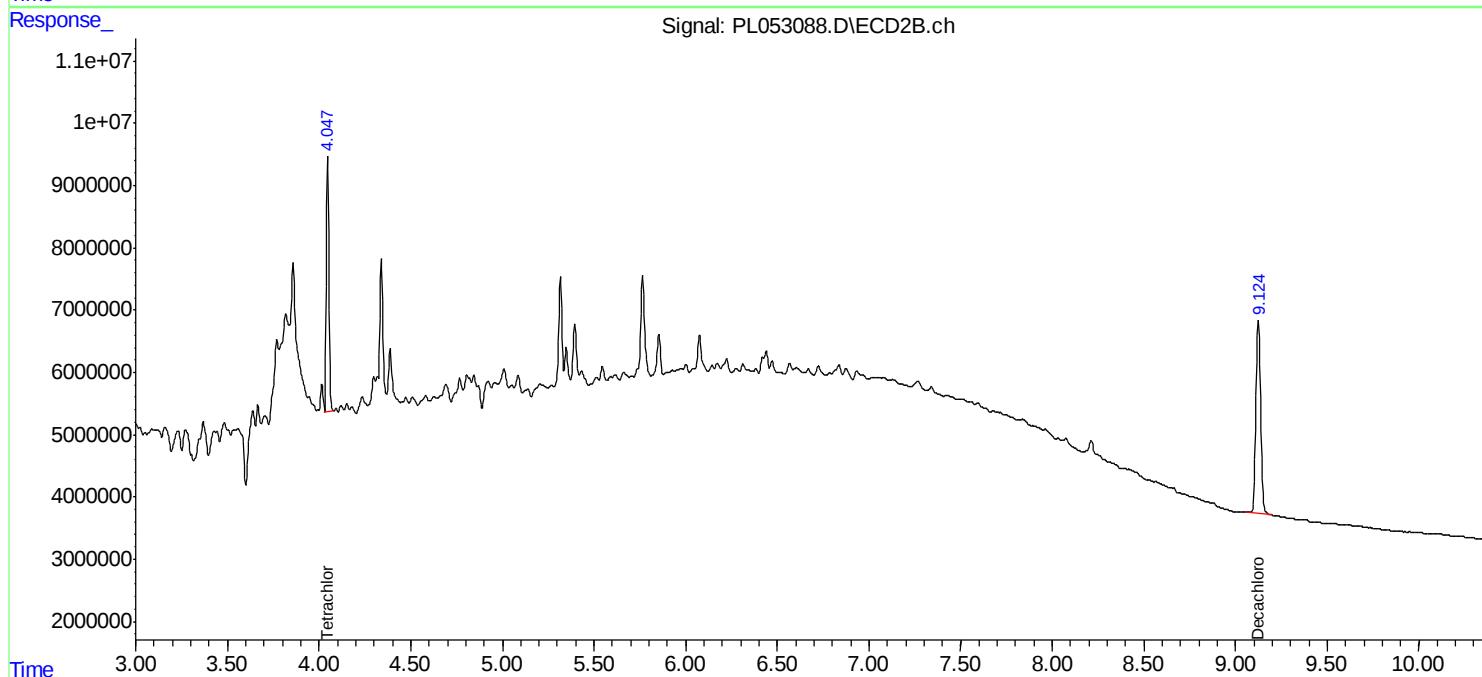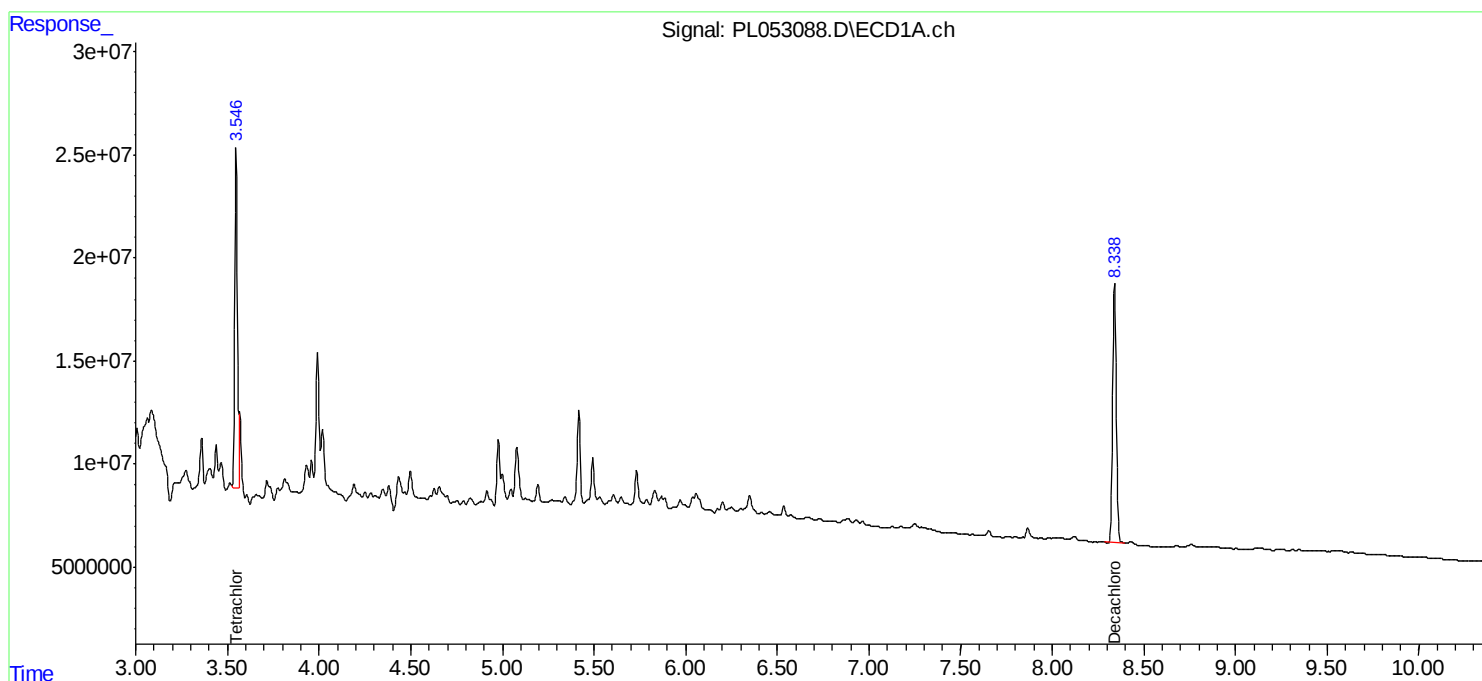

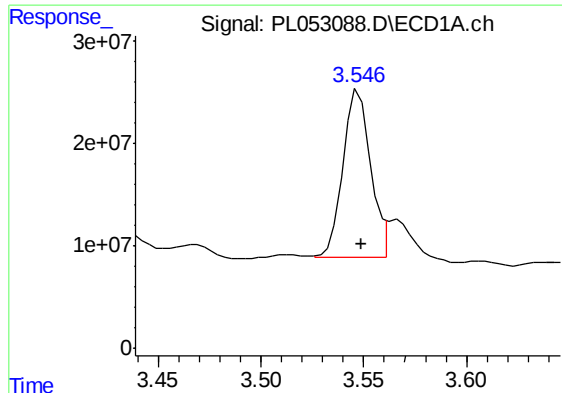


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 152391014
Conc: 15.32 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSEG-GAS


Manual Integrations
APPROVED

Ankita
10/7/2019 1:56:56 PM

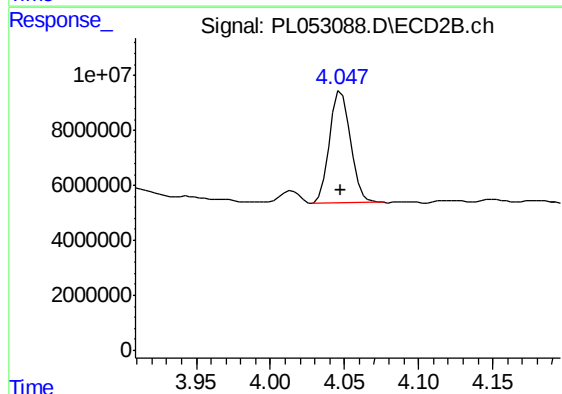


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.000 min
Response: 40446920
Conc: 15.06 ng/ml m

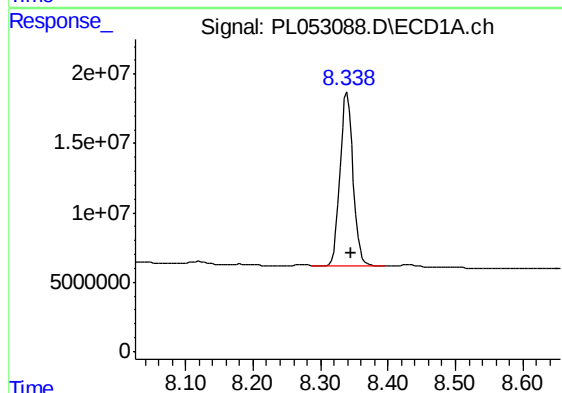

#28 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: -0.006 min
Response: 166720071
Conc: 16.65 ng/ml

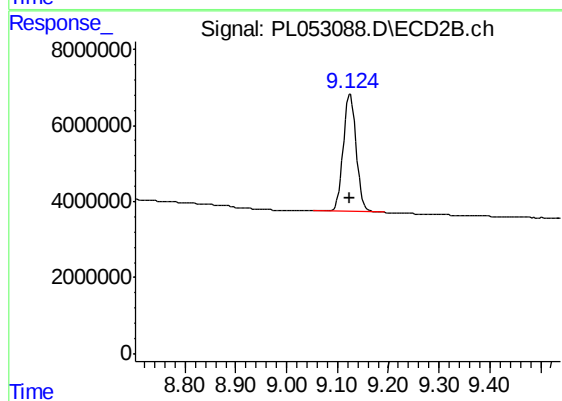

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.000 min
Response: 53178558
Conc: 18.13 ng/ml