

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100421\
 Data File : PL070129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2021 18:24
 Operator : AR\AJ
 Sample : M4037-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-100121

Manual Integrations
 APPROVED

Ankita
 10/5/2021 1:18:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 02:00:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.626	5.562	7621290	18657595	15.231	14.106
28)	SA Decachlor...	10.392	11.482	8953922	17576202	12.940	14.524
Target Compounds							
11)	B alpha-Chl...	7.410	8.376	309803	882072	0.425m	0.559m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100421\
Data File : PL070129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2021 18:24
Operator : AR\AJ
Sample : M4037-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
HD-01-100121


Manual Integrations
APPROVED

Ankita
10/5/2021 1:18:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 02:00:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

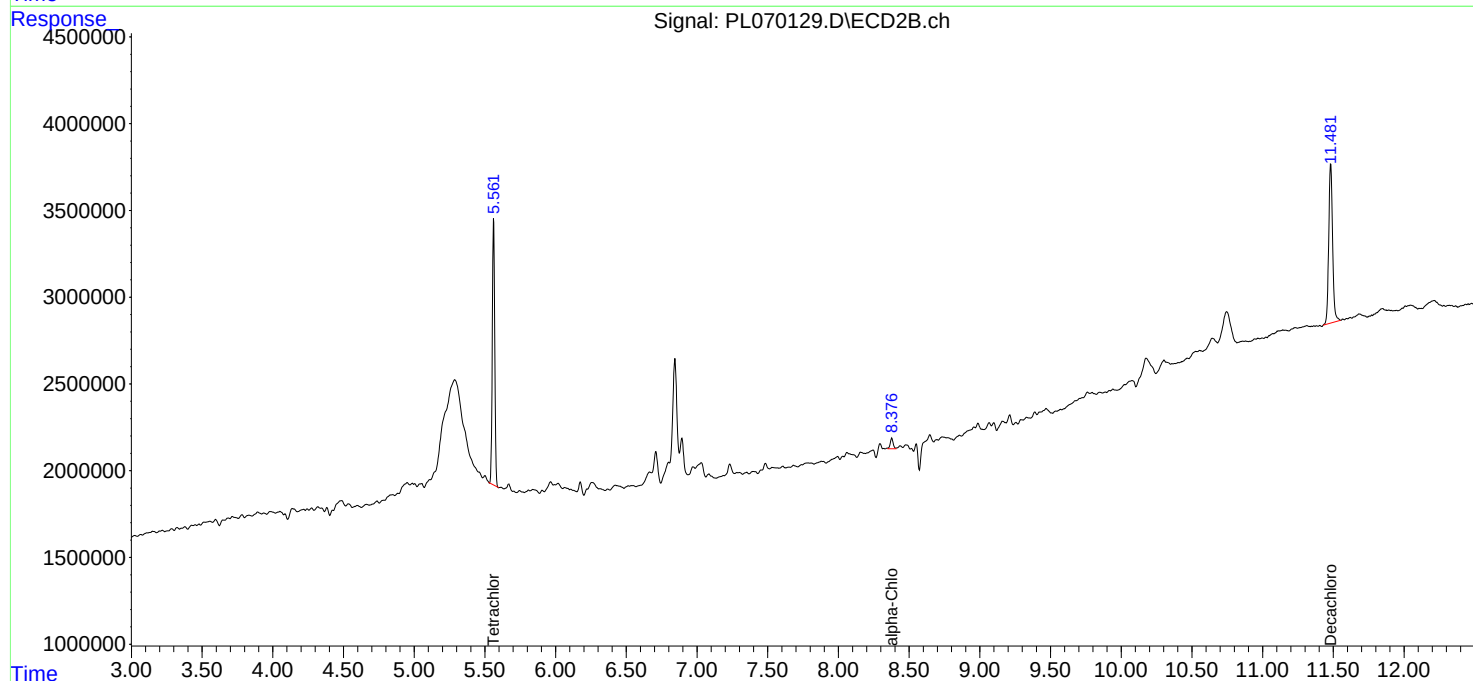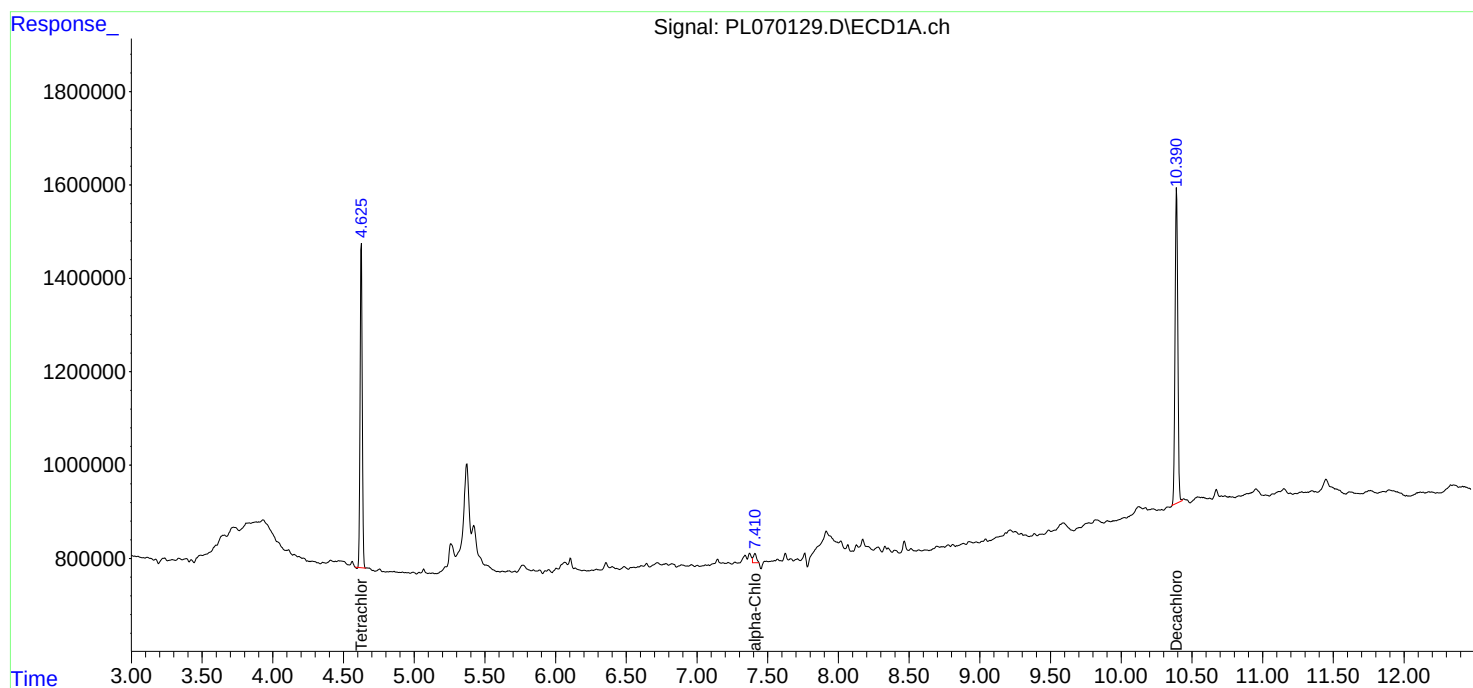

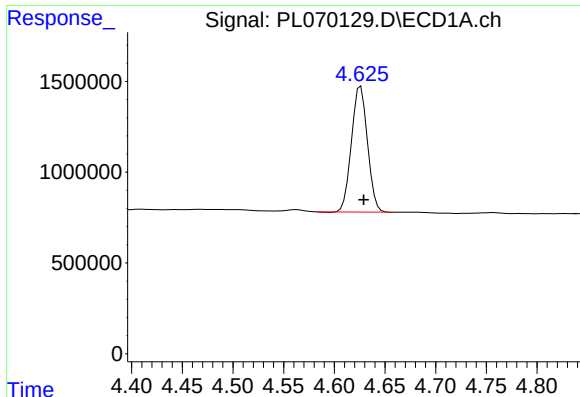


#1 Tetrachloro-m-xylene

R.T.: 4.626 min
Delta R.T.: -0.003 min
Response: 7621290
Conc: 15.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-100121


Manual Integrations
APPROVED

Ankita
10/5/2021 1:18:10 PM

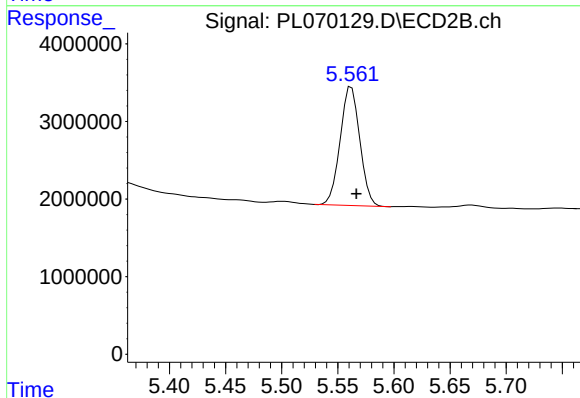


#1 Tetrachloro-m-xylene

R.T.: 5.562 min
Delta R.T.: -0.005 min
Response: 18657595
Conc: 14.11 ng/ml

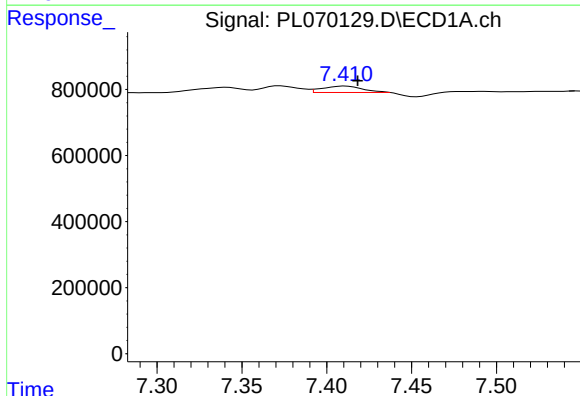


#11 alpha-Chlordane

R.T.: 7.410 min
Delta R.T.: -0.008 min
Response: 309803
Conc: 0.43 ng/ml m

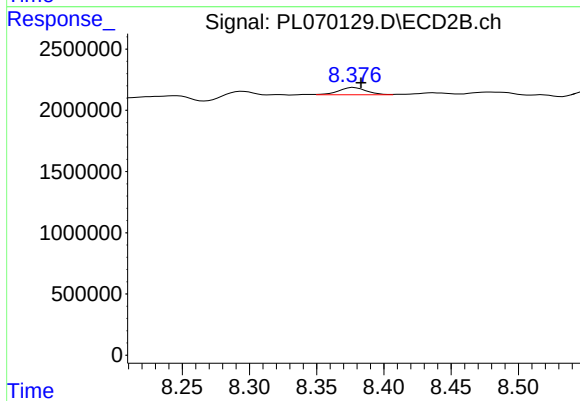

#11 alpha-Chlordane

R.T.: 8.376 min
Delta R.T.: -0.007 min
Response: 882072
Conc: 0.56 ng/ml m

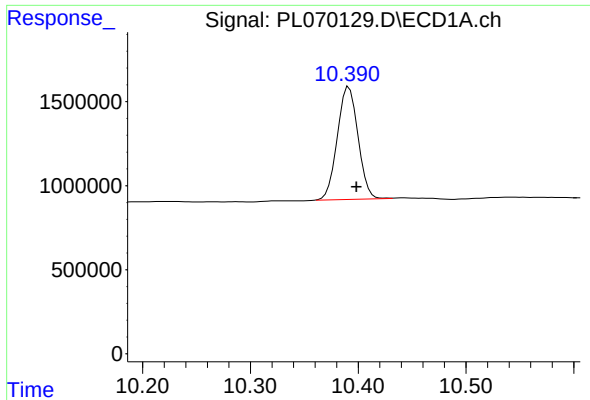


#28 Decachlorobiphenyl

R.T.: 10.392 min
Delta R.T.: -0.007 min
Response: 8953922
Conc: 12.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-100121

Manual Integrations
APPROVED

Ankita
10/5/2021 1:18:10 PM

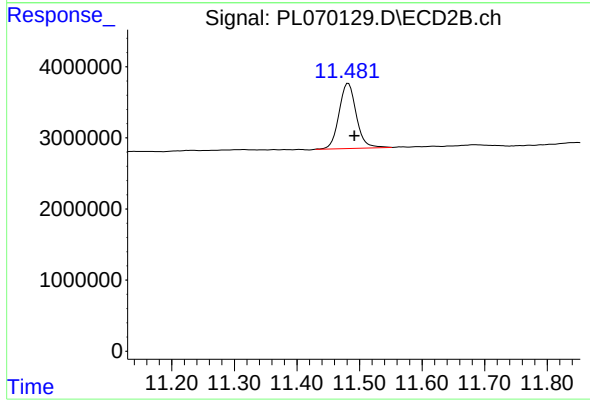

#28 Decachlorobiphenyl

R.T.: 11.482 min
Delta R.T.: -0.010 min
Response: 17576202
Conc: 14.52 ng/ml