

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100422\
 Data File : PL078085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 08:40
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 22:15:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 19:46:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) B	delta-BHC	4.676	0.000	649733	0	0.275	N.D.	#
8) B	Heptachlo...	5.574	4.532	10944223	311811	5.096	0.098	#
10) B	gamma-Chl...	0.000	4.795	0	432850	N.D.	0.136	#
13) MA	Dieldrin	0.000	5.168	0	4402391	N.D.	1.427	#
14) MA	Endrin	0.000	5.470f	0	5041318	N.D.	1.940	#
20) A	Methoxychlor	0.000	6.444f	0	103488	N.D.	0.080	#
21) B	Endrin ke...	7.526	0.000	2810188	0	1.680	N.D.	#
25)	Chlordane-3	0.000	4.795	0	432850	N.D.	1.348	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100422\
Data File : PL078085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 08:40
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 22:15:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 19:46:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

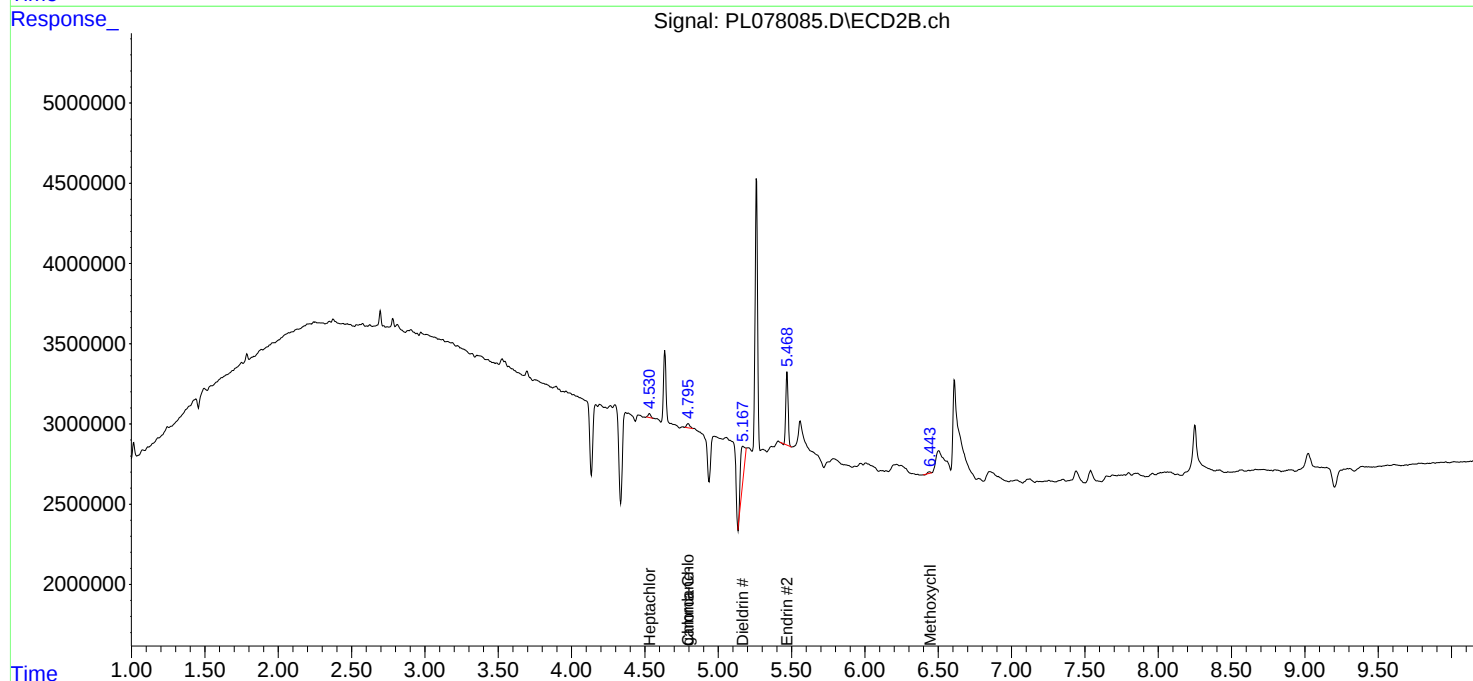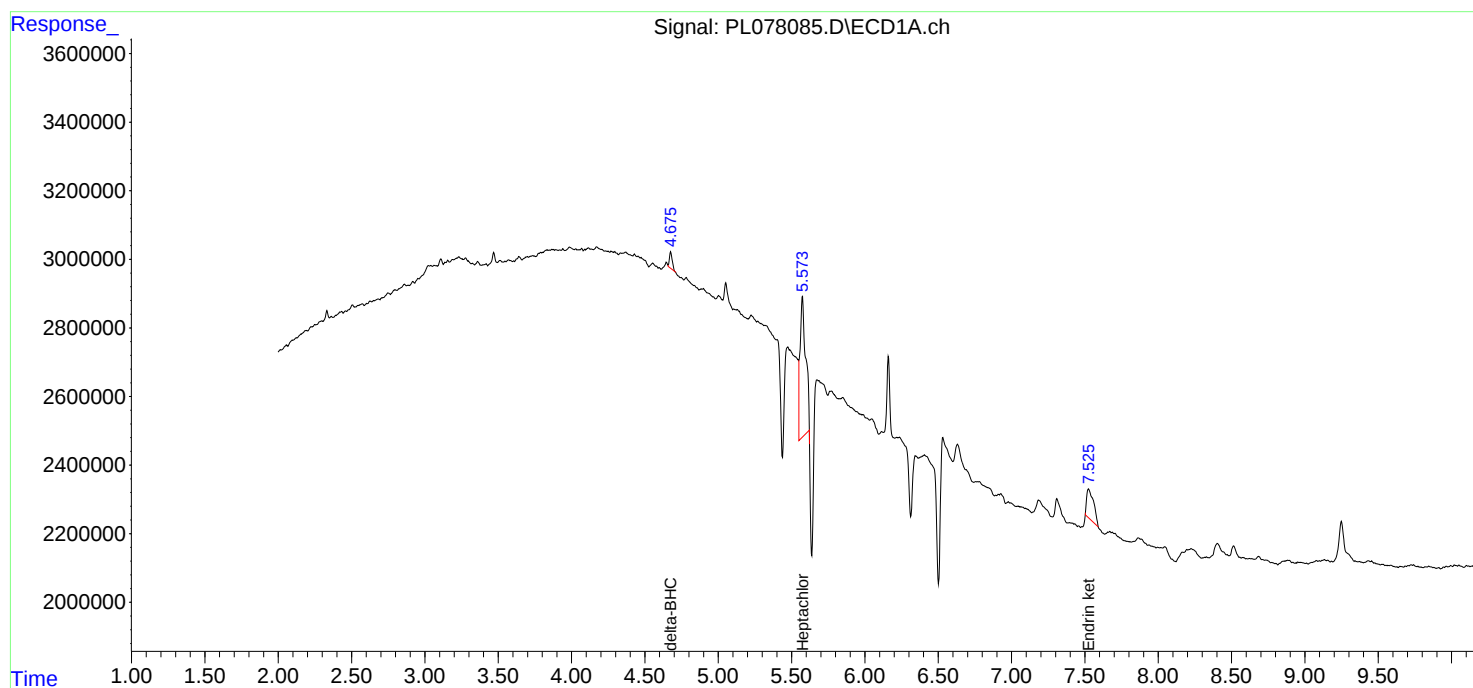


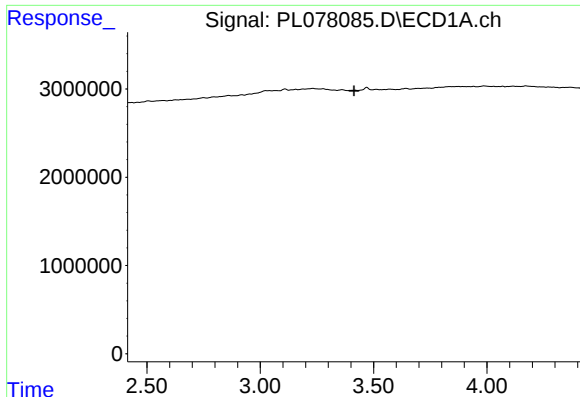

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

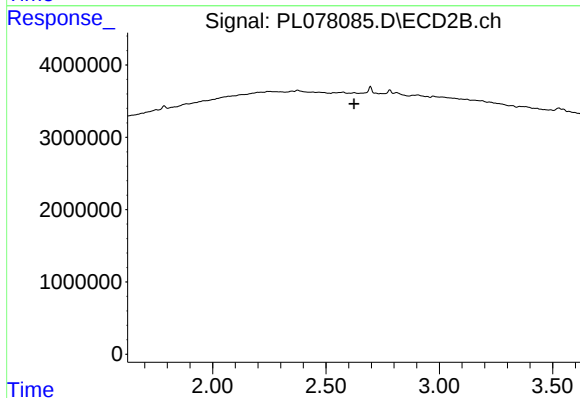


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.624 min
Response: 0
Conc: N.D.

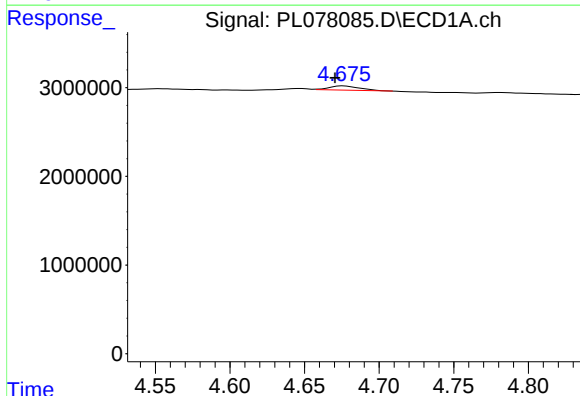


#7 delta-BHC

R.T.: 4.676 min
Delta R.T.: 0.006 min
Response: 649733
Conc: 0.27 ng/ml

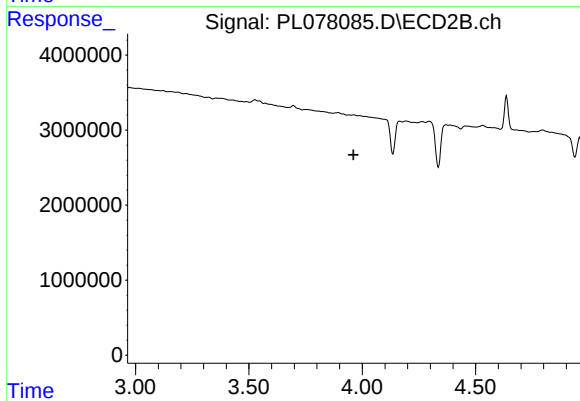

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 3.962 min
Response: 0
Conc: N.D.

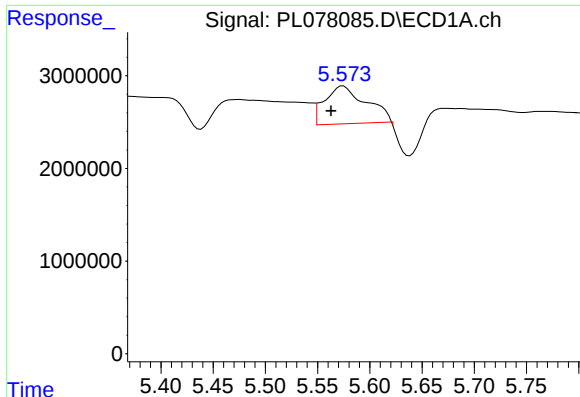

#8 Heptachlor epoxide


R.T.: 5.574 min
Delta R.T.: 0.012 min
Response: 10944223
Conc: 5.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

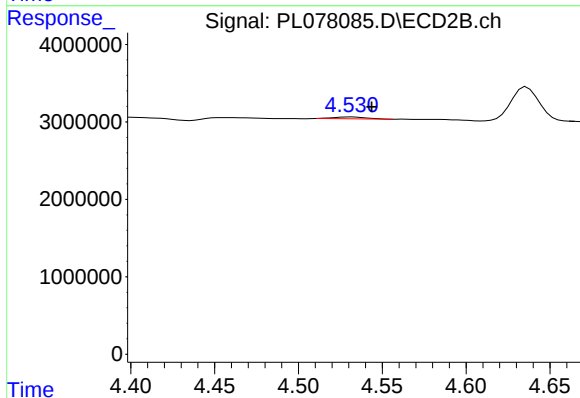


#8 Heptachlor epoxide

R.T.: 4.532 min
Delta R.T.: -0.012 min
Response: 311811
Conc: 0.10 ng/ml

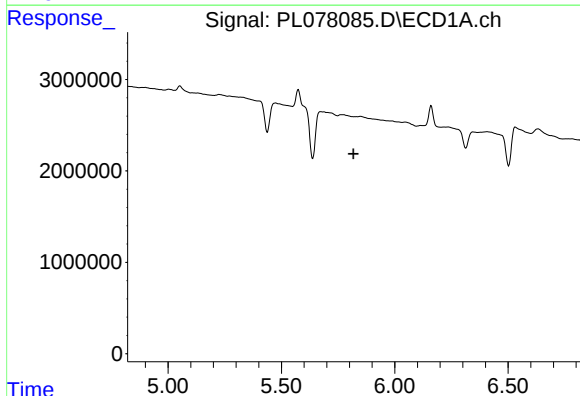


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.818 min
Response: 0
Conc: N.D.

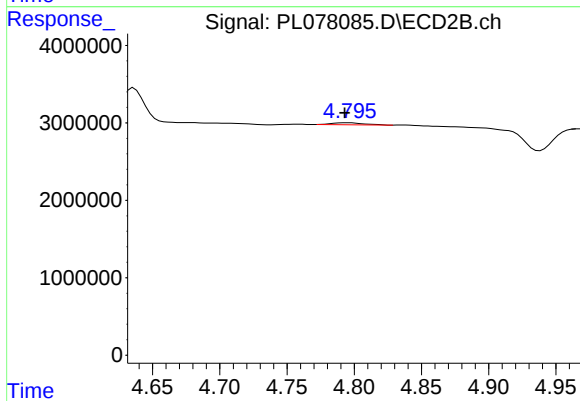

#10 gamma-Chlordane


R.T.: 4.795 min
Delta R.T.: 0.002 min
Response: 432850
Conc: 0.14 ng/ml

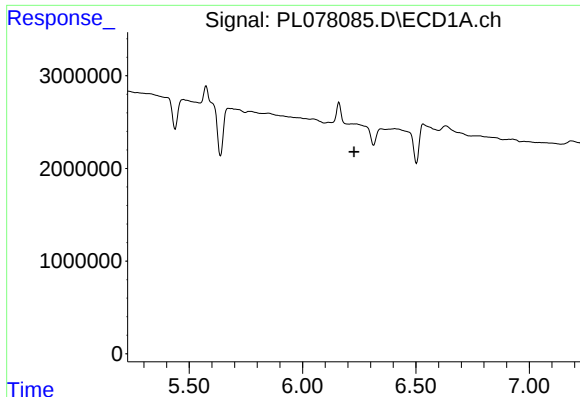

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

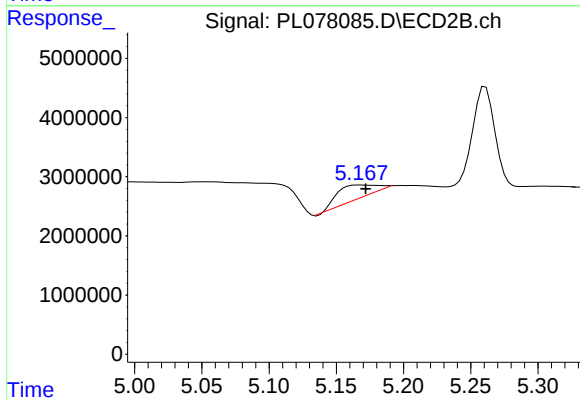


#13 Dieldrin

R.T.: 5.168 min
Delta R.T.: -0.004 min
Response: 4402391
Conc: 1.43 ng/ml

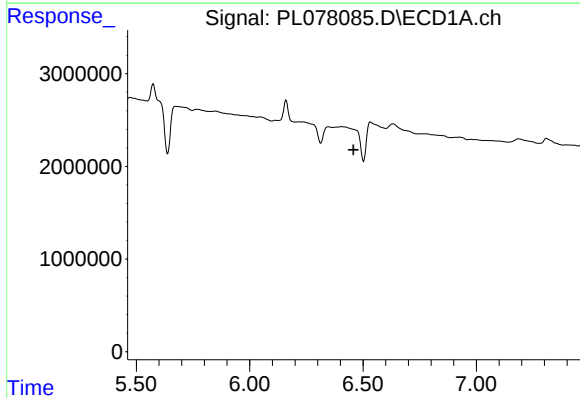


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.458 min
Response: 0
Conc: N.D.

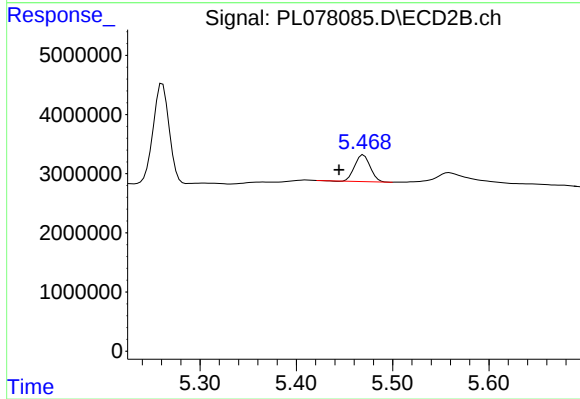

#14 Endrin


R.T.: 5.470 min
Delta R.T.: 0.025 min
Response: 5041318
Conc: 1.94 ng/ml

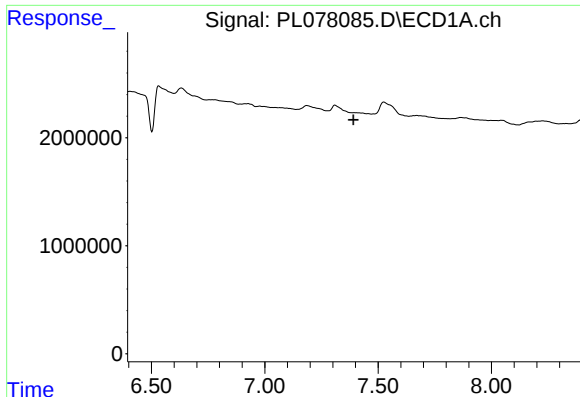

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

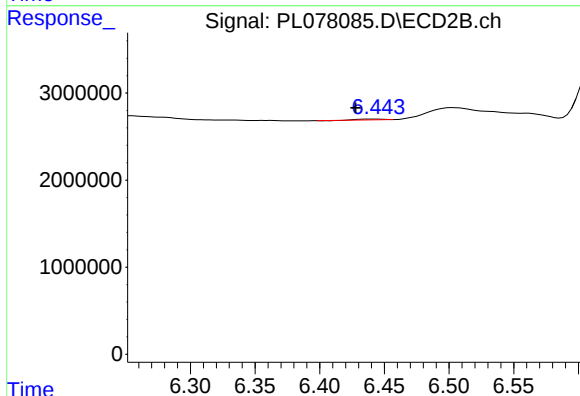


#20 Methoxychlor

R.T.: 6.444 min
Delta R.T.: 0.016 min
Response: 103488
Conc: 0.08 ng/ml

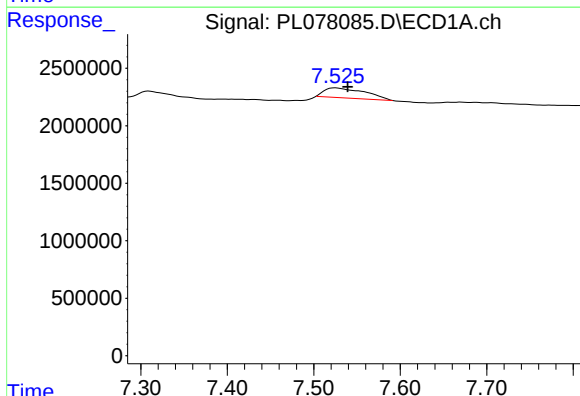


#21 Endrin ketone

R.T.: 7.526 min
Delta R.T.: -0.013 min
Response: 2810188
Conc: 1.68 ng/ml

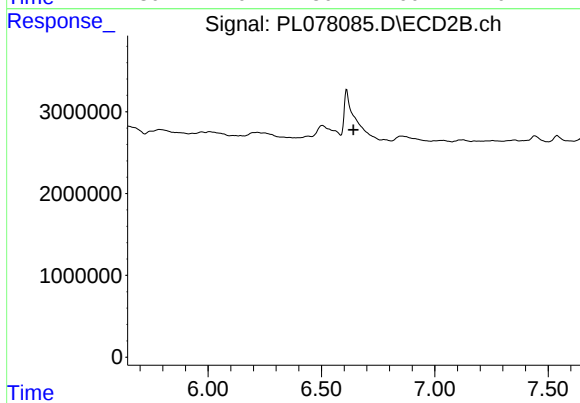

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.642 min
Response: 0
Conc: N.D.

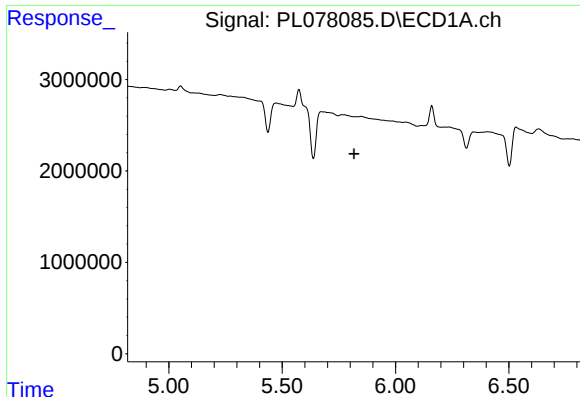

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.818 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

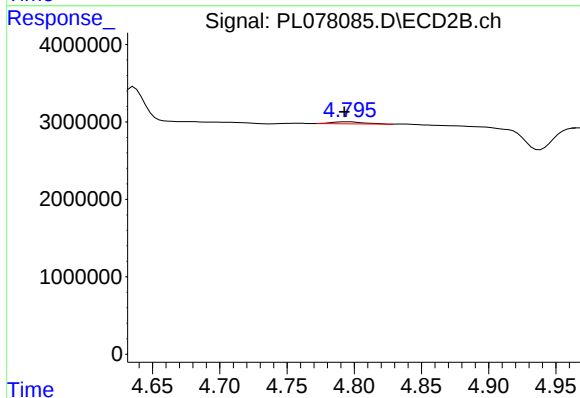


#25 Chlordane-3

R.T.: 4.795 min
Delta R.T.: 0.003 min
Response: 432850
Conc: 1.35 ng/ml

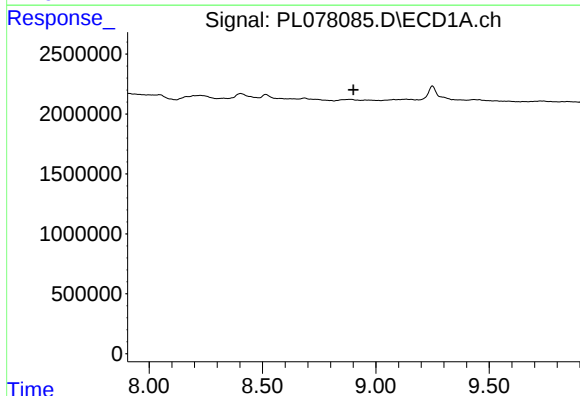

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.902 min
Response: 0
Conc: N.D.

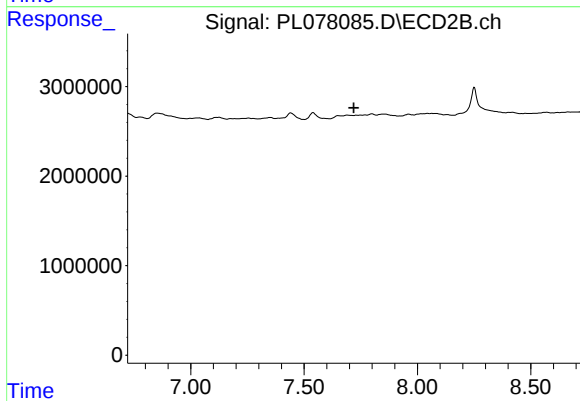

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.720 min
Response: 0
Conc: N.D.