

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100422\
 Data File : PL078089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 11:26
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 22:16:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 19:46:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.621	86185178	156.7E6	46.730	55.741
28)	SA Decachlor...	8.912	7.724	78940682	109.9E6	50.284	50.660
Target Compounds							
23)	Chlordane-1	4.581	3.599	36257844	50925503	494.315	497.468
24)	Chlordane-2	5.114	4.169	37668604	53723319	466.920	481.894
25)	Chlordane-3	5.826	4.794	145.7E6	154.6E6	489.515	481.625
26)	Chlordane-4	5.905	4.855	174.7E6	163.7E6	486.554	488.782
27)	Chlordane-5	6.763	5.520	29220086	42785381	482.564	516.466



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100422\
Data File : PL078089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 11:26
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 22:16:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 19:46:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

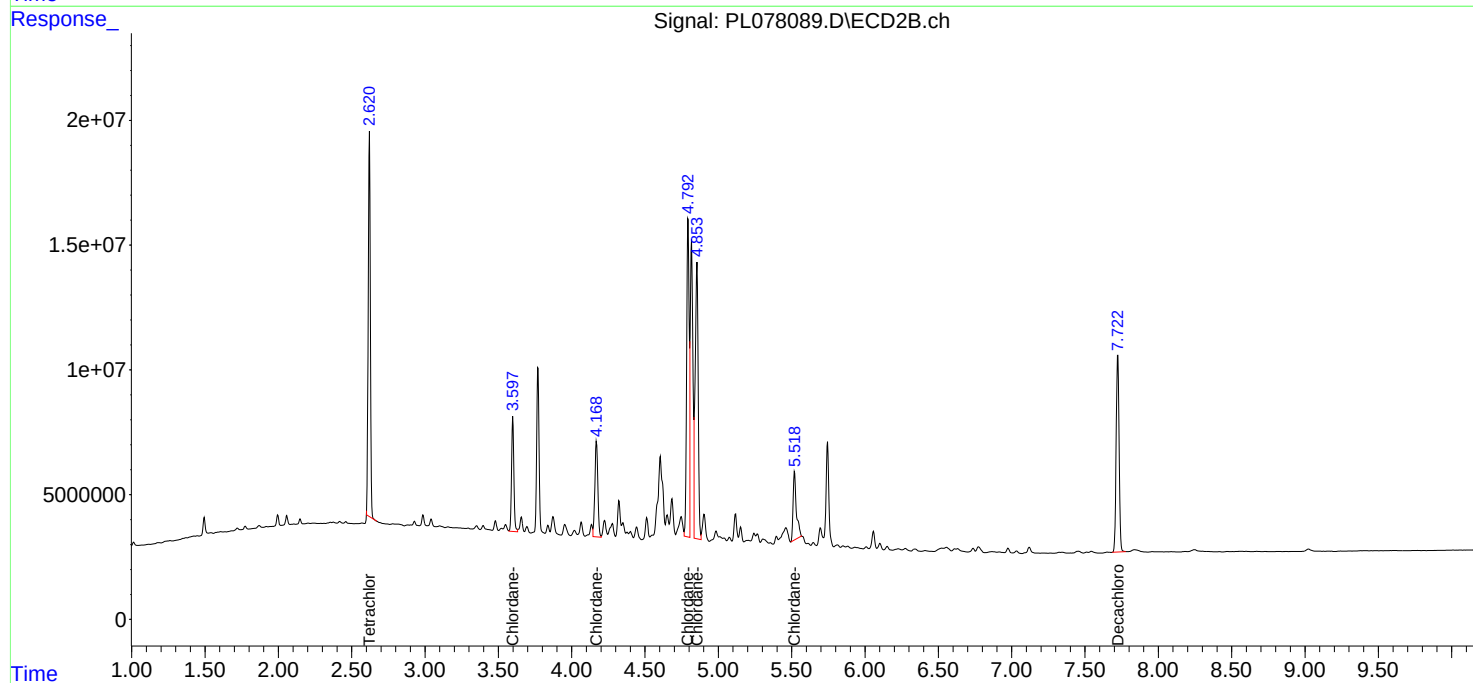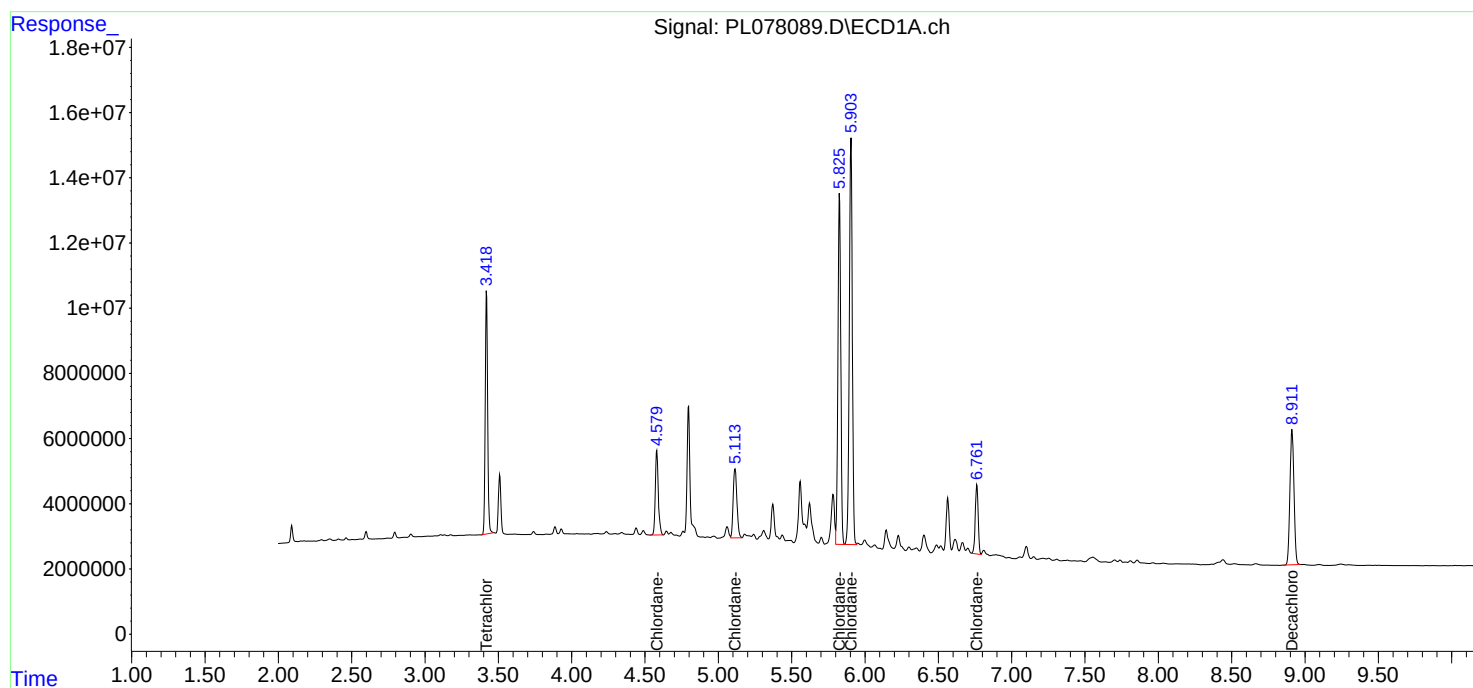


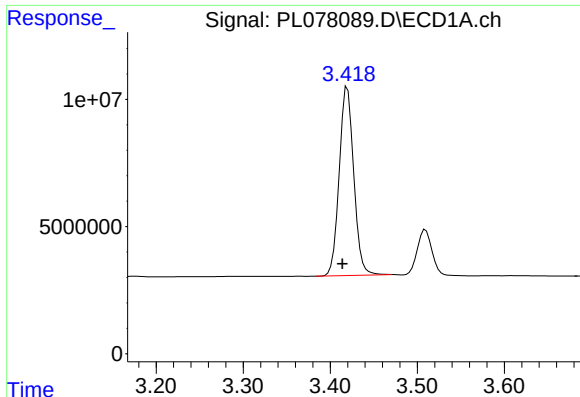

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.006 min
Response: 86185178
Conc: 46.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

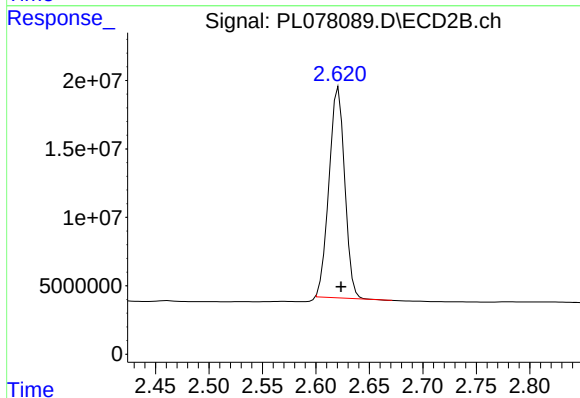


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.002 min
Response: 156669942
Conc: 55.74 ng/ml

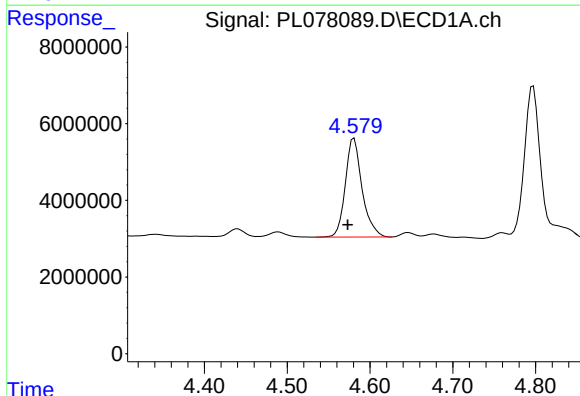


#23 Chlordane-1

R.T.: 4.581 min
Delta R.T.: 0.008 min
Response: 36257844
Conc: 494.31 ng/ml

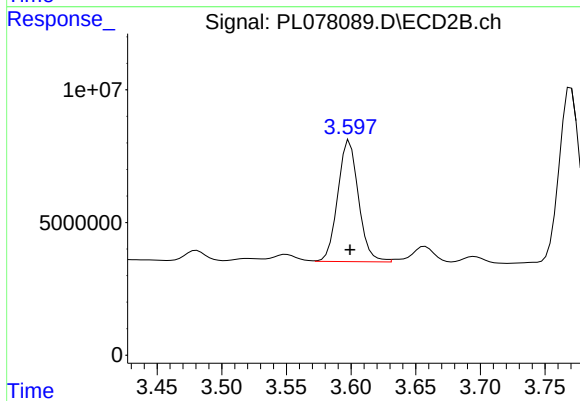

#23 Chlordane-1


R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 50925503
Conc: 497.47 ng/ml

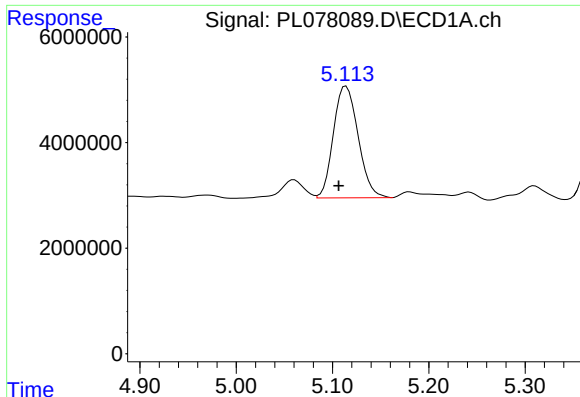

#24 Chlordane-2


R.T.: 5.114 min
Delta R.T.: 0.008 min
Response: 37668604
Conc: 466.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

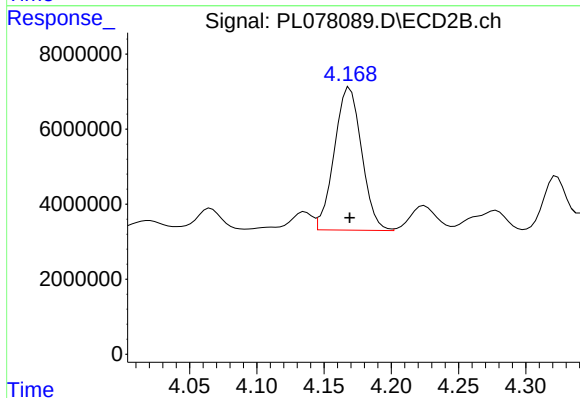


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 53723319
Conc: 481.89 ng/ml

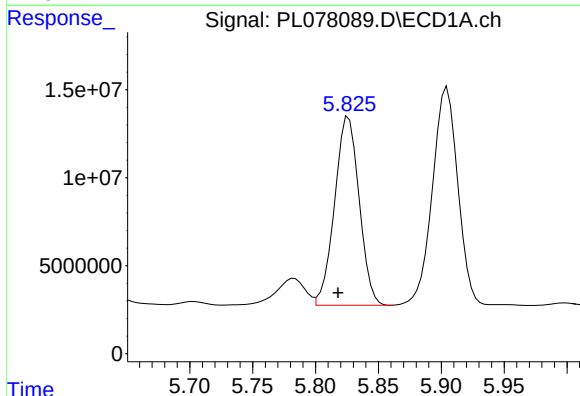


#25 Chlordane-3

R.T.: 5.826 min
Delta R.T.: 0.008 min
Response: 145697517
Conc: 489.52 ng/ml

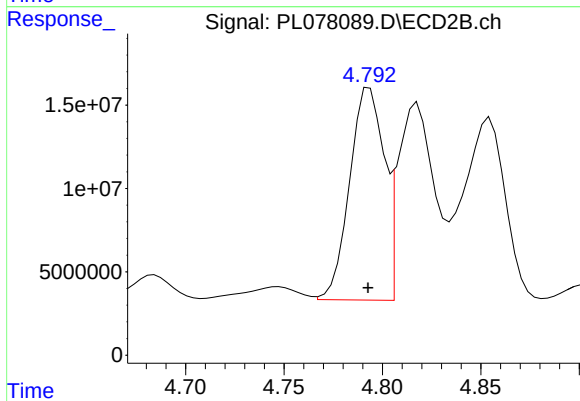

#25 Chlordane-3


R.T.: 4.794 min
Delta R.T.: 0.000 min
Response: 154617043
Conc: 481.62 ng/ml

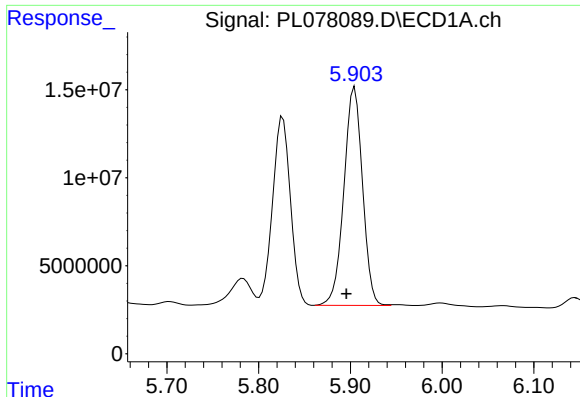

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: 0.009 min
Response: 174661753
Conc: 486.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

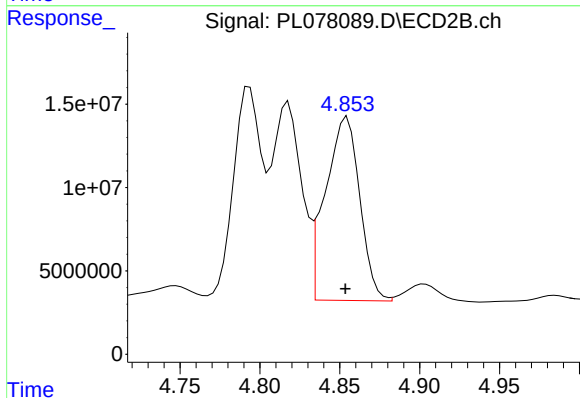


#26 Chlordane-4

R.T.: 4.855 min
Delta R.T.: 0.001 min
Response: 163731935
Conc: 488.78 ng/ml

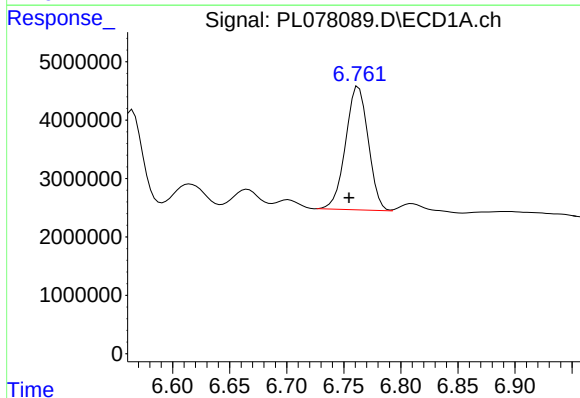


#27 Chlordane-5

R.T.: 6.763 min
Delta R.T.: 0.008 min
Response: 29220086
Conc: 482.56 ng/ml

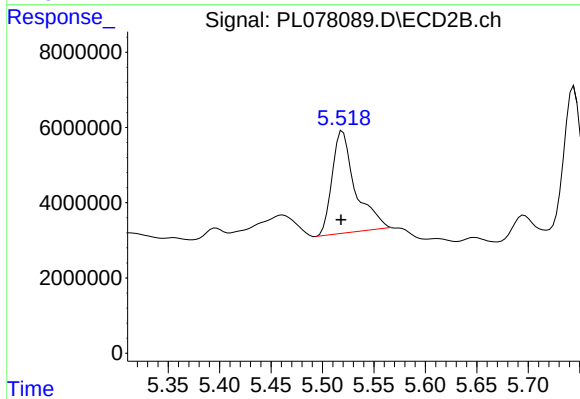

#27 Chlordane-5


R.T.: 5.520 min
Delta R.T.: 0.002 min
Response: 42785381
Conc: 516.47 ng/ml

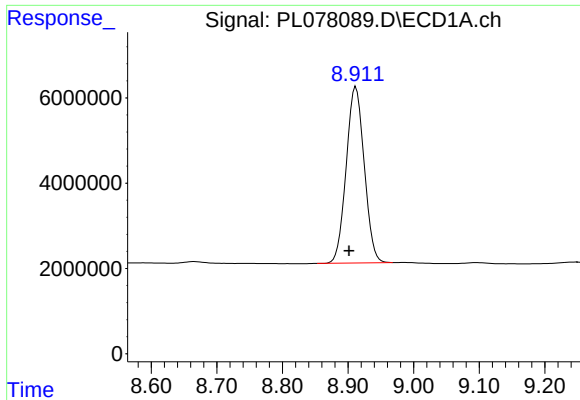

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.010 min
Response: 78940682
Conc: 50.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

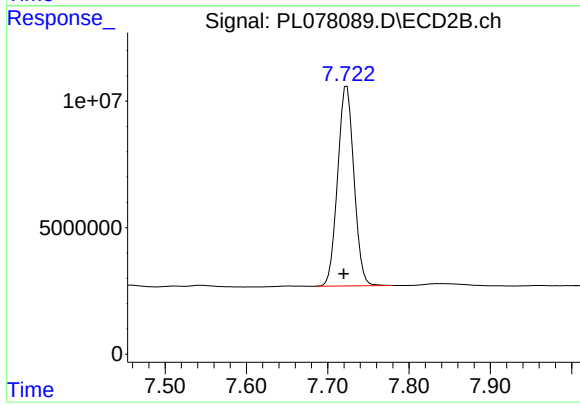

#28 Decachlorobiphenyl

R.T.: 7.724 min
Delta R.T.: 0.004 min
Response: 109937076
Conc: 50.66 ng/ml