

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100422\
 Data File : PL078094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 13:07
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 22:17:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 03 19:46:18 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	87782835	166.7E6	47.596	59.312
28)	SA Decachlor...	8.903	7.720	78718532	113.3E6	50.142	52.191
Target Compounds							
23)	Chlordane-1	4.574	3.599	36319489	53392603	495.155	521.568
24)	Chlordane-2	5.107	4.169	37997368	56593228	470.995	507.637
25)	Chlordane-3	5.820	4.793	146.4E6	161.7E6	491.771	503.822
26)	Chlordane-4	5.898	4.854	174.9E6	170.0E6	487.172	507.376
27)	Chlordane-5	6.757	5.518	29944873	43961625	494.534	530.665



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100422\
Data File : PL078094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 13:07
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 22:17:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100322.M
Quant Title : GC Extractables
QLast Update : Mon Oct 03 19:46:18 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

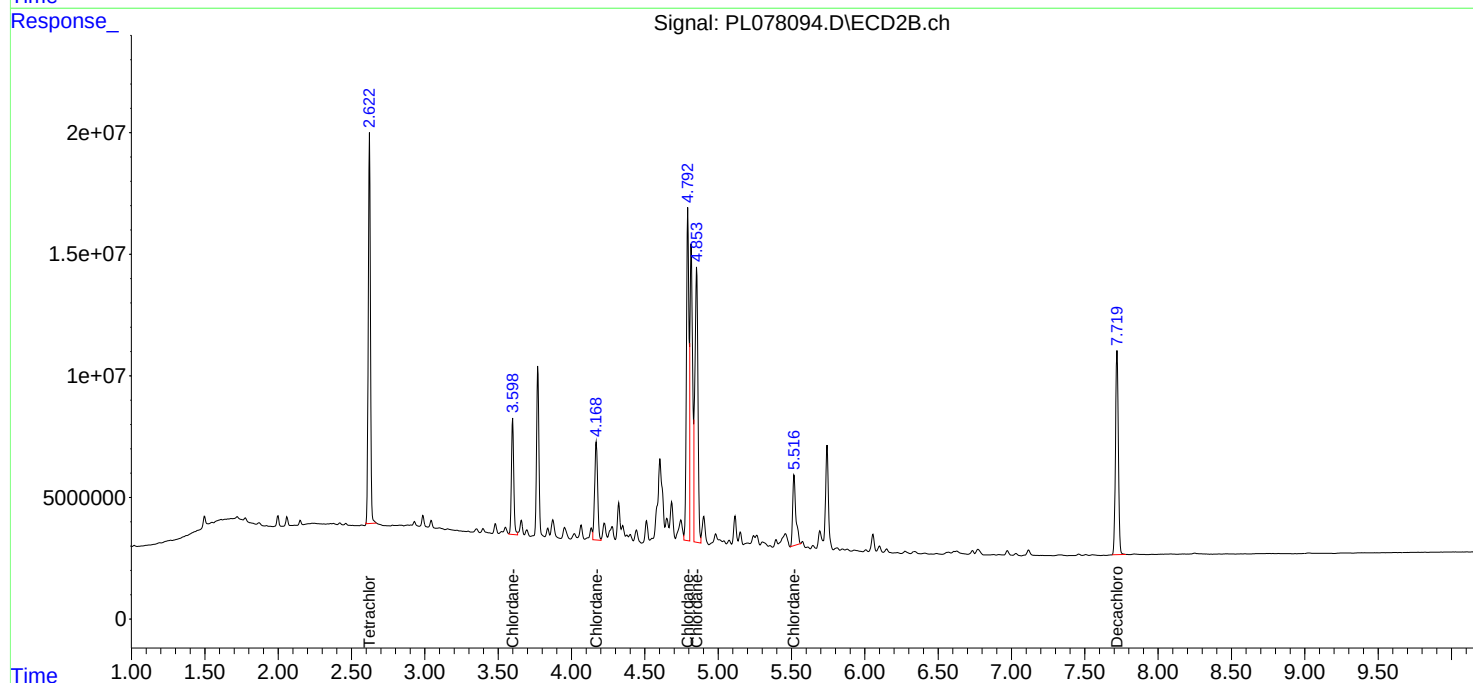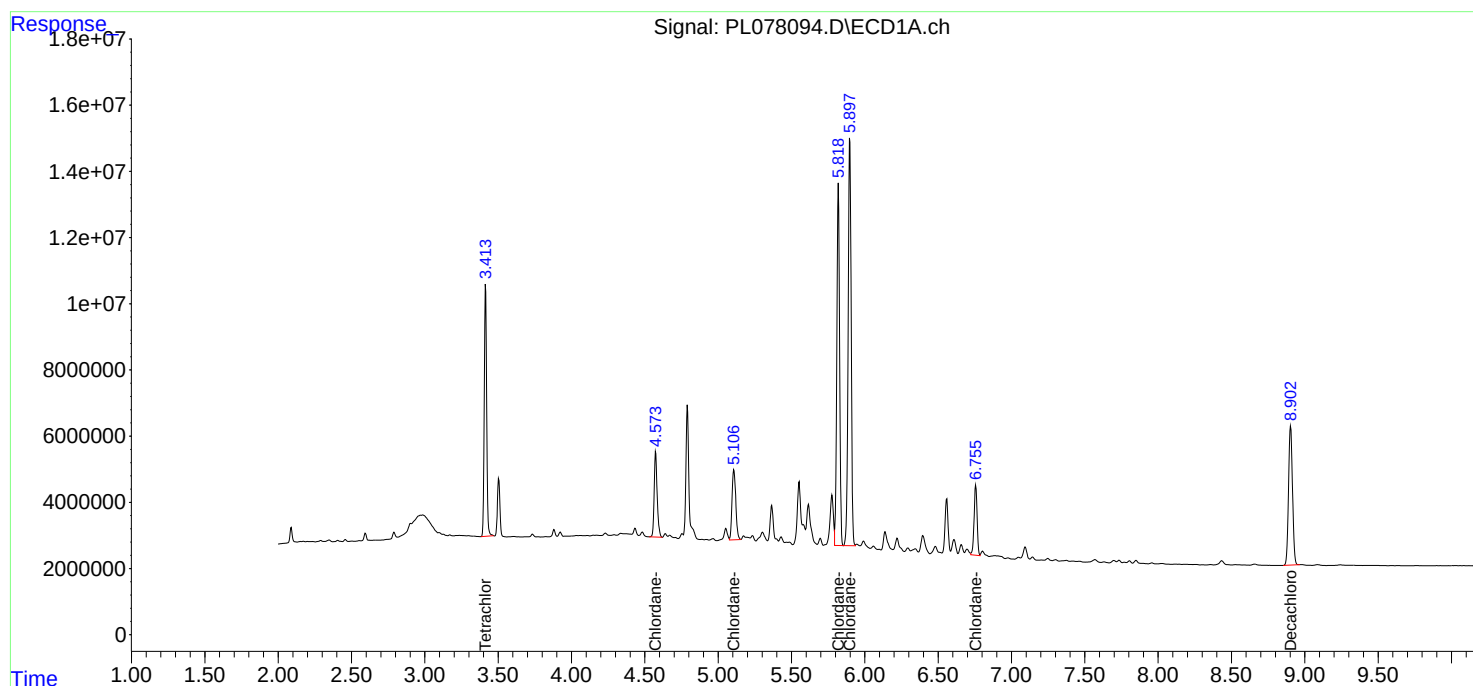


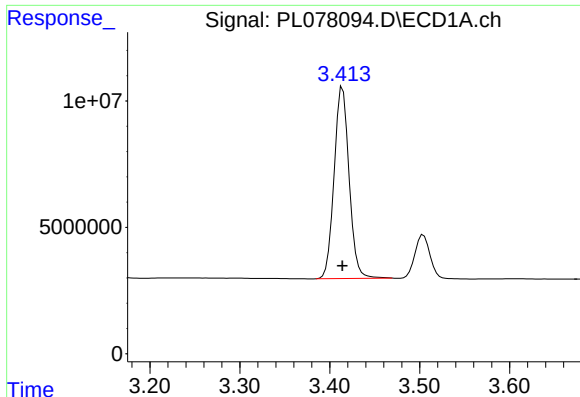

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.000 min
Response: 87782835
Conc: 47.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

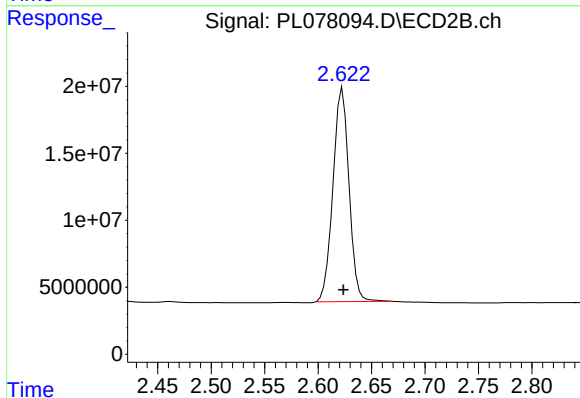


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 166706525
Conc: 59.31 ng/ml

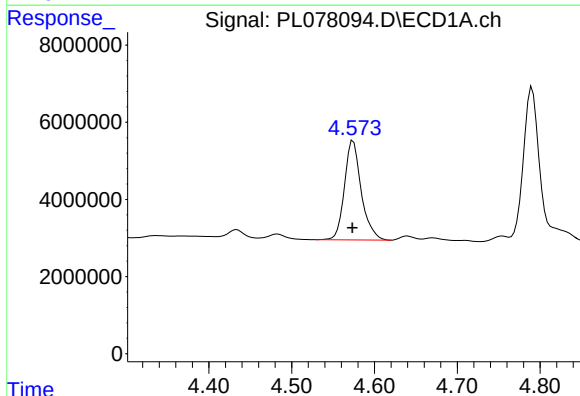


#23 Chlordane-1

R.T.: 4.574 min
Delta R.T.: 0.001 min
Response: 36319489
Conc: 495.16 ng/ml

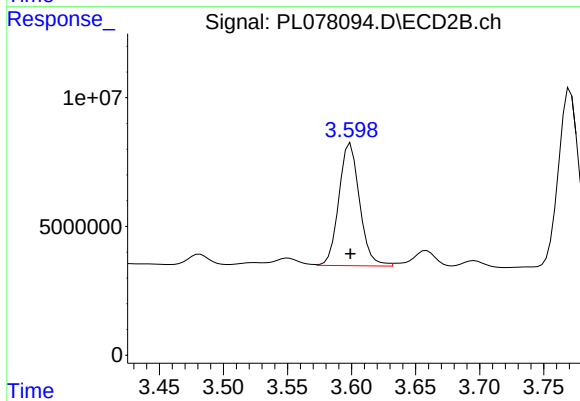

#23 Chlordane-1


R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 53392603
Conc: 521.57 ng/ml

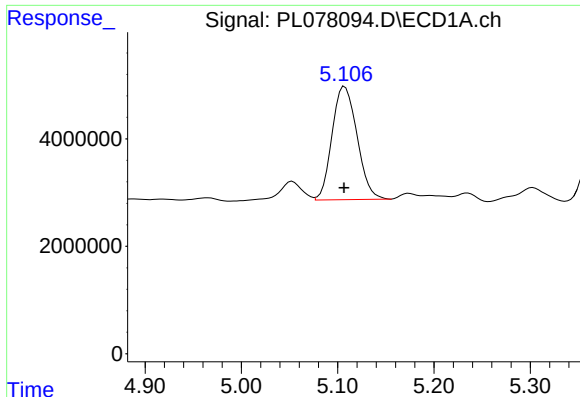

#24 Chlordane-2


R.T.: 5.107 min
Delta R.T.: 0.000 min
Response: 37997368
Conc: 471.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

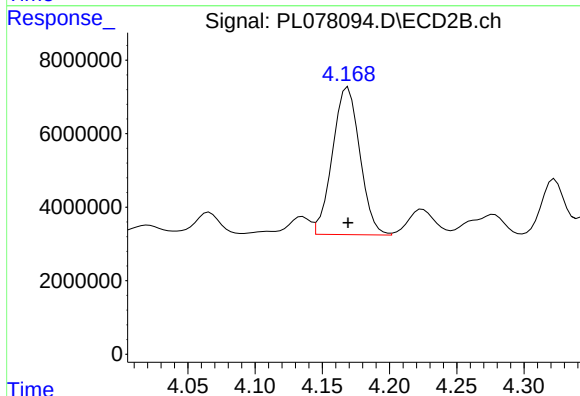


#24 Chlordane-2

R.T.: 4.169 min
Delta R.T.: 0.000 min
Response: 56593228
Conc: 507.64 ng/ml

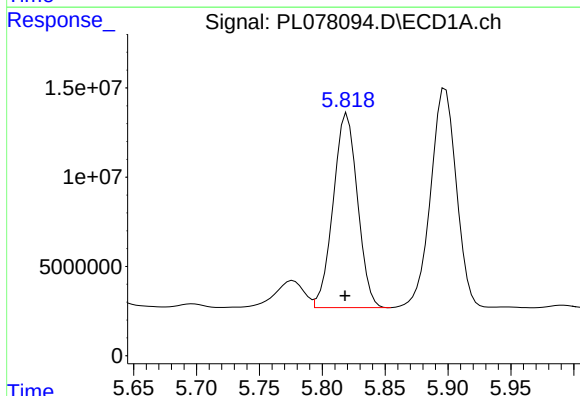


#25 Chlordane-3

R.T.: 5.820 min
Delta R.T.: 0.002 min
Response: 146368885
Conc: 491.77 ng/ml

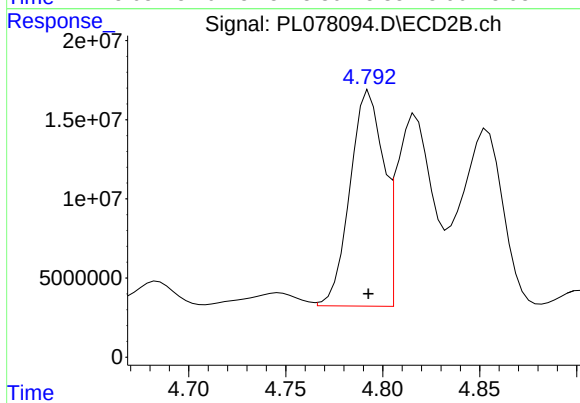

#25 Chlordane-3


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 161743062
Conc: 503.82 ng/ml

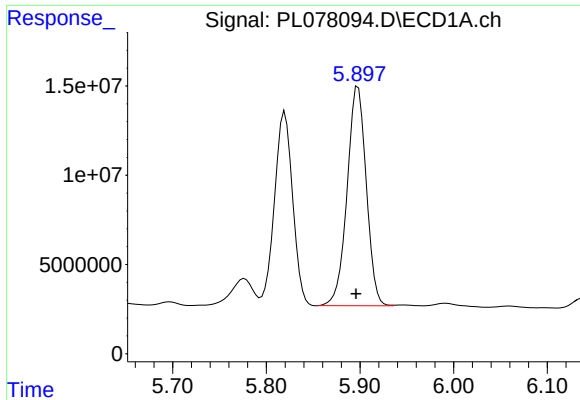

#26 Chlordane-4


R.T.: 5.898 min
Delta R.T.: 0.002 min
Response: 174883599
Conc: 487.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

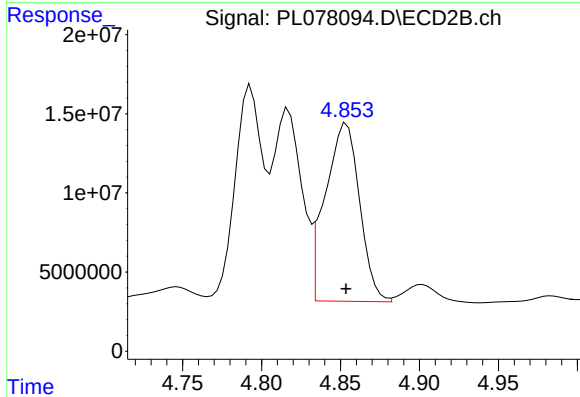


#26 Chlordane-4

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 169960801
Conc: 507.38 ng/ml

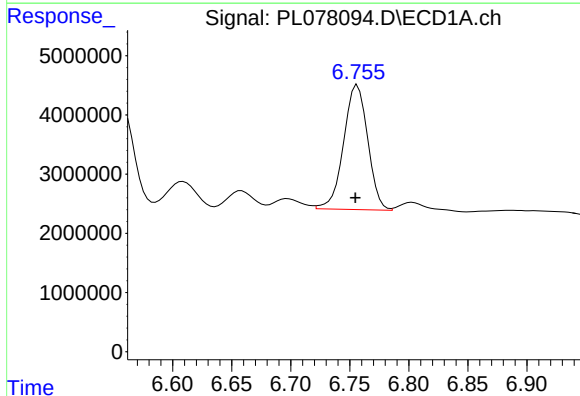


#27 Chlordane-5

R.T.: 6.757 min
Delta R.T.: 0.002 min
Response: 29944873
Conc: 494.53 ng/ml

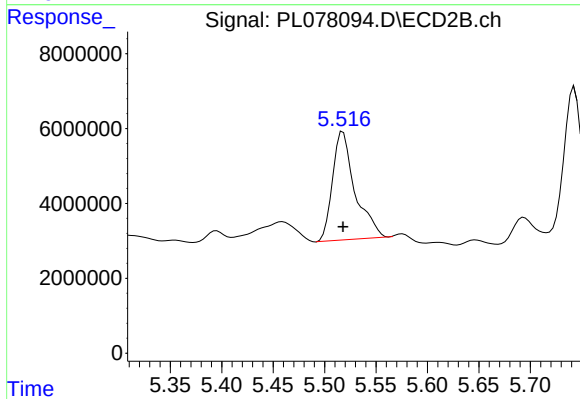

#27 Chlordane-5


R.T.: 5.518 min
Delta R.T.: 0.000 min
Response: 43961625
Conc: 530.66 ng/ml

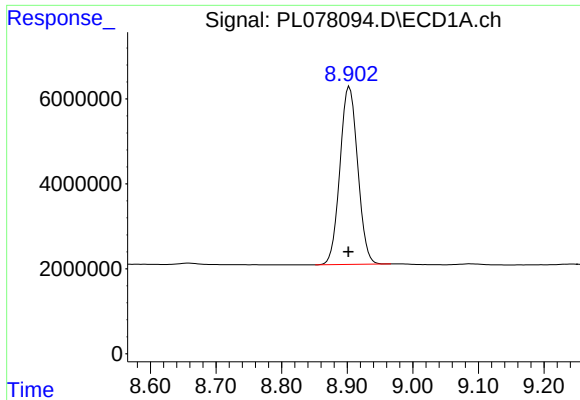

#28 Decachlorobiphenyl

R.T.: 8.903 min
Delta R.T.: 0.002 min
Response: 78718532
Conc: 50.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

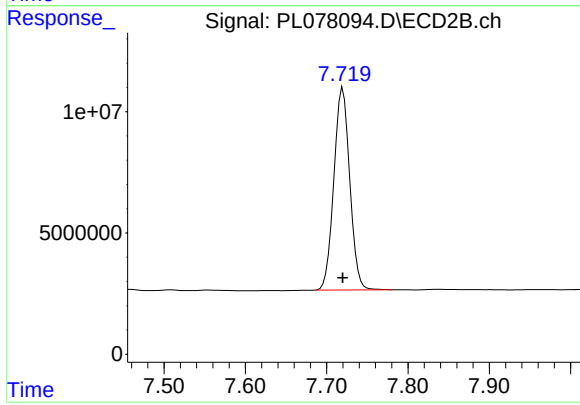

#28 Decachlorobiphenyl

R.T.: 7.720 min
Delta R.T.: 0.000 min
Response: 113259013
Conc: 52.19 ng/ml