

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100423\
 Data File : PL085680.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2023 12:36
 Operator : AR\AJ
 Sample : 04634-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/05/2023
 Supervised By :Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 21:18:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.360	2.624	42209121	15990947	14.192	17.119
2) SA Decachlor...	8.859	7.772	47664527	17600314	21.884m	19.069

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100423\
Data File : PL085680.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2023 12:36
Operator : AR\AJ
Sample : 04634-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/05/2023
Supervised By : Ankita Jodhani 10/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 21:18:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

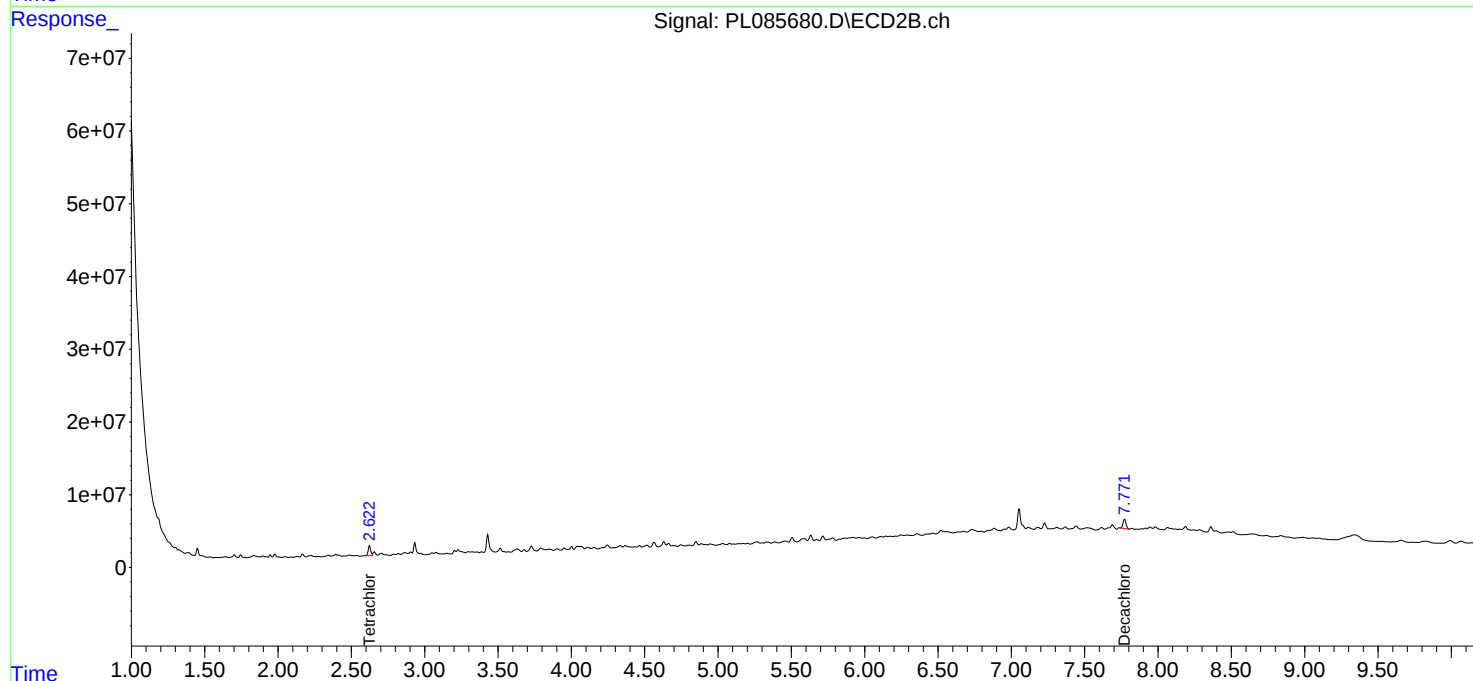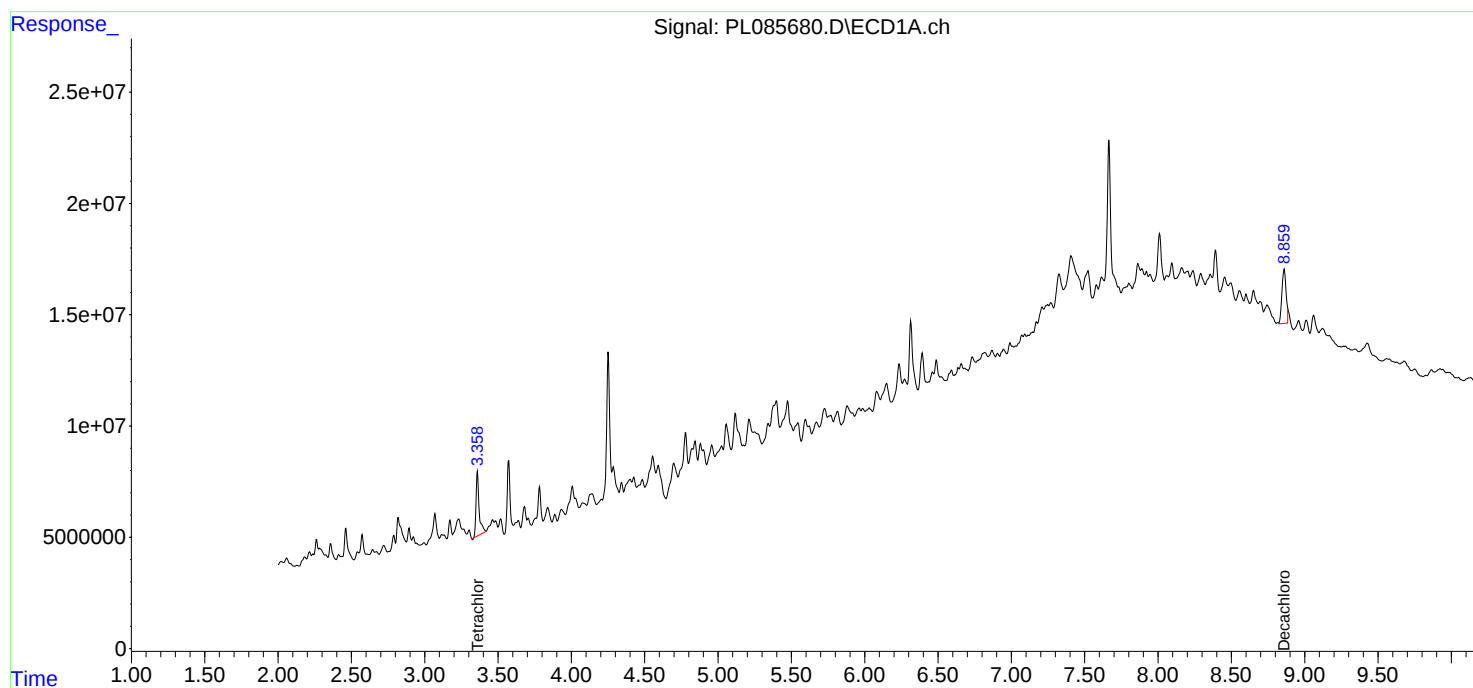

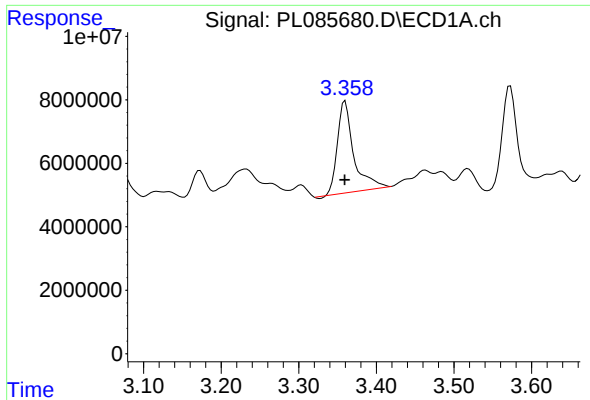


#1 Tetrachloro-m-xylene

R.T.: 3.360 min
Delta R.T.: 0.000 min
Response: 42209121
Conc: 14.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/05/2023
Supervised By :Ankita Jodhani 10/05/2023

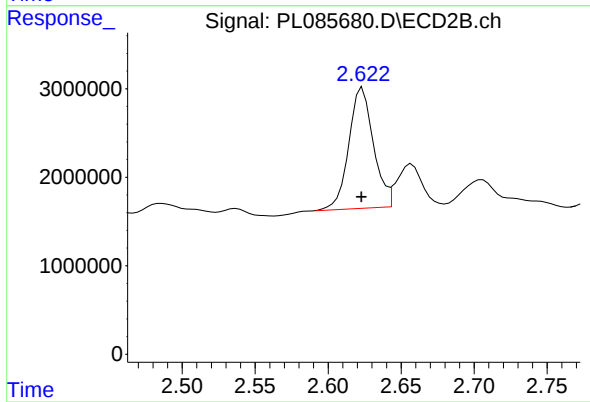


#1 Tetrachloro-m-xylene

R.T.: 2.624 min
Delta R.T.: 0.000 min
Response: 15990947
Conc: 17.12 ng/ml

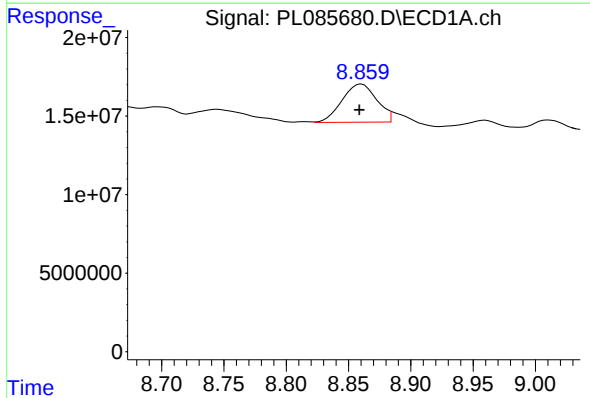

#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 47664527
Conc: 21.88 ng/ml m

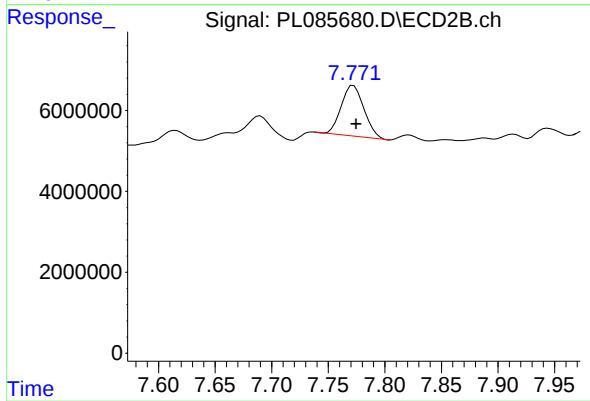

#28 Decachlorobiphenyl

R.T.: 7.772 min
Delta R.T.: -0.002 min
Response: 17600314
Conc: 19.07 ng/ml