

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
 Data File : PL040700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2018 16:43
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 05:21:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 06 04:55:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.804	179.3E6	66707782	19.985	20.322
28)	SA Decachlor...	7.808	8.728	227.3E6	60170904	21.021	21.368
Target Compounds							
16)	A 4,4'-DDD	0.000	6.620f	0	6283959	N.D.	2.282 #
27)	Chlordane-5	5.878	0.000	26941880	0	59.297	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
Data File : PL040700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2018 16:43
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 05:21:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
Quant Title : GC Extractables
QLast Update : Sat Oct 06 04:55:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

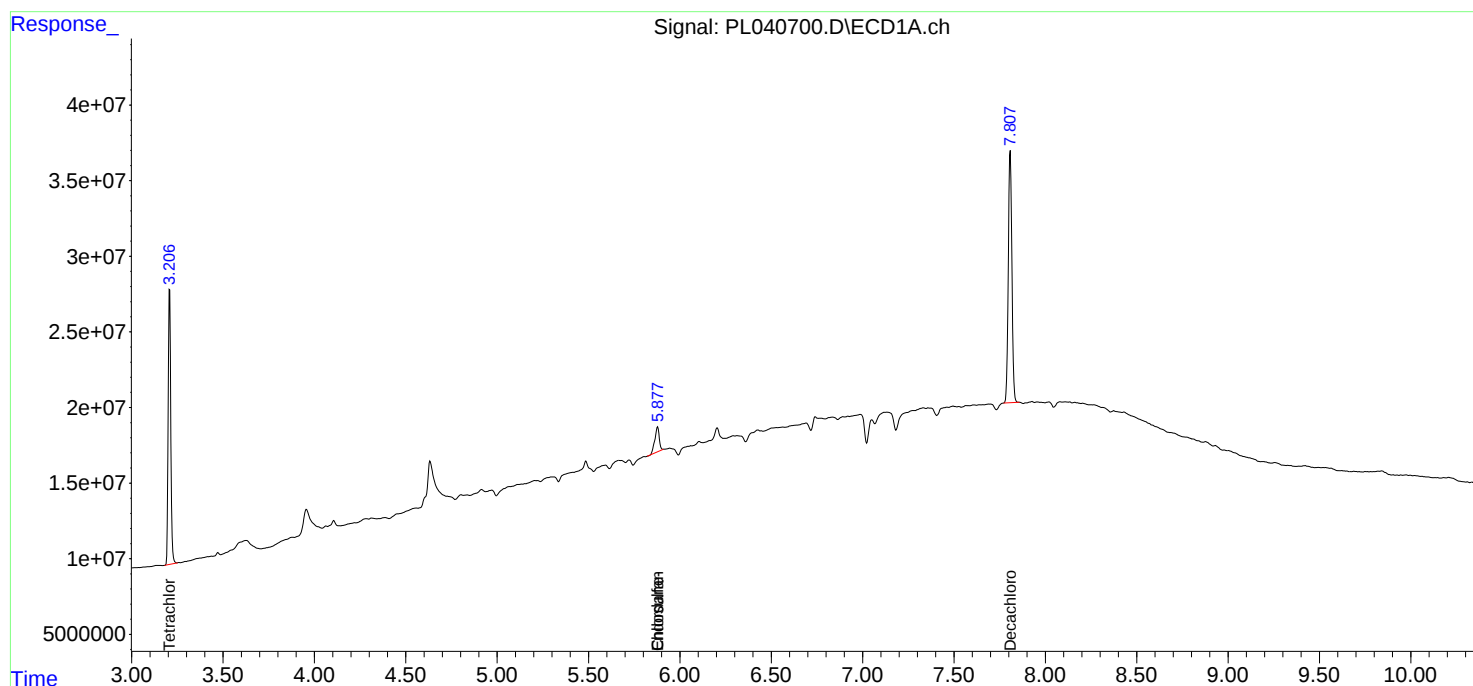


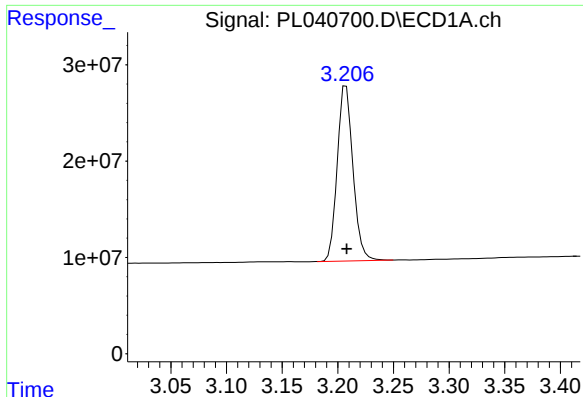

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 179297244
Conc: 19.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

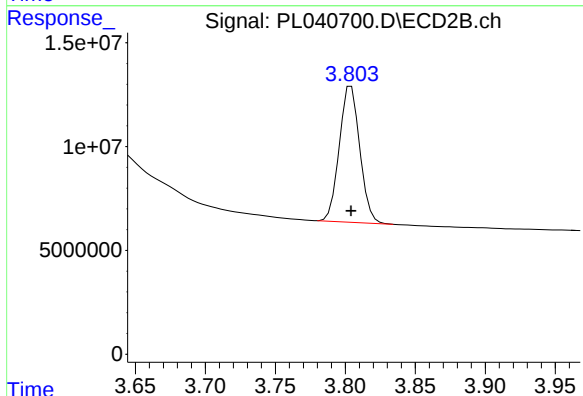


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 66707782
Conc: 20.32 ng/ml

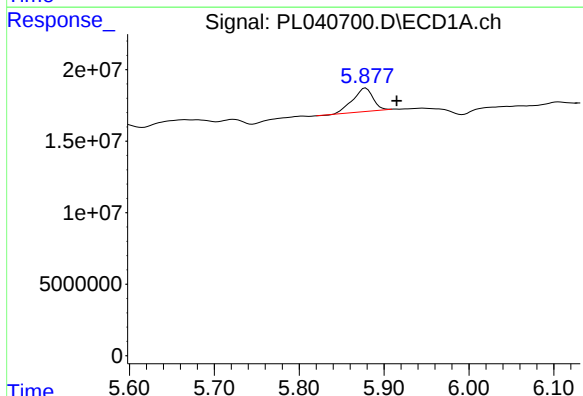


#15 Endosulfan II

R.T.: 5.878 min
Delta R.T.: -0.036 min
Response: 26941880
Conc: 2.34 ng/ml

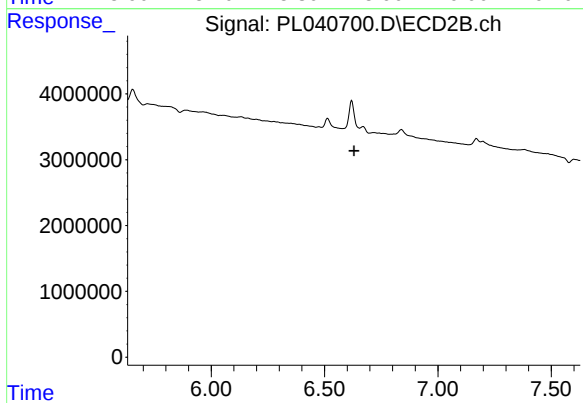

#15 Endosulfan II


R.T.: 6.620 min
Delta R.T.: -0.010 min
Response: 6283959
Conc: N.D.

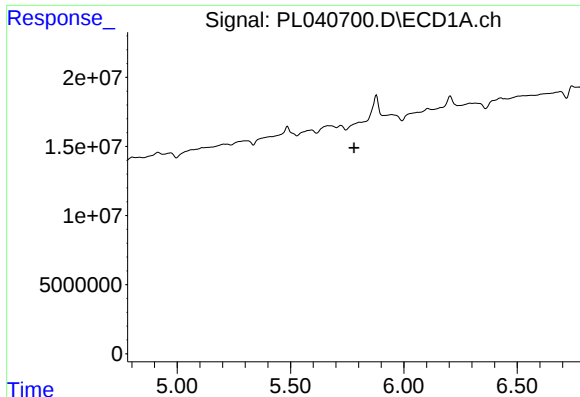

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.781 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

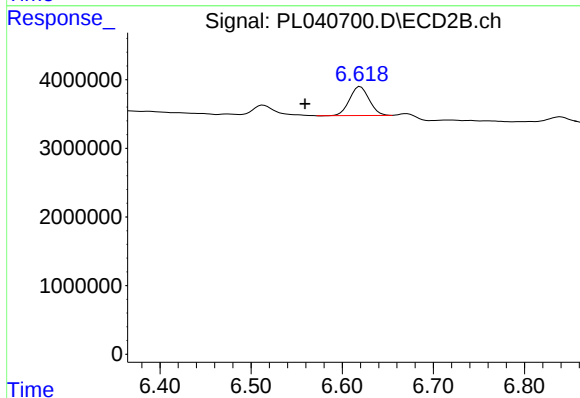


#16 4,4'-DDD

R.T.: 6.620 min
Delta R.T.: 0.061 min
Response: 6283959
Conc: 2.28 ng/ml

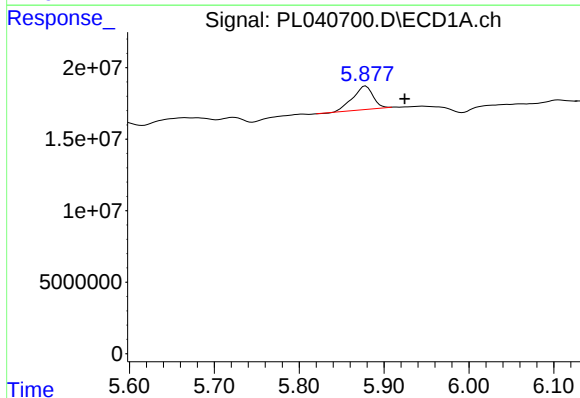


#27 Chlordane-5

R.T.: 5.878 min
Delta R.T.: -0.046 min
Response: 26941880
Conc: 59.30 ng/ml

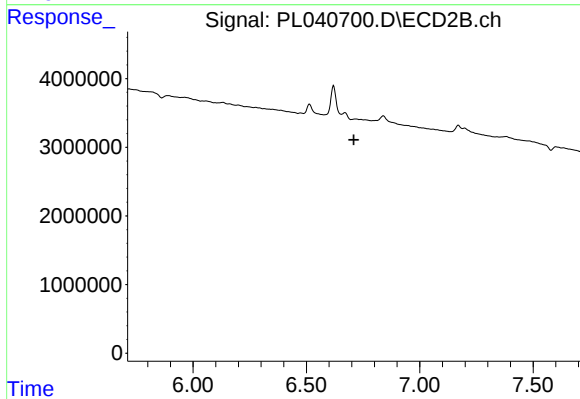

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.710 min
Response: 0
Conc: N.D.

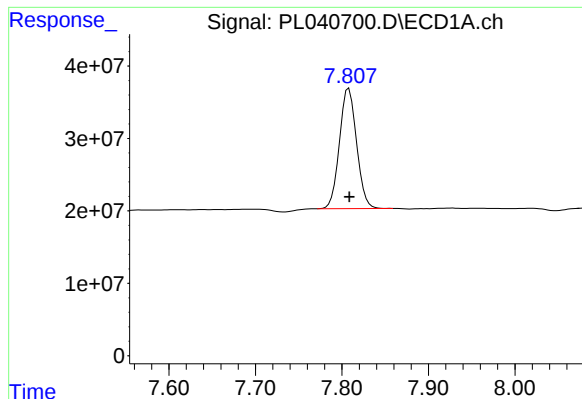

#28 Decachlorobiphenyl

R.T.: 7.808 min
Delta R.T.: 0.000 min
Response: 227323205
Conc: 21.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

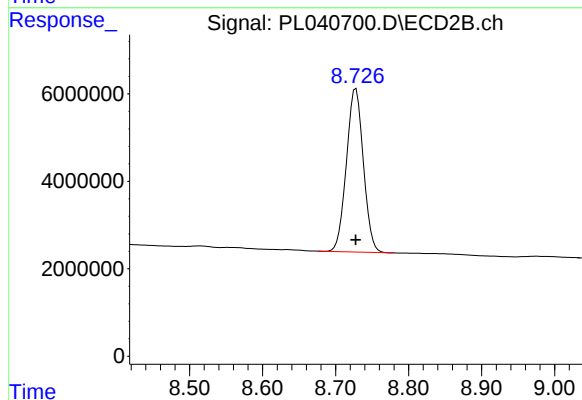

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 60170904
Conc: 21.37 ng/ml