

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
 Data File : PL040721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2018 22:26
 Operator : AJ\SJ
 Sample : PB113575BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 05:24:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
 Quant Title : GC Extractables
 QLast Update : Sat Oct 06 04:55:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.805	166.1E6	63088713	18.510	19.219
28)	SA Decachlor...	7.807	8.728	219.7E6	60841317	20.318	21.606
Target Compounds							
20)	A Methoxychlor	6.508f	0.000	86226048	0	15.436	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
Data File : PL040721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2018 22:26
Operator : AJ\SJ
Sample : PB113575BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 05:24:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
Quant Title : GC Extractables
QLast Update : Sat Oct 06 04:55:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

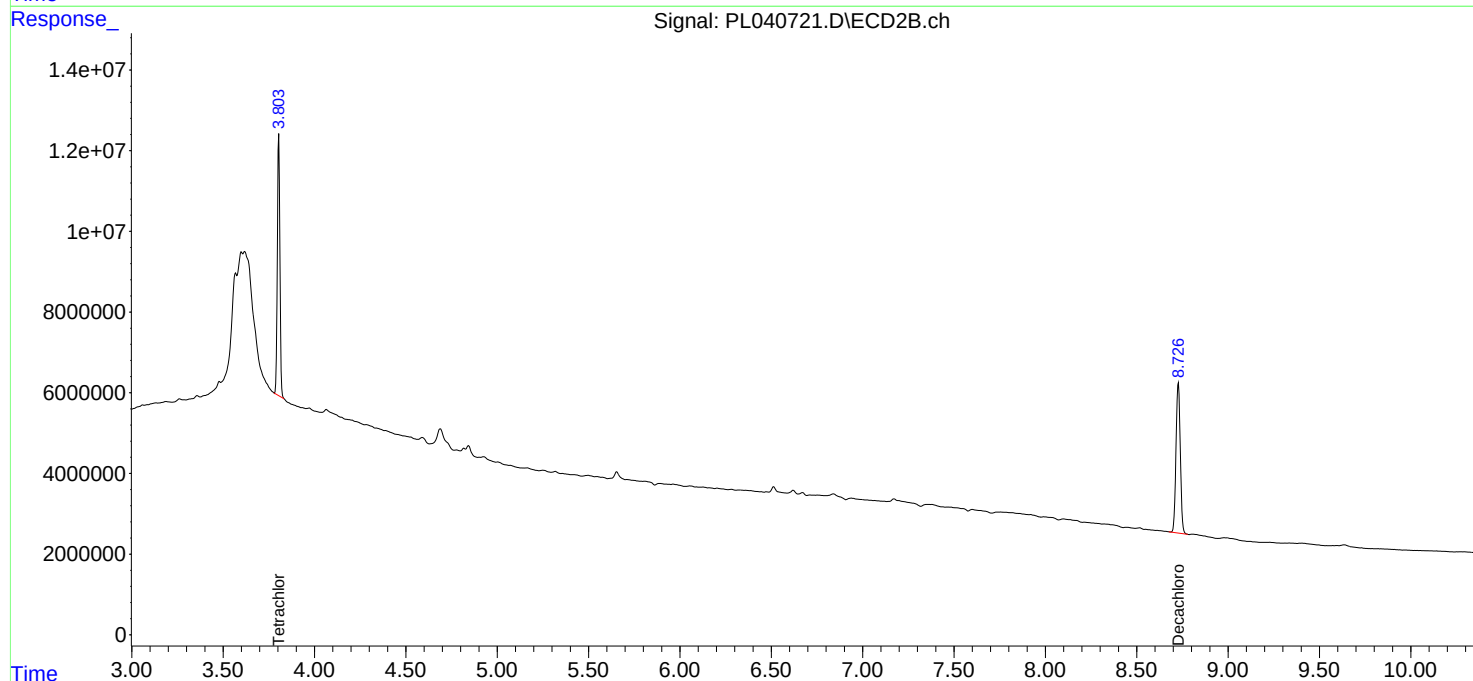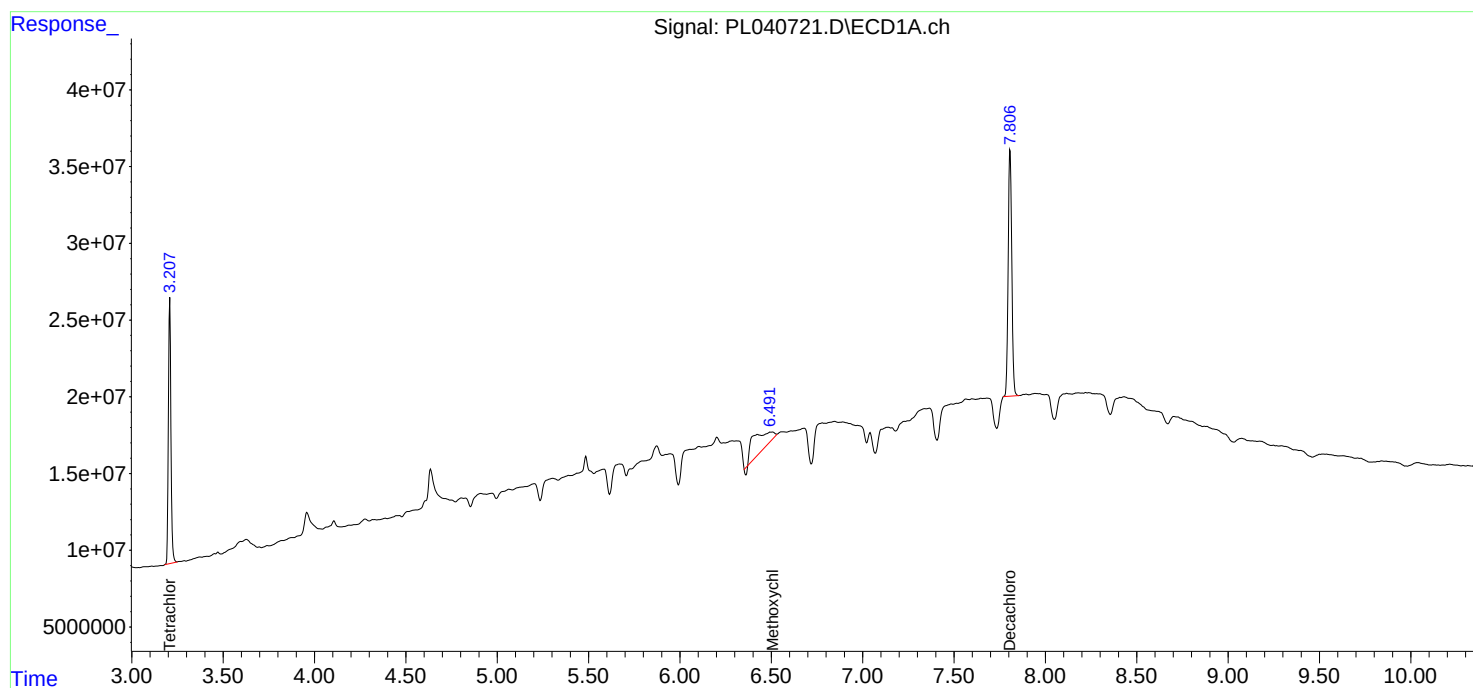


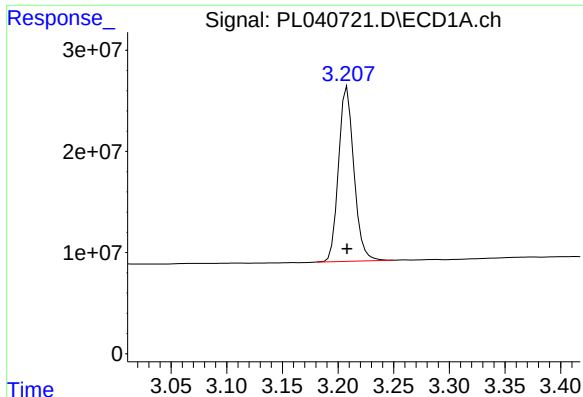

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 166062475
Conc: 18.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

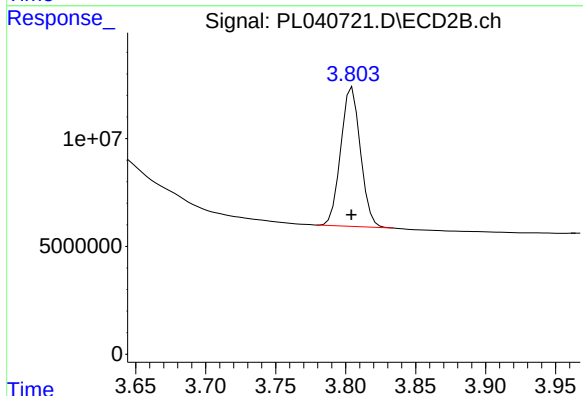


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 63088713
Conc: 19.22 ng/ml

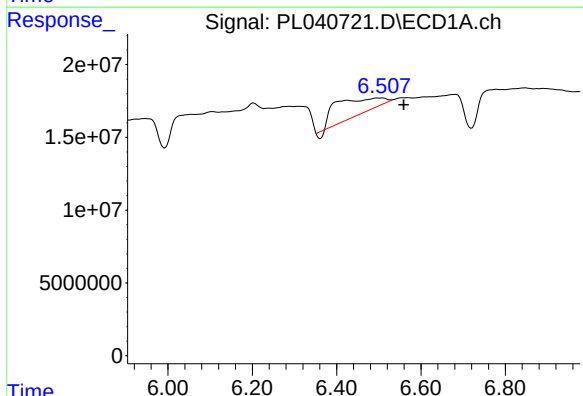


#20 Methoxychlor

R.T.: 6.508 min
Delta R.T.: -0.051 min
Response: 86226048
Conc: 15.44 ng/ml

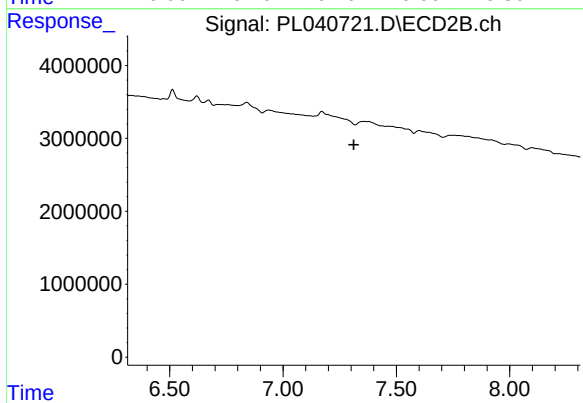

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.312 min
Response: 0
Conc: N.D.

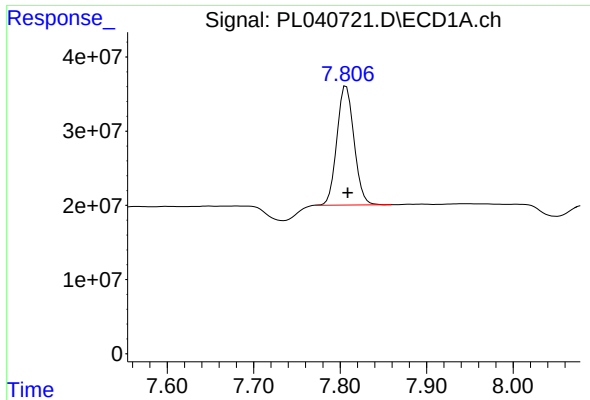

#28 Decachlorobiphenyl

R.T.: 7.807 min
Delta R.T.: -0.001 min
Response: 219717504
Conc: 20.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

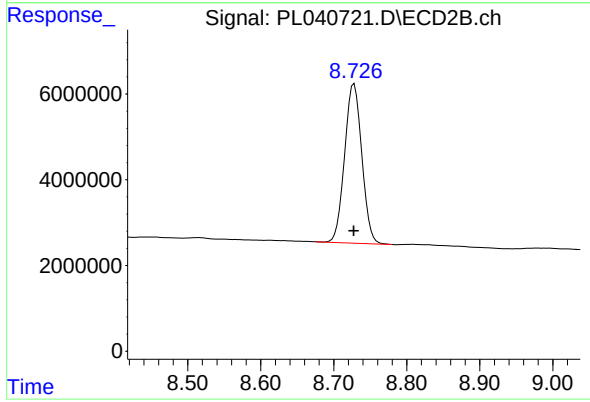

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 60841317
Conc: 21.61 ng/ml