

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
 Data File : PL040687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2018 13:37
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 14:31:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 05 14:19:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.805	888.2E6	315.7E6	97.063	98.362
28)	SA Decachlor...	7.808	8.727	1001.9E6	260.4E6	93.887	93.501
Target Compounds							
23)	Chlordane-1	4.029	4.764	408.3E6	146.4E6	967.346	998.092
24)	Chlordane-2	4.510	5.220	383.4E6	145.1E6	950.732	969.292
25)	Chlordane-3	5.053	5.851	1366.5E6	494.0E6	946.895	992.518
26)	Chlordane-4	5.107	5.925	1339.5E6	581.9E6	965.942	981.251
27)	Chlordane-5	5.917	6.708	457.4E6	111.3E6	967.387	999.667



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
Data File : PL040687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2018 13:37
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 14:31:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
Quant Title : GC Extractables
QLast Update : Fri Oct 05 14:19:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

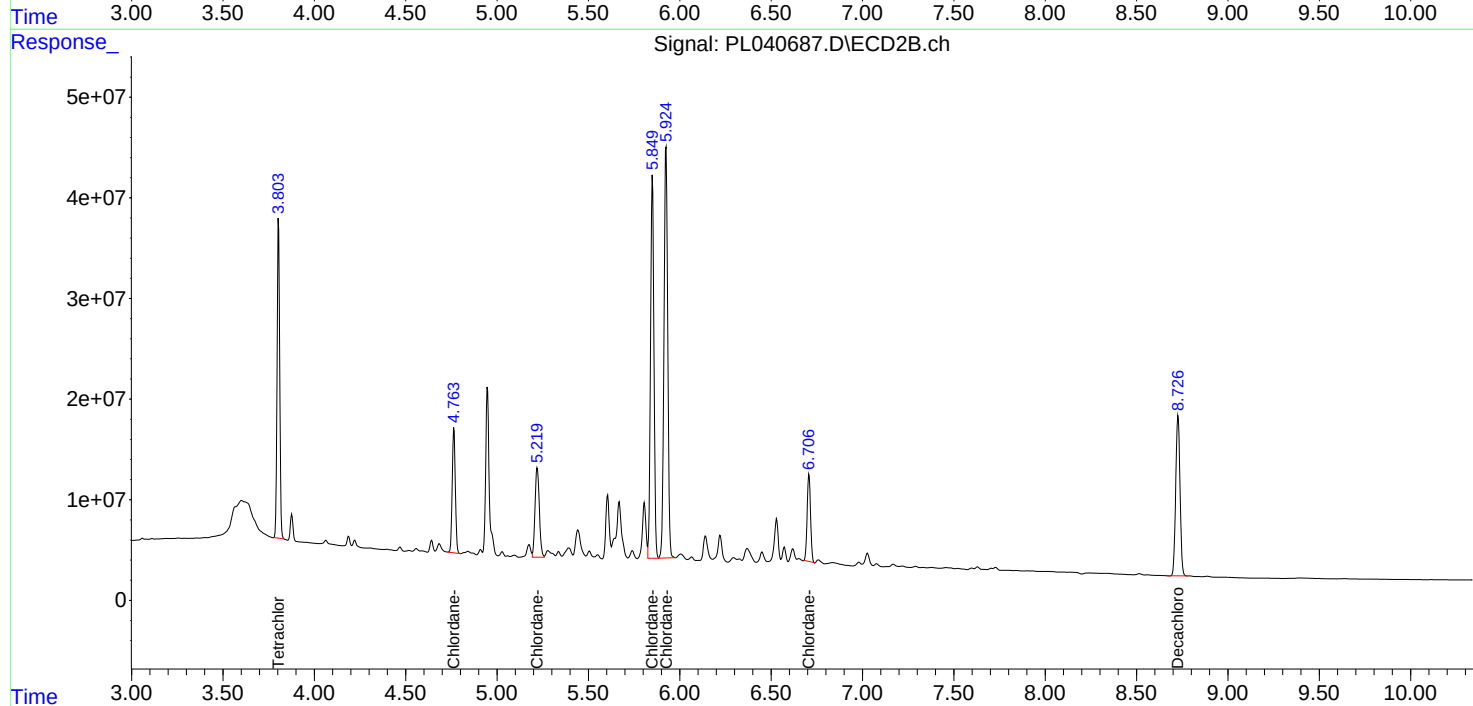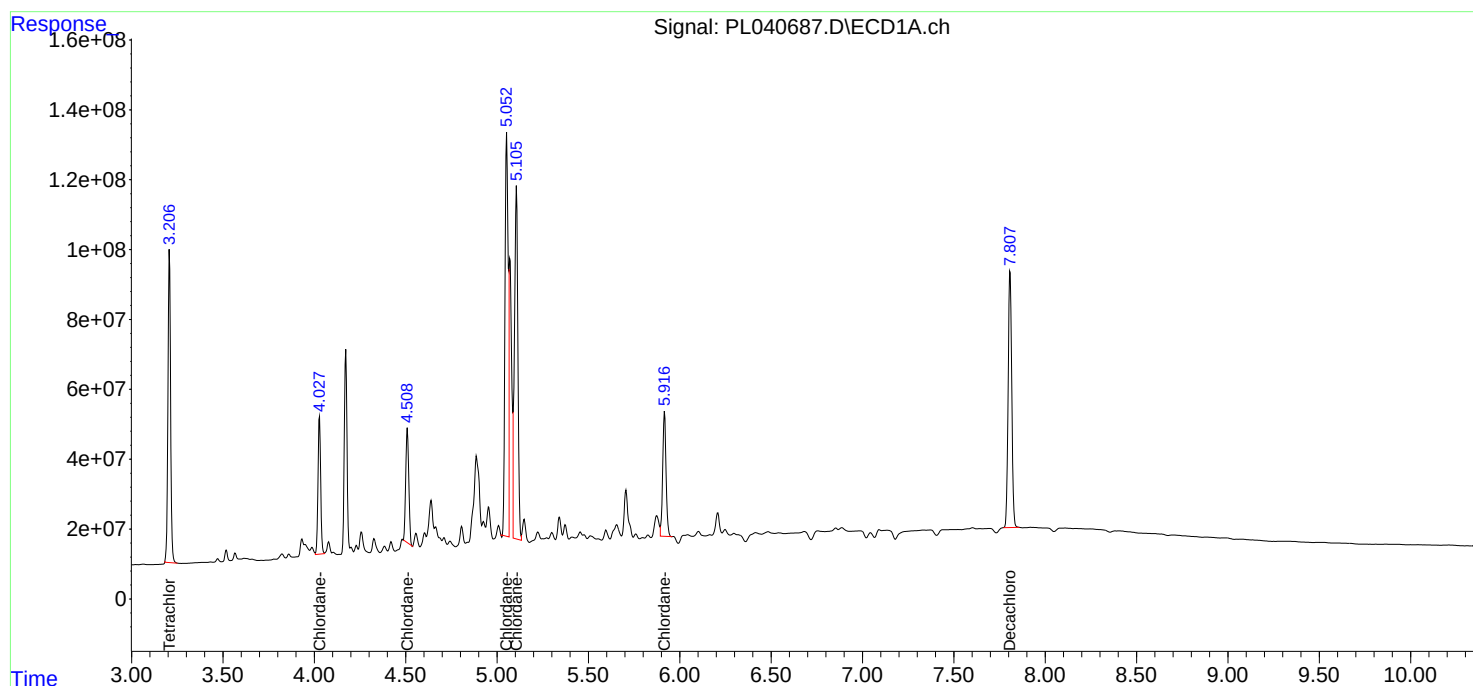


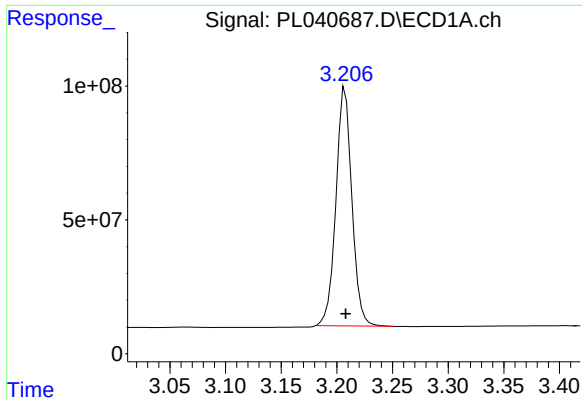

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 888181424
Conc: 97.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

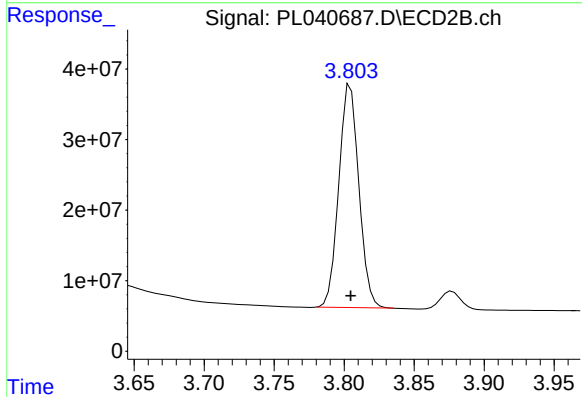


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 315698129
Conc: 98.36 ng/ml

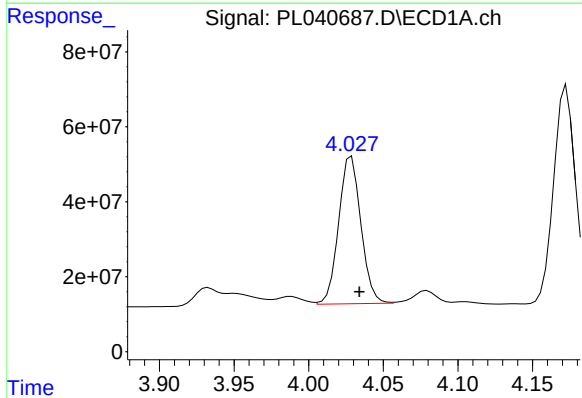


#23 Chlordane-1

R.T.: 4.029 min
Delta R.T.: -0.005 min
Response: 408309936
Conc: 967.35 ng/ml

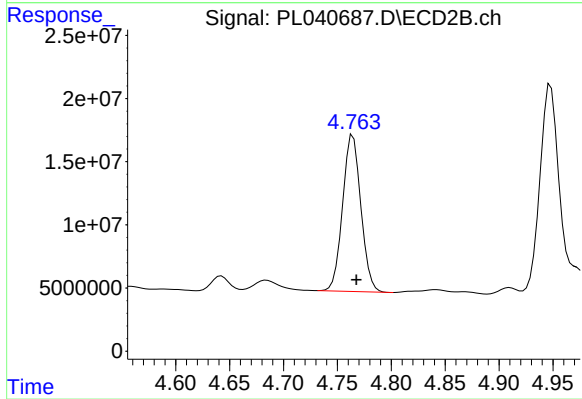

#23 Chlordane-1


R.T.: 4.764 min
Delta R.T.: -0.003 min
Response: 146399127
Conc: 998.09 ng/ml

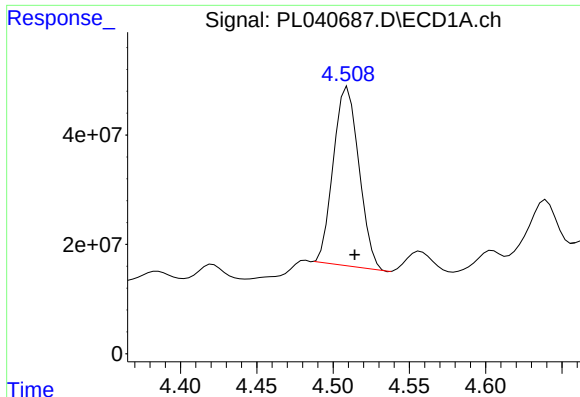

#24 Chlordane-2


R.T.: 4.510 min
Delta R.T.: -0.005 min
Response: 383387978
Conc: 950.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

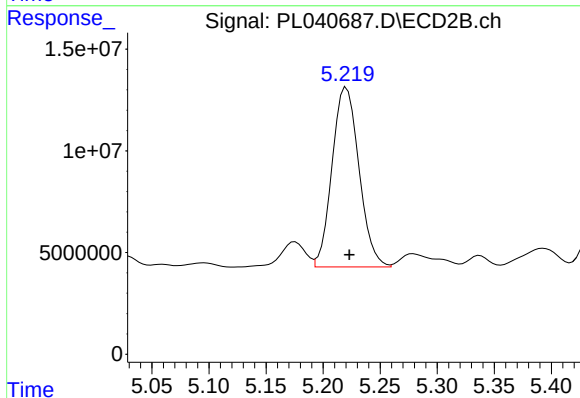


#24 Chlordane-2

R.T.: 5.220 min
Delta R.T.: -0.003 min
Response: 145137792
Conc: 969.29 ng/ml

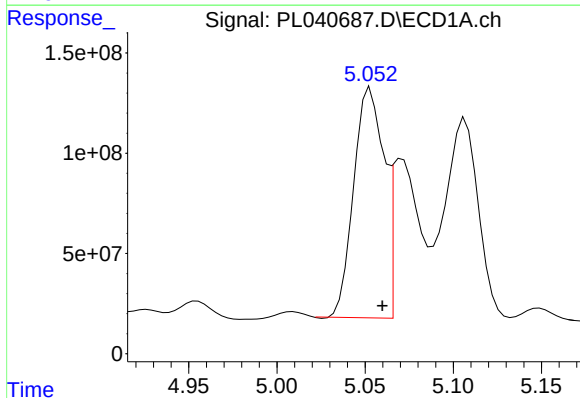


#25 Chlordane-3

R.T.: 5.053 min
Delta R.T.: -0.007 min
Response: 1366516387
Conc: 946.90 ng/ml

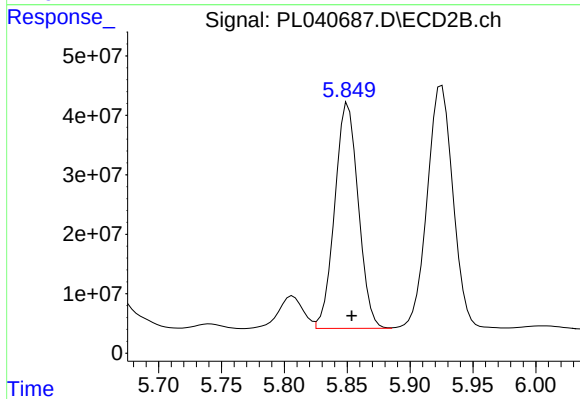

#25 Chlordane-3


R.T.: 5.851 min
Delta R.T.: -0.003 min
Response: 493985847
Conc: 992.52 ng/ml

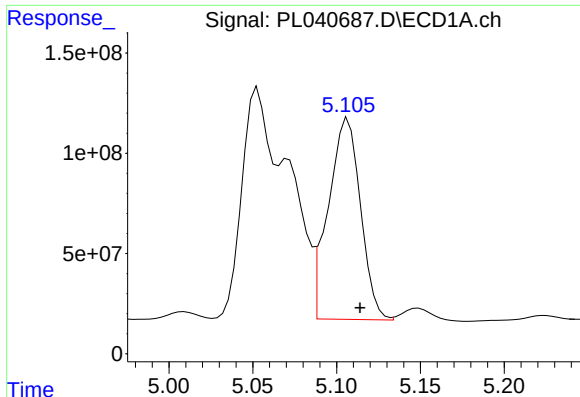

#26 Chlordane-4


R.T.: 5.107 min
Delta R.T.: -0.007 min
Response: 1339482987
Conc: 965.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

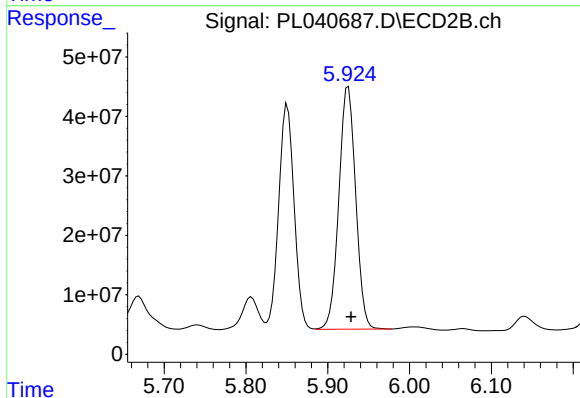


#26 Chlordane-4

R.T.: 5.925 min
Delta R.T.: -0.003 min
Response: 581865317
Conc: 981.25 ng/ml

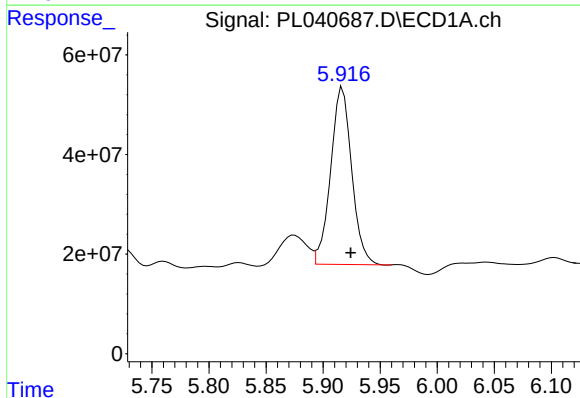


#27 Chlordane-5

R.T.: 5.917 min
Delta R.T.: -0.007 min
Response: 457361511
Conc: 967.39 ng/ml

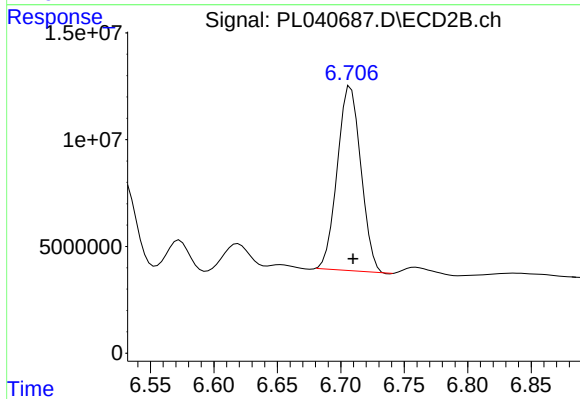

#27 Chlordane-5


R.T.: 6.708 min
Delta R.T.: -0.002 min
Response: 111336857
Conc: 999.67 ng/ml

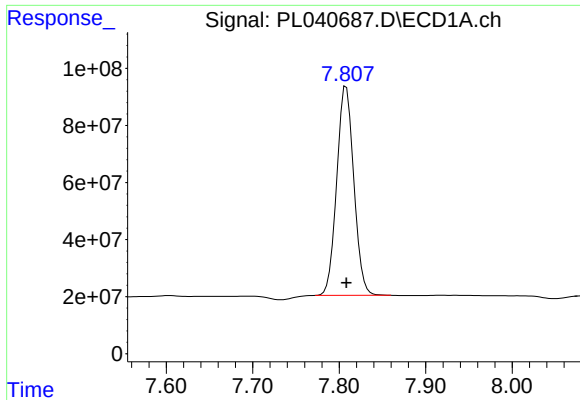

#28 Decachlorobiphenyl

R.T.: 7.808 min
Delta R.T.: 0.000 min
Response: 1001902219
Conc: 93.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

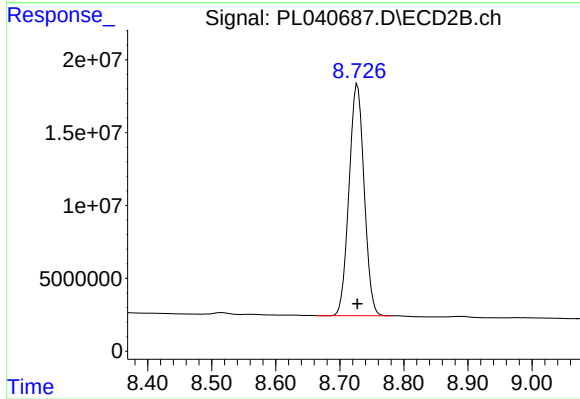

#28 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: 0.000 min
Response: 260426631
Conc: 93.50 ng/ml