

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
 Data File : PL040688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2018 13:51
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Manual Integrations
 APPROVED

Sohil
 10/8/2018 10:52:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 14:31:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 05 14:19:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.804	686.4E6	241.3E6	75.008	75.179
28)	SA Decachlor...	7.808	8.728	780.6E6	203.7E6	73.147	73.118
Target Compounds							
23)	Chlordane-1	4.029	4.764	314.3E6	111.1E6	744.667	757.180
24)	Chlordane-2	4.509	5.220	297.4E6	111.2E6	737.511	742.483
25)	Chlordane-3	5.052	5.850	1122.2E6	377.3E6	777.603m	758.058
26)	Chlordane-4	5.107	5.925	1035.7E6	446.0E6	746.871	752.145
27)	Chlordane-5	5.917	6.707	351.8E6	84822769	744.121	761.604

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
Data File : PL040688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2018 13:51
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
10/8/2018 10:52:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 14:31:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
Quant Title : GC Extractables
QLast Update : Fri Oct 05 14:19:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

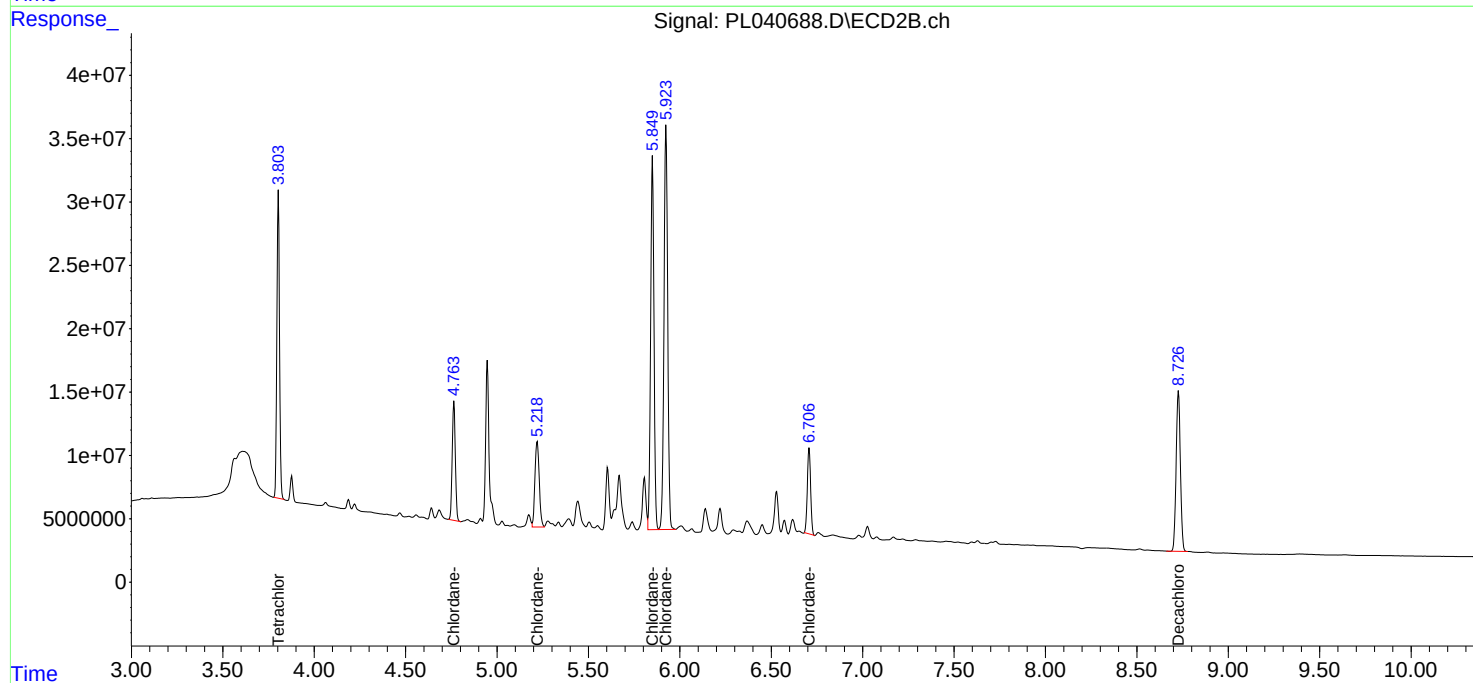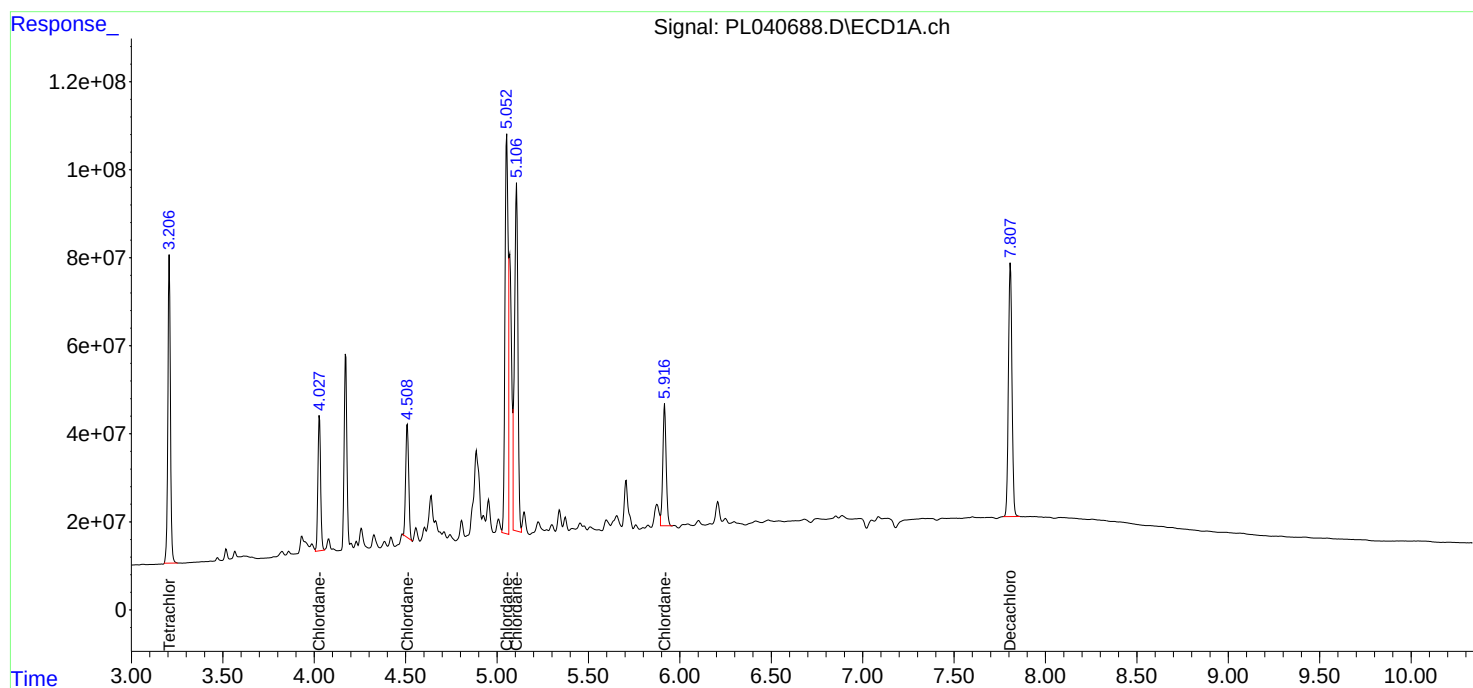

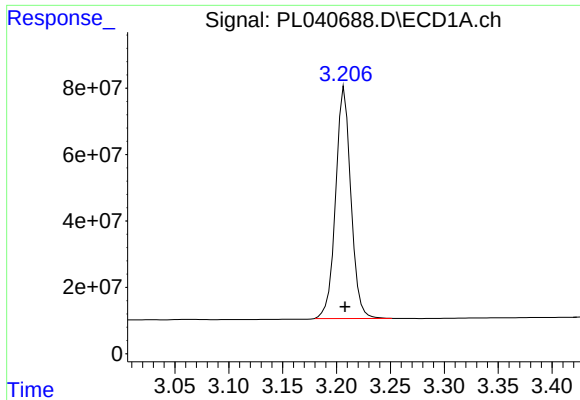


#1 Tetrachloro-m-xylene

R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 686370189
Conc: 75.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
10/8/2018 10:52:47 AM

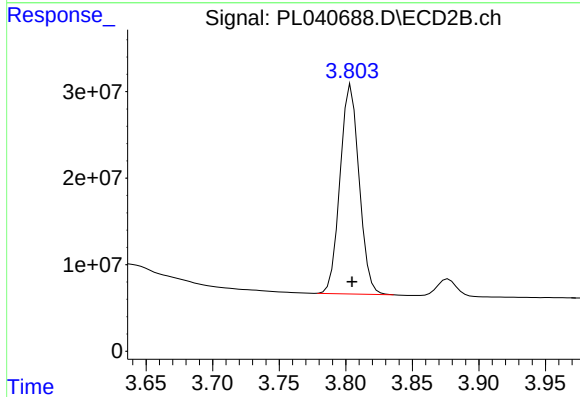


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 241291477
Conc: 75.18 ng/ml

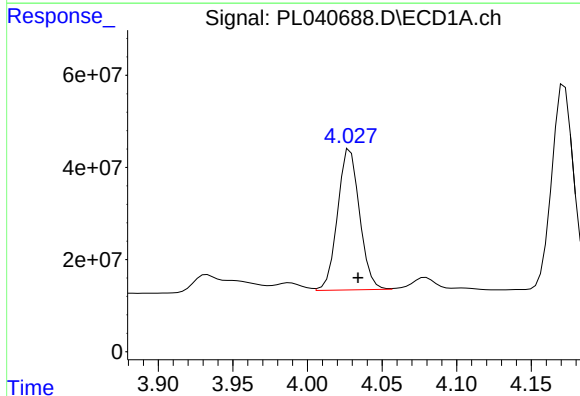


#23 Chlordane-1

R.T.: 4.029 min
Delta R.T.: -0.005 min
Response: 314318634
Conc: 744.67 ng/ml

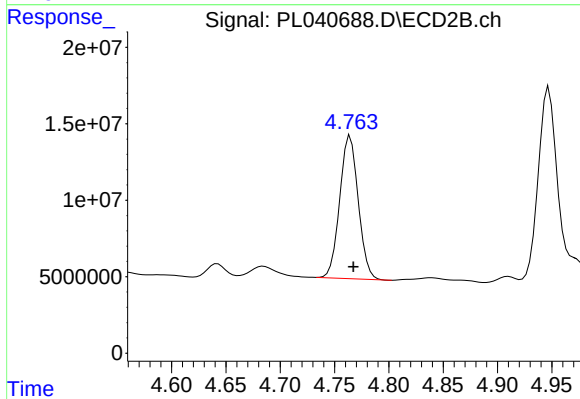

#23 Chlordane-1

R.T.: 4.764 min
Delta R.T.: -0.003 min
Response: 111062372
Conc: 757.18 ng/ml

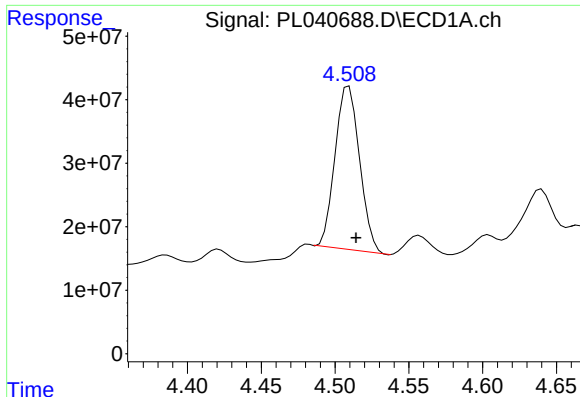


#24 Chlordane-2

R.T.: 4.509 min
Delta R.T.: -0.005 min
Response: 297405311
Conc: 737.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
10/8/2018 10:52:47 AM

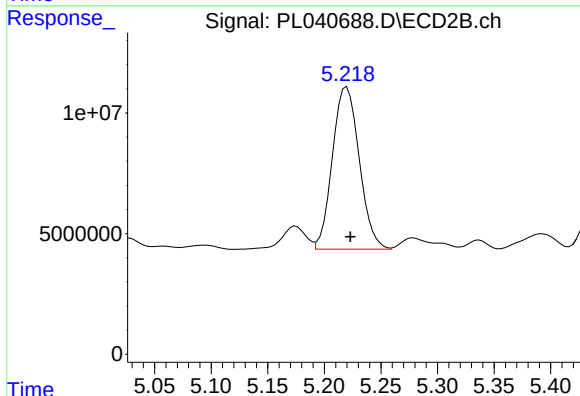


#24 Chlordane-2

R.T.: 5.220 min
Delta R.T.: -0.003 min
Response: 111176431
Conc: 742.48 ng/ml

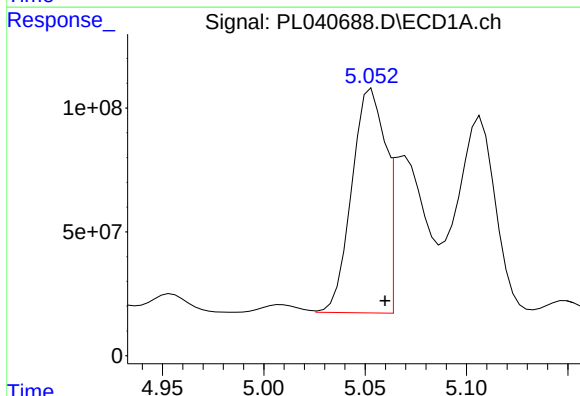


#25 Chlordane-3

R.T.: 5.052 min
Delta R.T.: -0.008 min
Response: 1122200827
Conc: 777.60 ng/ml m

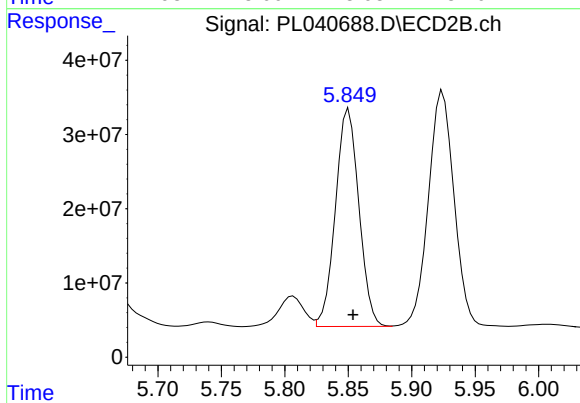

#25 Chlordane-3

R.T.: 5.850 min
Delta R.T.: -0.003 min
Response: 377292977
Conc: 758.06 ng/ml

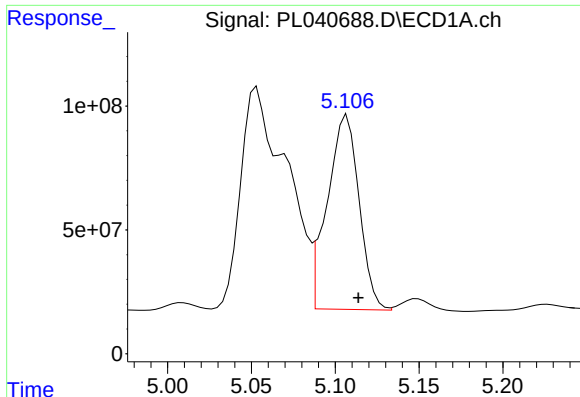


#26 Chlordane-4

R.T.: 5.107 min
Delta R.T.: -0.007 min
Response: 1035694545
Conc: 746.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750


Manual Integrations
APPROVED

Sohil
10/8/2018 10:52:47 AM

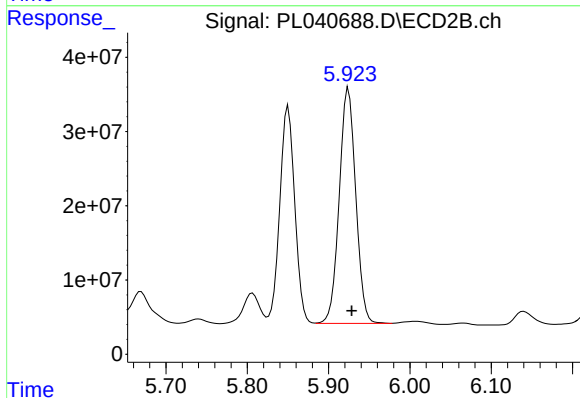


#26 Chlordane-4

R.T.: 5.925 min
Delta R.T.: -0.004 min
Response: 446009466
Conc: 752.14 ng/ml

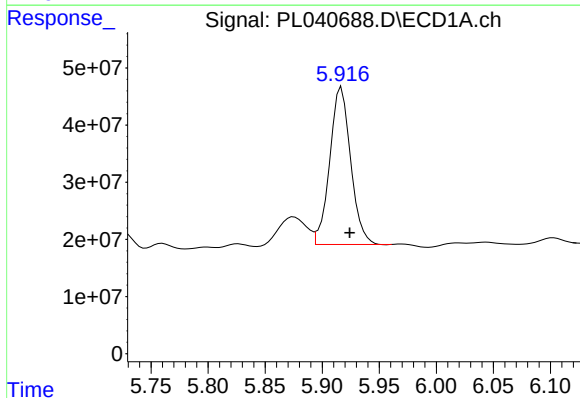


#27 Chlordane-5

R.T.: 5.917 min
Delta R.T.: -0.007 min
Response: 351805468
Conc: 744.12 ng/ml

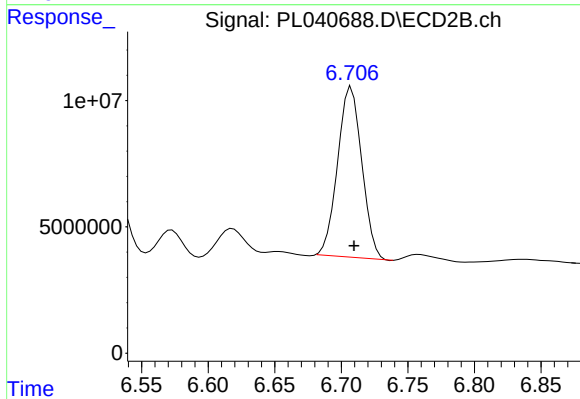

#27 Chlordane-5

R.T.: 6.707 min
Delta R.T.: -0.002 min
Response: 84822769
Conc: 761.60 ng/ml

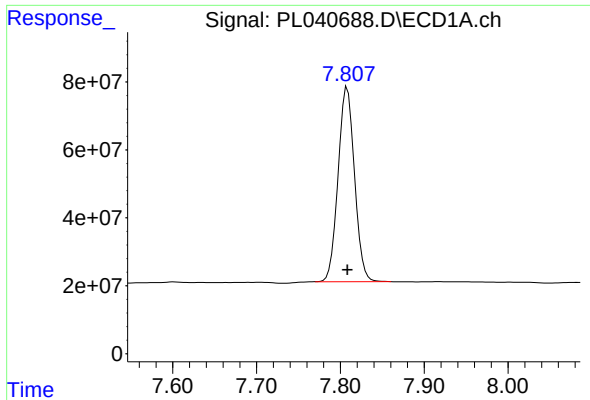


#28 Decachlorobiphenyl

R.T.: 7.808 min
Delta R.T.: 0.000 min
Response: 780577060
Conc: 73.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Manual Integrations
APPROVED

Sohil
10/8/2018 10:52:47 AM

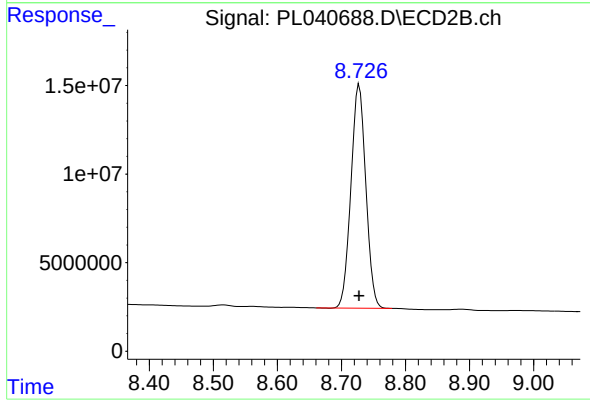

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 203654197
Conc: 73.12 ng/ml