

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
 Data File : PL040690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2018 14:19
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 14:31:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 05 14:19:09 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.804	225.5E6	78964559	24.647	24.603
28)	SA Decachlor...	7.808	8.728	269.7E6	71282717	25.272	25.593
Target Compounds							
23)	Chlordane-1	4.028	4.764	104.6E6	35513027	247.709	242.114
24)	Chlordane-2	4.509	5.220	102.4E6	37851569	253.813	252.789
25)	Chlordane-3	5.053	5.851	360.1E6	119.7E6	249.550	240.414
26)	Chlordane-4	5.106	5.925	338.9E6	144.5E6	244.391	243.685
27)	Chlordane-5	5.917	6.707	117.3E6	26888684	248.149	241.427


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100518\
Data File : PL040690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2018 14:19
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 14:31:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL0100518.M
Quant Title : GC Extractables
QLast Update : Fri Oct 05 14:19:09 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

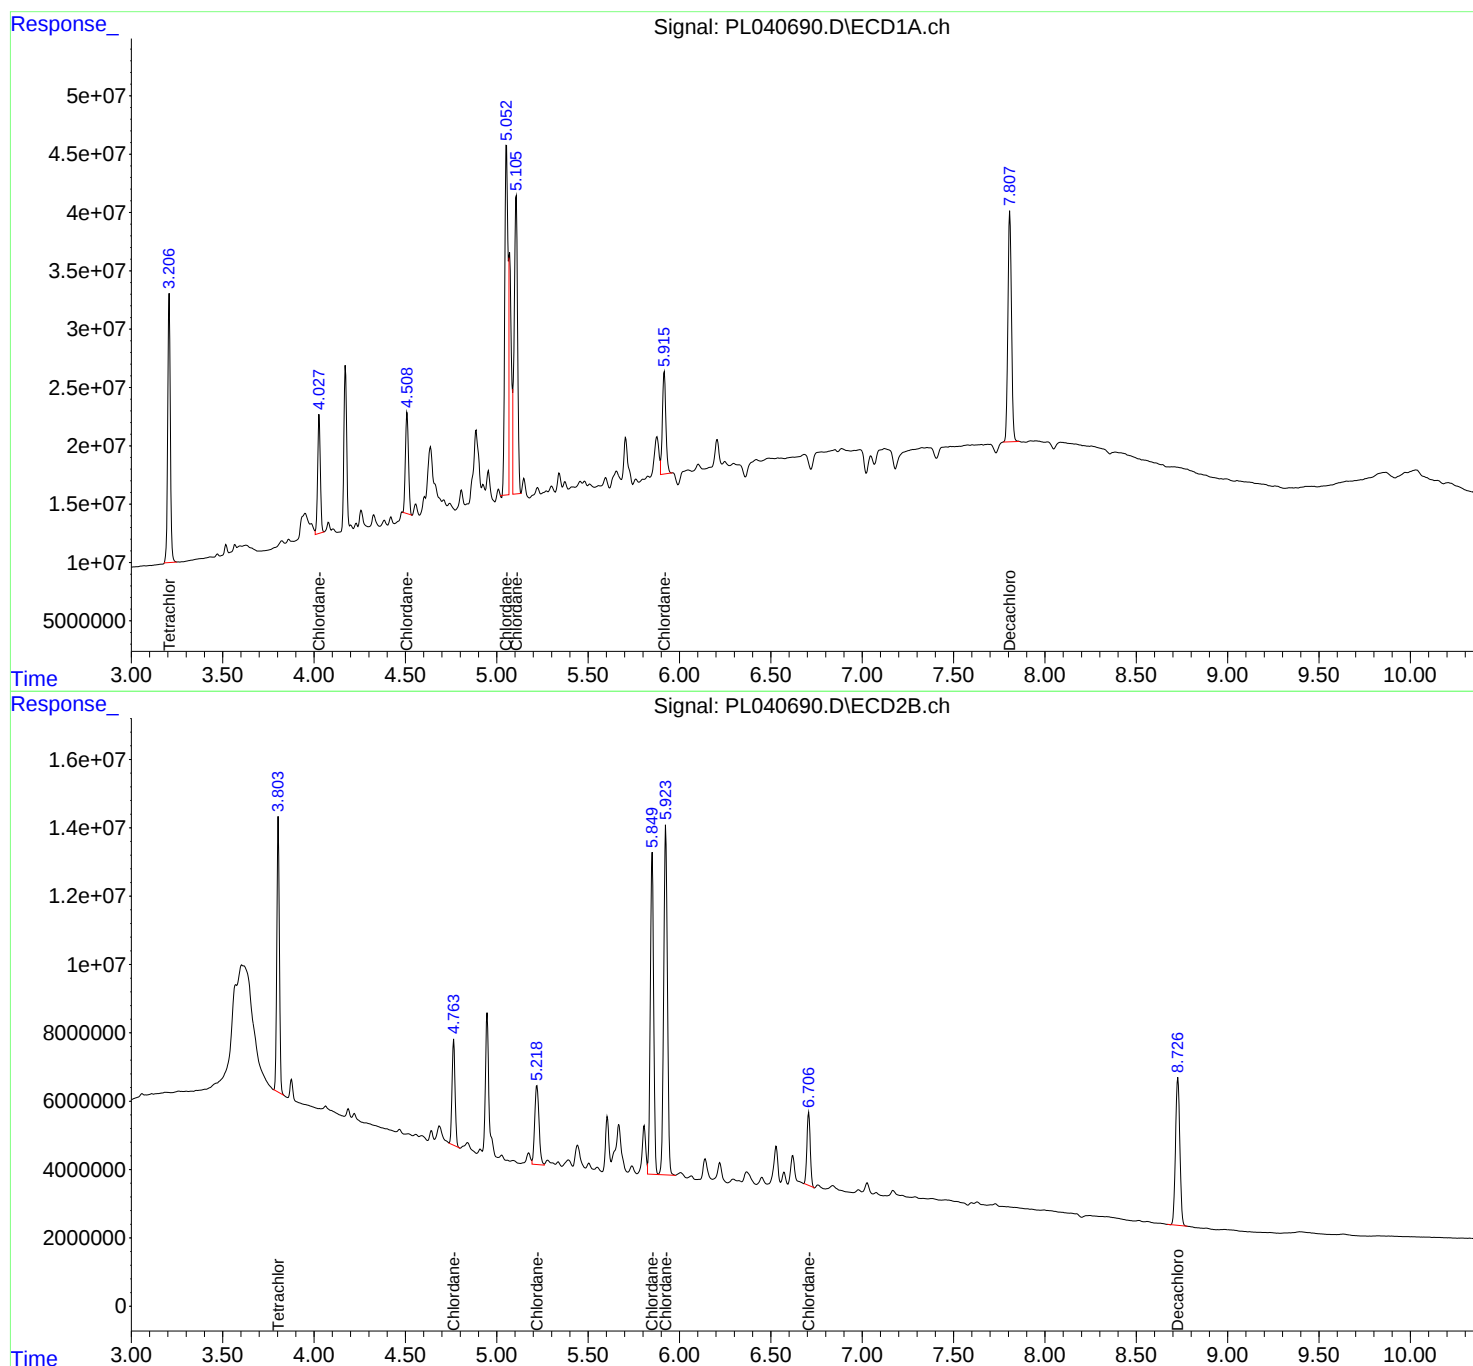


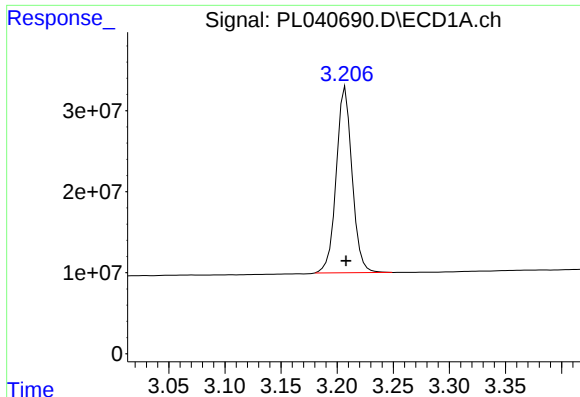

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.000 min
Response: 225534757
Conc: 24.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

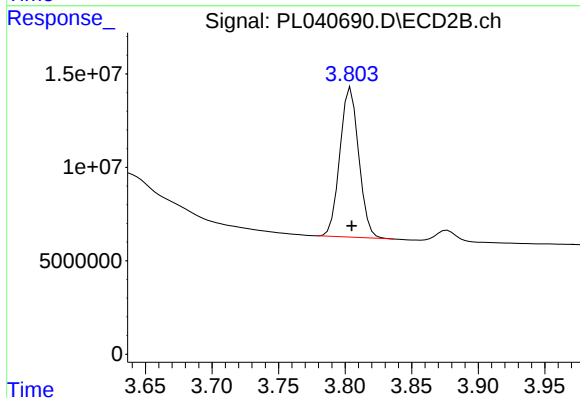


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 78964559
Conc: 24.60 ng/ml

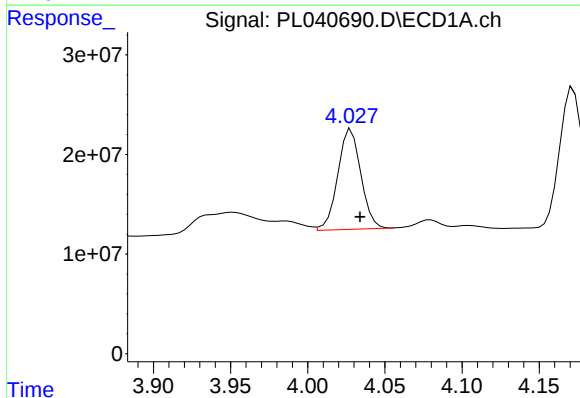


#23 Chlordane-1

R.T.: 4.028 min
Delta R.T.: -0.006 min
Response: 104556413
Conc: 247.71 ng/ml

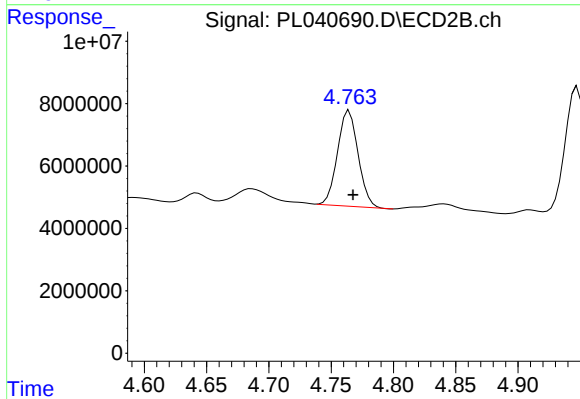

#23 Chlordane-1


R.T.: 4.764 min
Delta R.T.: -0.003 min
Response: 35513027
Conc: 242.11 ng/ml

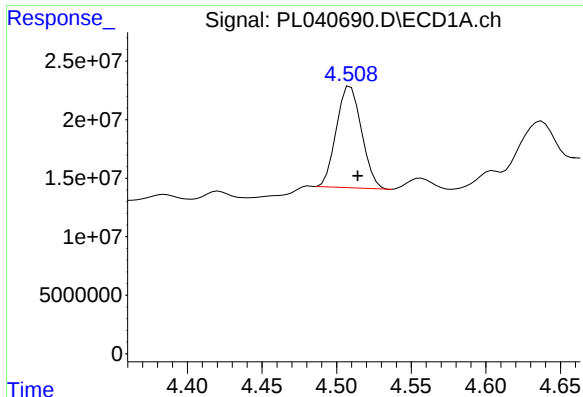

#24 Chlordane-2


R.T.: 4.509 min
Delta R.T.: -0.005 min
Response: 102351273
Conc: 253.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

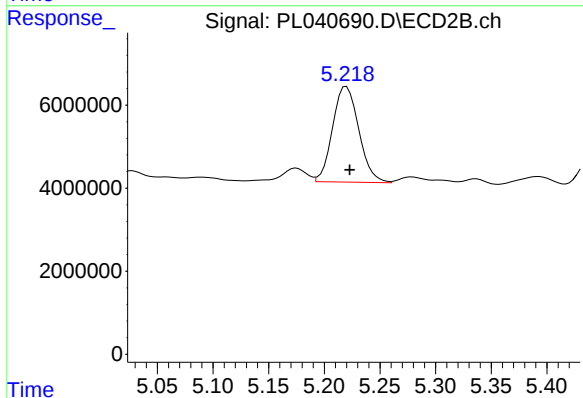


#24 Chlordane-2

R.T.: 5.220 min
Delta R.T.: -0.003 min
Response: 37851569
Conc: 252.79 ng/ml

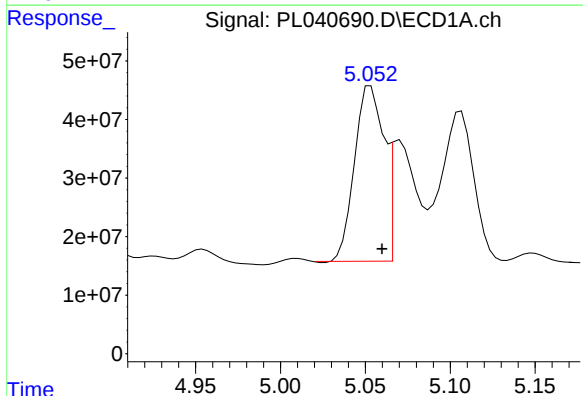


#25 Chlordane-3

R.T.: 5.053 min
Delta R.T.: -0.007 min
Response: 360139048
Conc: 249.55 ng/ml

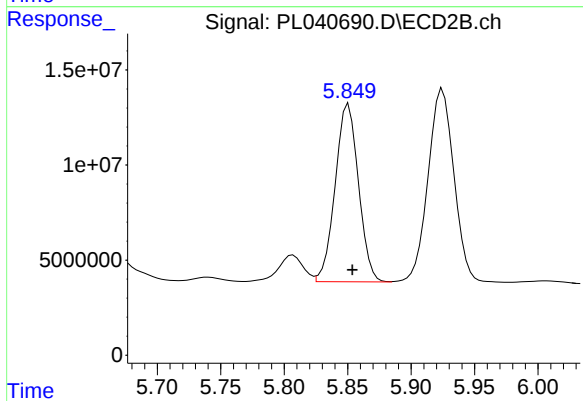

#25 Chlordane-3


R.T.: 5.851 min
Delta R.T.: -0.003 min
Response: 119656633
Conc: 240.41 ng/ml

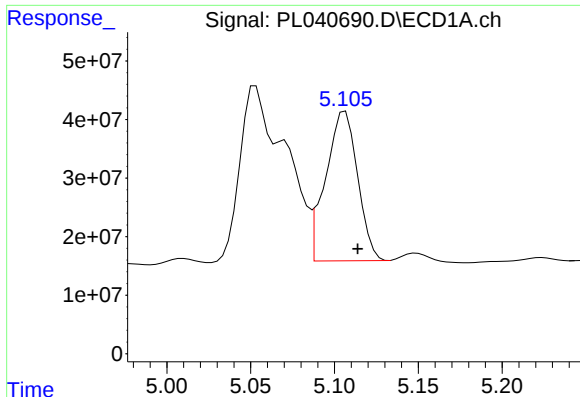

#26 Chlordane-4


R.T.: 5.106 min
Delta R.T.: -0.008 min
Response: 338899344
Conc: 244.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

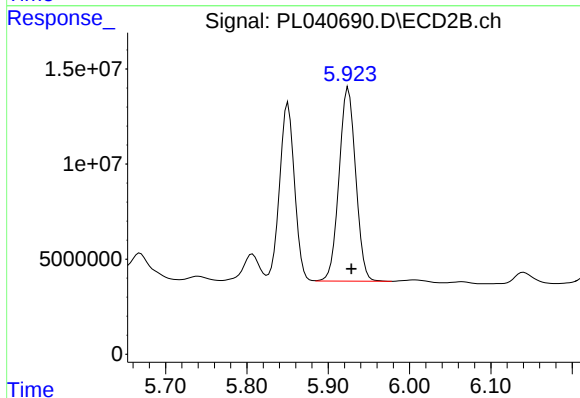


#26 Chlordane-4

R.T.: 5.925 min
Delta R.T.: -0.004 min
Response: 144501410
Conc: 243.69 ng/ml

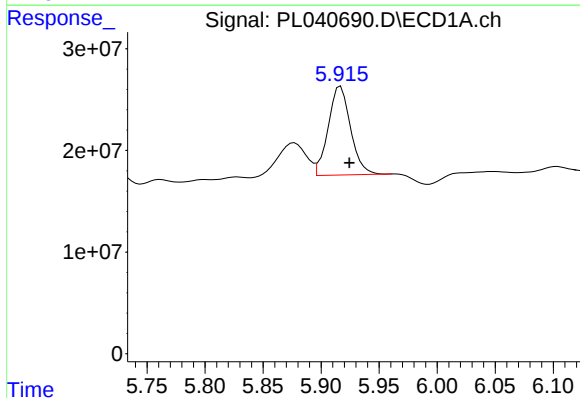


#27 Chlordane-5

R.T.: 5.917 min
Delta R.T.: -0.007 min
Response: 117319945
Conc: 248.15 ng/ml

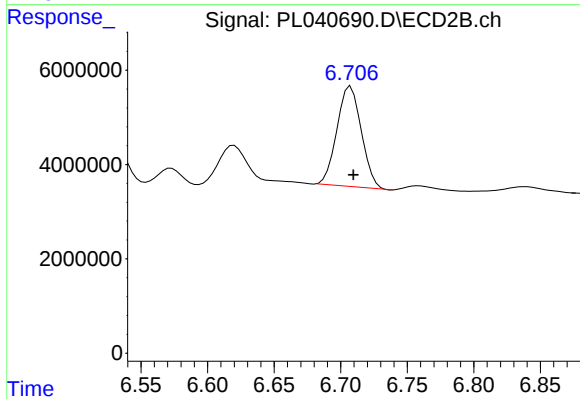

#27 Chlordane-5


R.T.: 6.707 min
Delta R.T.: -0.002 min
Response: 26888684
Conc: 241.43 ng/ml

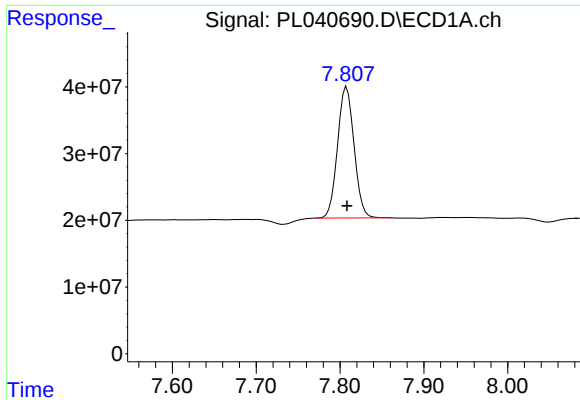

#28 Decachlorobiphenyl

R.T.: 7.808 min
Delta R.T.: 0.000 min
Response: 269692435
Conc: 25.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

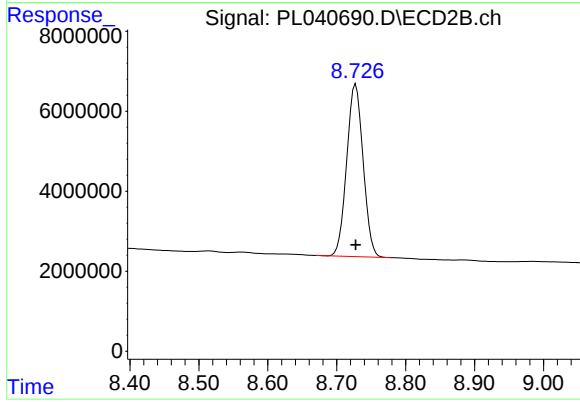

#28 Decachlorobiphenyl

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 71282717
Conc: 25.59 ng/ml