

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
 Data File : PL061996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2020 13:01
 Operator : DD\AJ
 Sample : L4190-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 16:47:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	4.006	37670998	56412917	22.082	20.677
28)	SA Decachlor...	8.209	9.094	31611170	42635216	19.432	19.368
Target Compounds							
9)	A Endosulfan I	5.530f	0.000	3917242	0	2.417	N.D. #
15)	B Endosulfa...	0.000	6.943	0	14191433	N.D.	5.491 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
Data File : PL061996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2020 13:01
Operator : DD\AJ
Sample : L4190-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 16:47:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

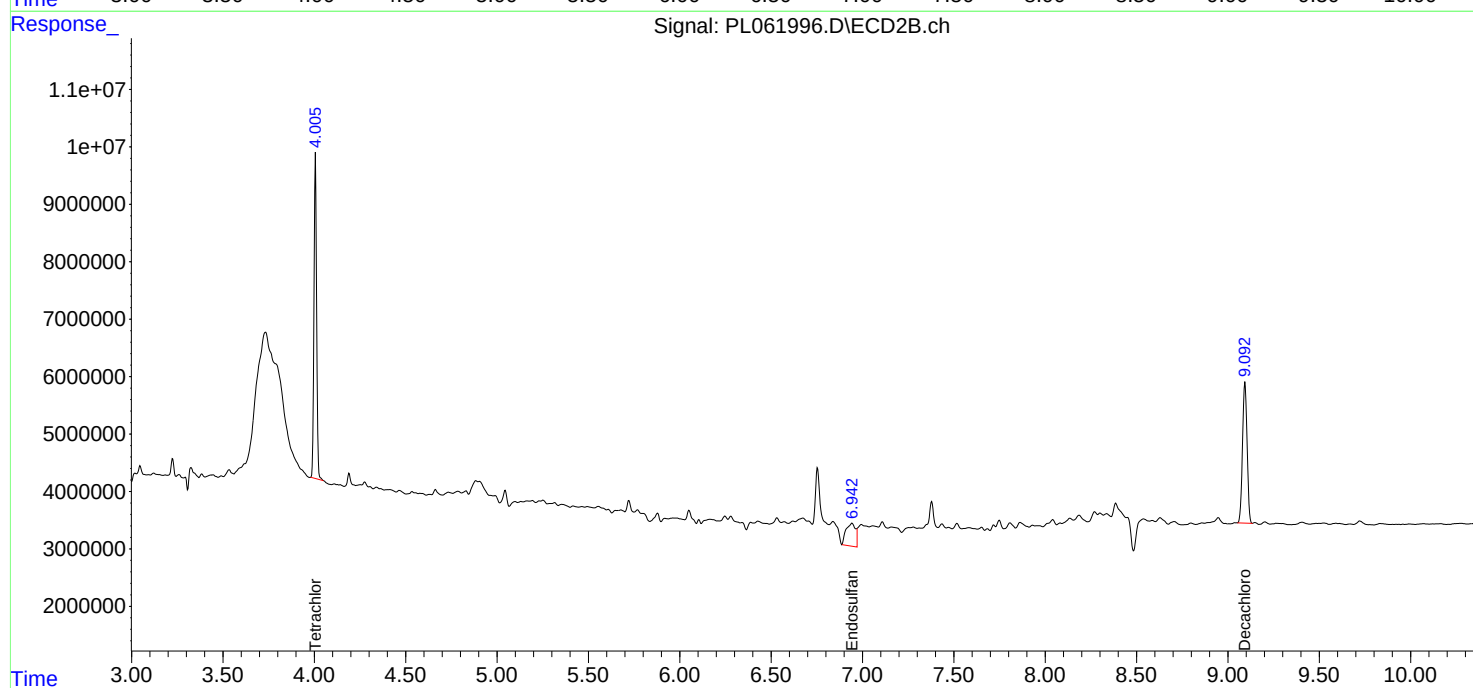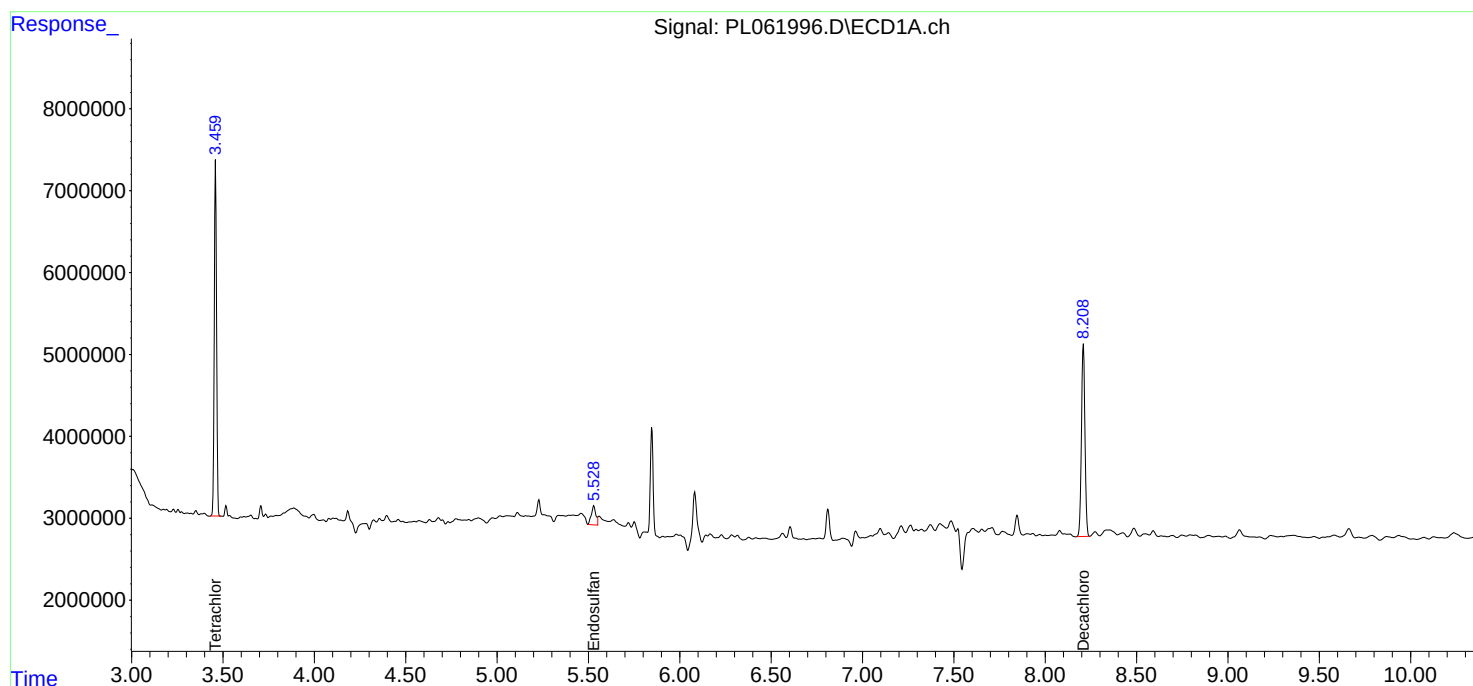


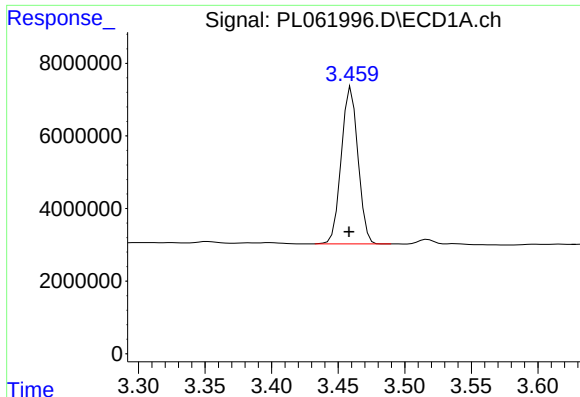

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.002 min
Response: 37670998
Conc: 22.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

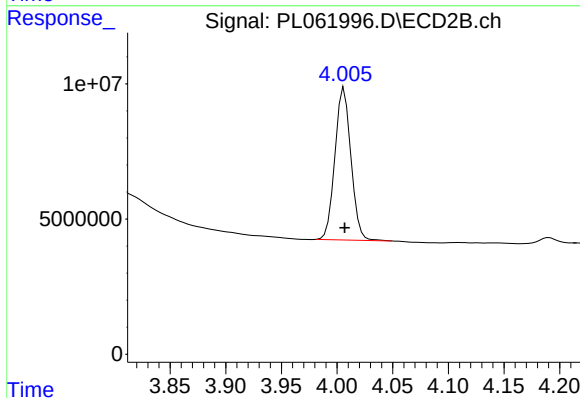


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 56412917
Conc: 20.68 ng/ml

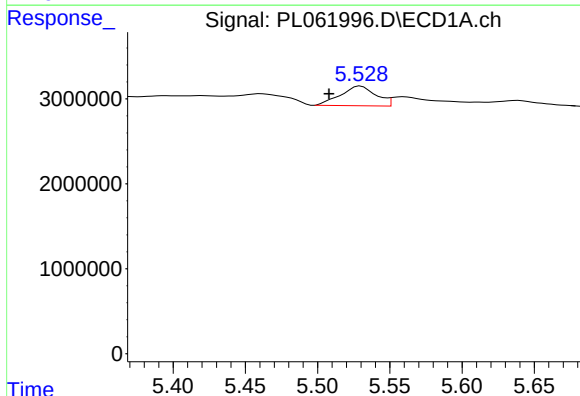


#9 Endosulfan I

R.T.: 5.530 min
Delta R.T.: 0.022 min
Response: 3917242
Conc: 2.42 ng/ml

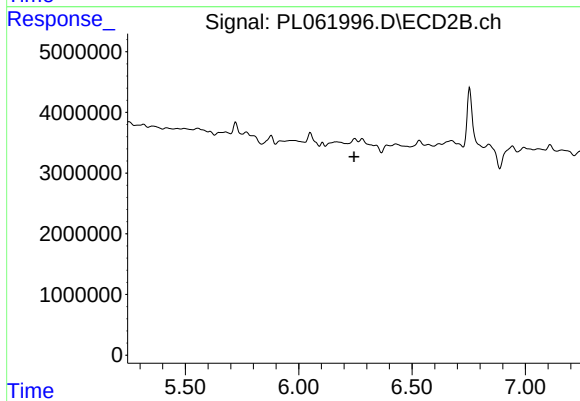

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.245 min
Response: 0
Conc: N.D.

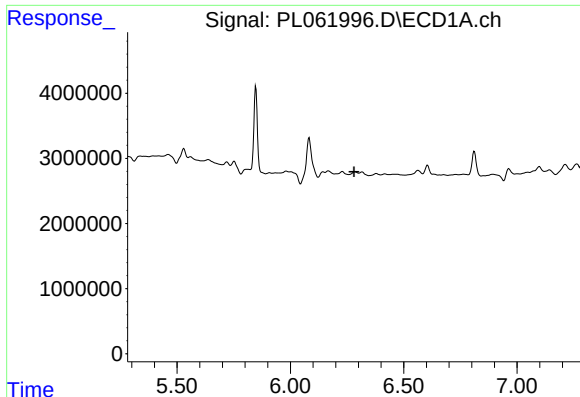

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

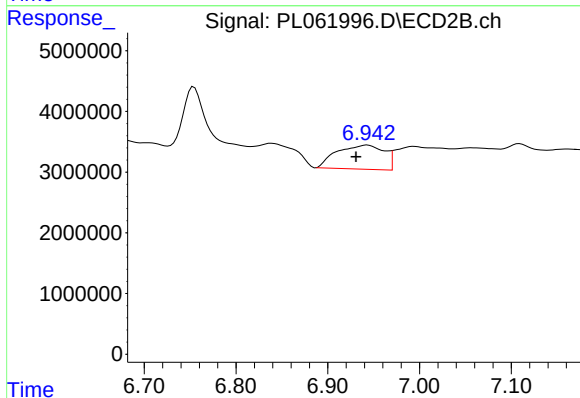


#15 Endosulfan II

R.T.: 6.943 min
Delta R.T.: 0.012 min
Response: 14191433
Conc: 5.49 ng/ml

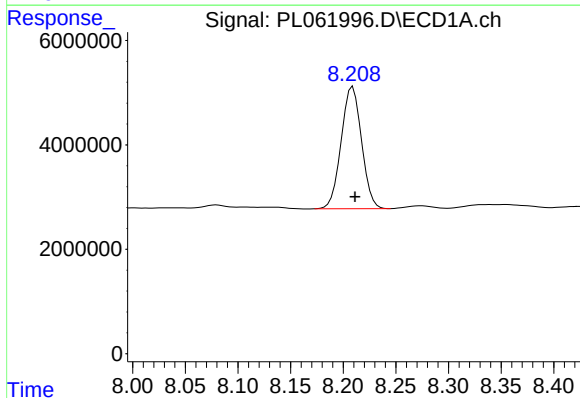

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 31611170
Conc: 19.43 ng/ml

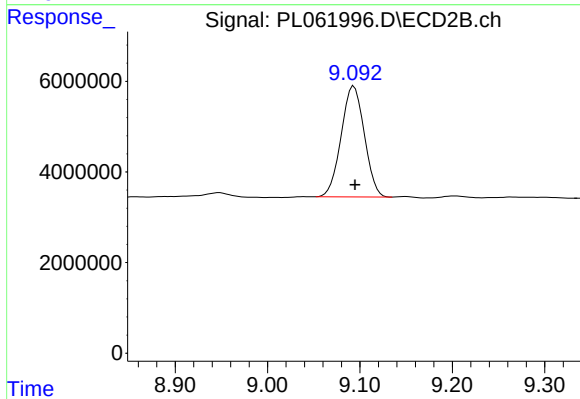

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: -0.001 min
Response: 42635216
Conc: 19.37 ng/ml