

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
 Data File : PL062021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2020 19:12
 Operator : DD\AJ
 Sample : L4226-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-100120

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 00:58:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	35153182	54763049	20.606	20.073
28)	SA Decachlor...	8.208	9.091	35505515	49766373	21.826	22.607
Target Compounds							
7)	B delta-BHC	0.000	5.047f	0	2722516	N.D.	1.068 #
22)	Mirex	7.356f	0.000	3447409	0	2.459	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
Data File : PL062021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2020 19:12
Operator : DD\AJ
Sample : L4226-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-05-100120

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 00:58:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

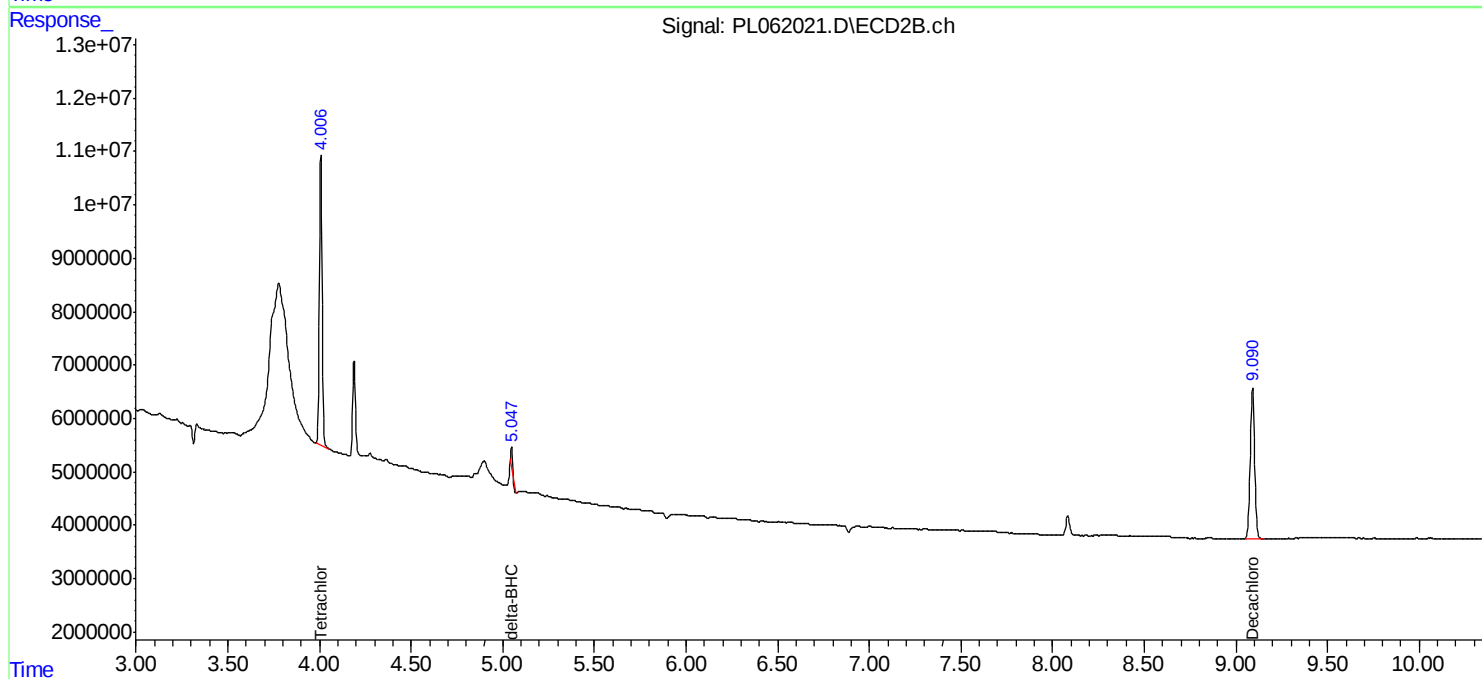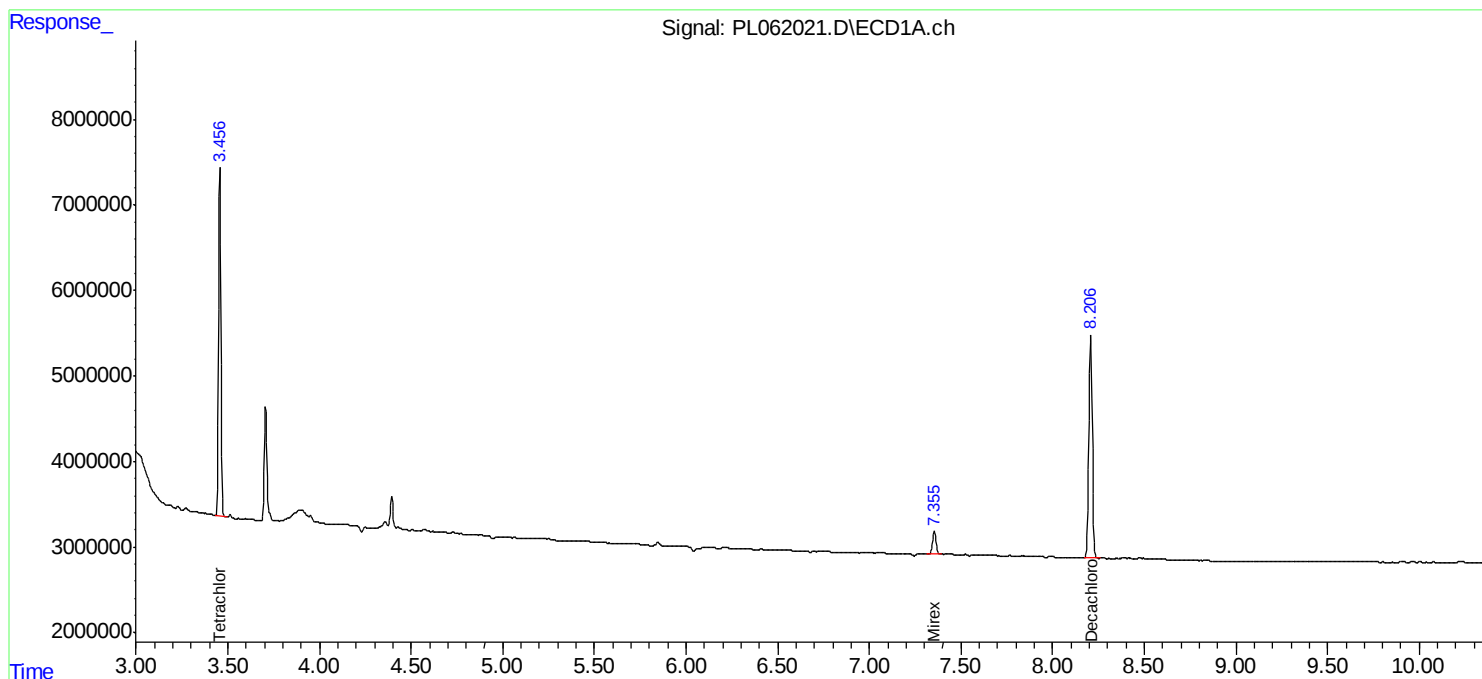


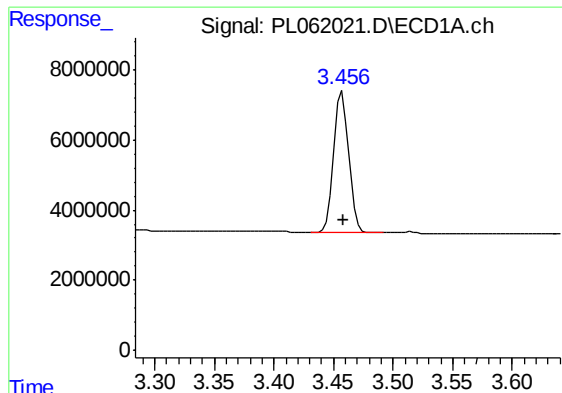

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 35153182
Conc: 20.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-100120

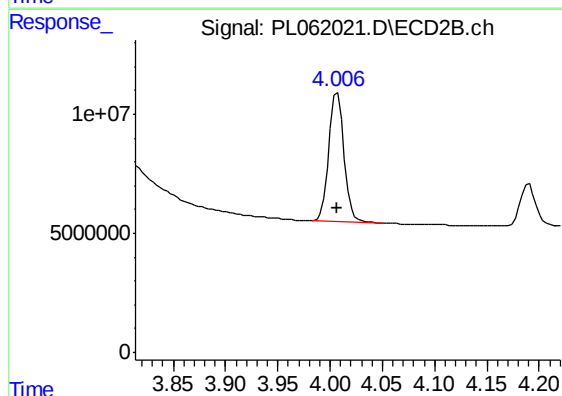


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 54763049
Conc: 20.07 ng/ml

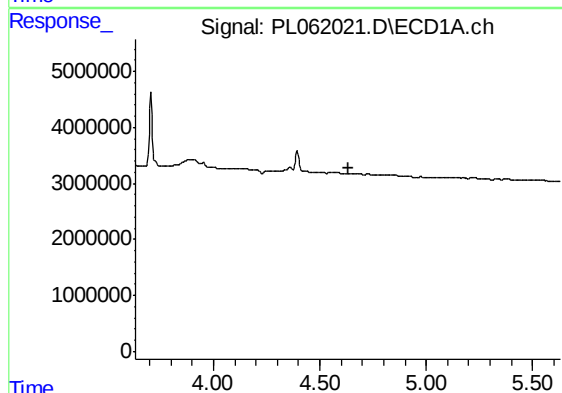


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.632 min
Response: 0
Conc: N.D.

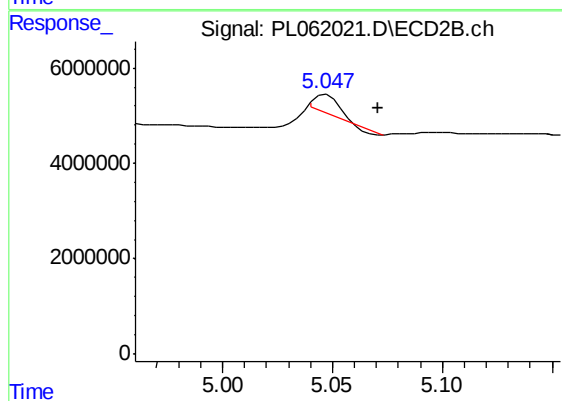

#7 delta-BHC


R.T.: 5.047 min
Delta R.T.: -0.024 min
Response: 2722516
Conc: 1.07 ng/ml

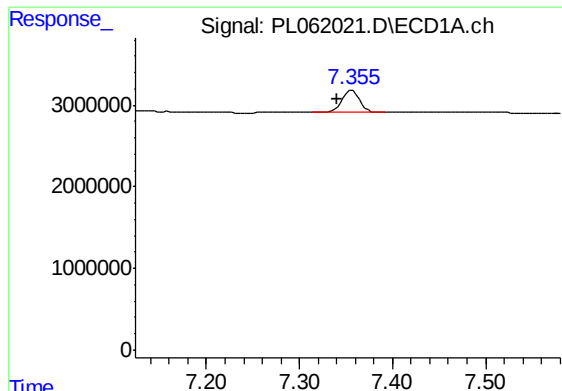

#22 Mirex


R.T.: 7.356 min
Delta R.T.: 0.016 min
Response: 3447409
Conc: 2.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-100120

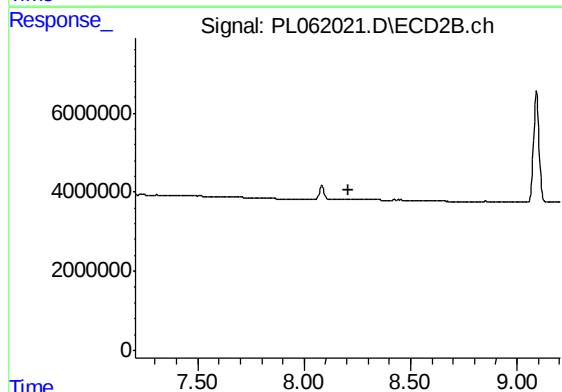


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.207 min
Response: 0
Conc: N.D.

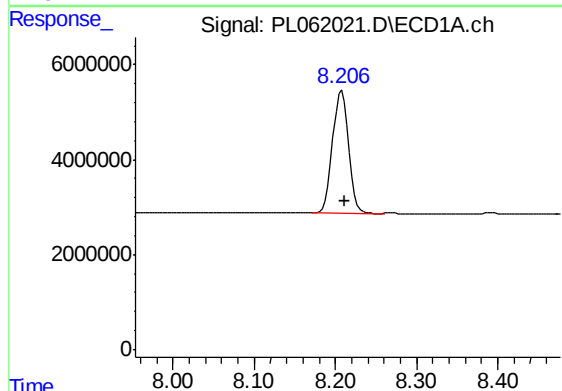

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.004 min
Response: 35505515
Conc: 21.83 ng/ml

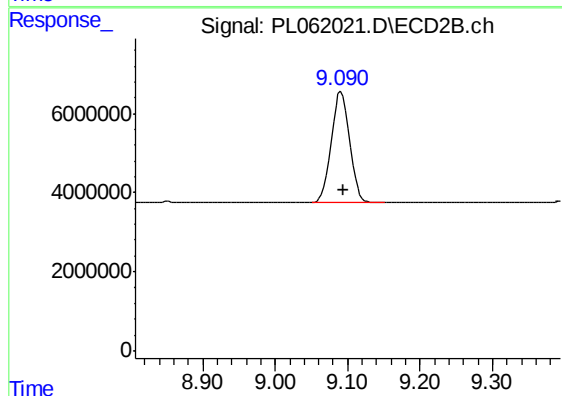

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: -0.003 min
Response: 49766373
Conc: 22.61 ng/ml