

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
 Data File : PL062045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 00:51
 Operator : DD\AJ
 Sample : L4260-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 05:34:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.007	24945527	28125101	14.622	10.309 #
28)	SA Decachlor...	8.208	9.093	21686315	31468057	13.331	14.295
Target Compounds							
5)	MB Aldrin	0.000	5.493	0	4142558	N.D.	1.279 #
10)	B gamma-Chl...	0.000	6.130	0	3984567	N.D.	1.357 #
11)	B alpha-Chl...	0.000	6.173f	0	4676428	N.D.	1.557 #
13)	MA Dieldrin	5.753	0.000	4667719	0	2.775	N.D. #
23)	Chlordane-1	4.323	5.033f	5506921	1434523	111.215	15.236 #
24)	Chlordane-2	4.801f	5.493f	3382286	4142558	57.516	40.256 #
25)	Chlordane-3	0.000	6.130	0	3984567	N.D.	10.874 #
26)	Chlordane-4	0.000	6.173f	0	4676428	N.D.	10.417 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
Data File : PL062045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 00:51
Operator : DD\AJ
Sample : L4260-03
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 05:34:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

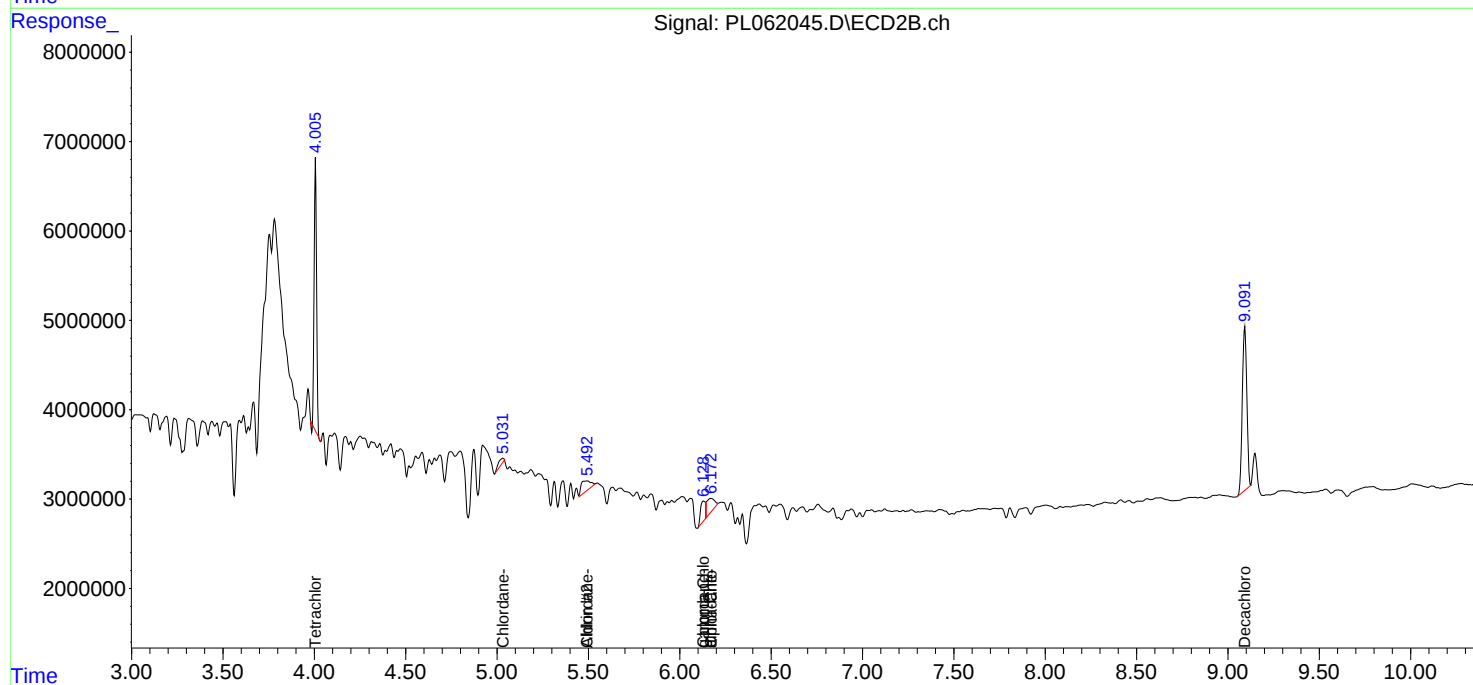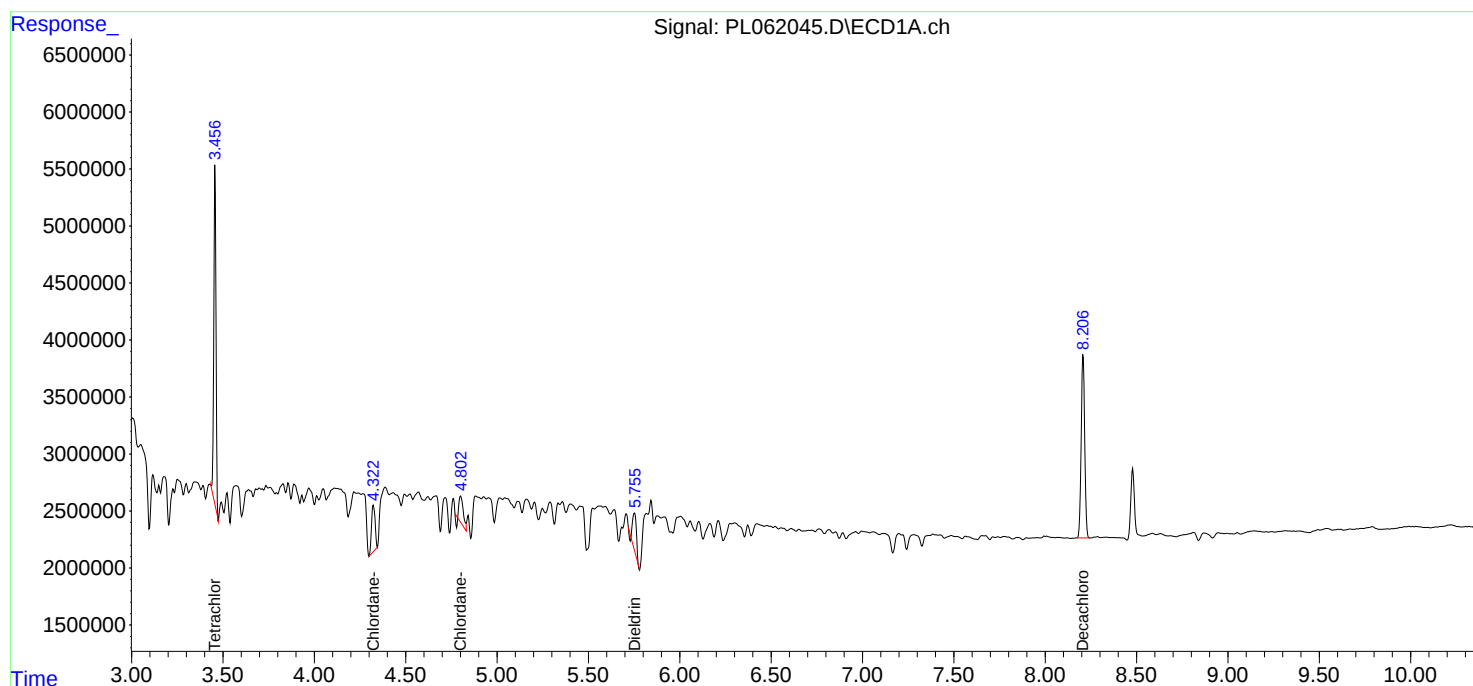


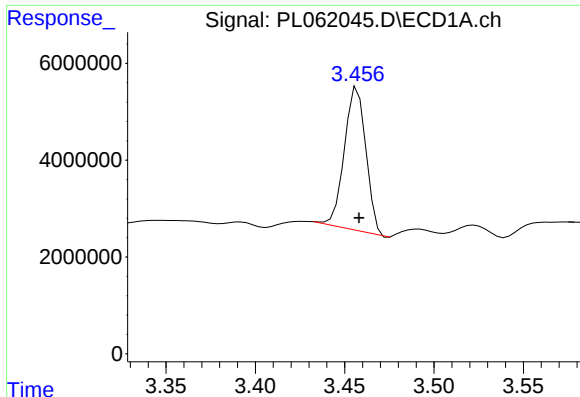

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 24945527
Conc: 14.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

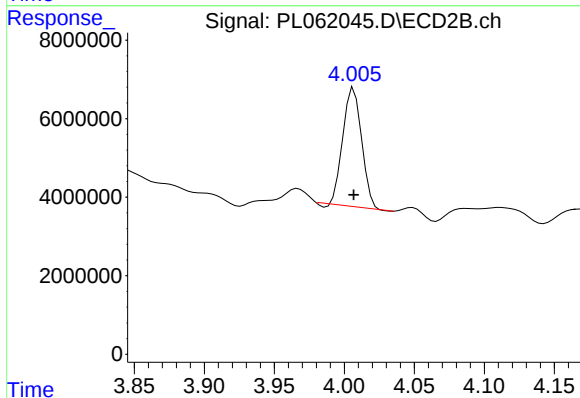


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 28125101
Conc: 10.31 ng/ml

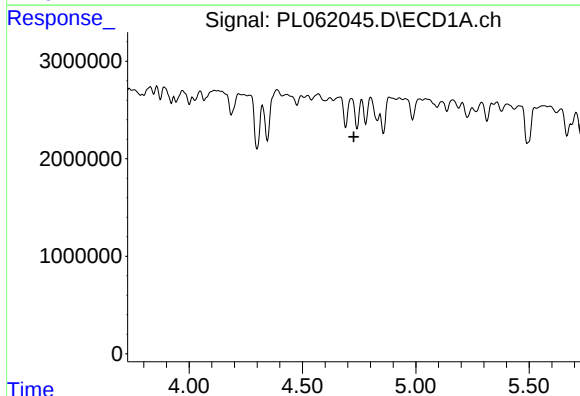


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

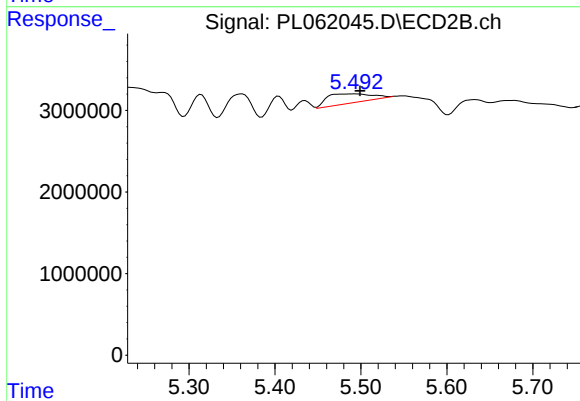

#5 Aldrin


R.T.: 5.493 min
Delta R.T.: -0.006 min
Response: 4142558
Conc: 1.28 ng/ml

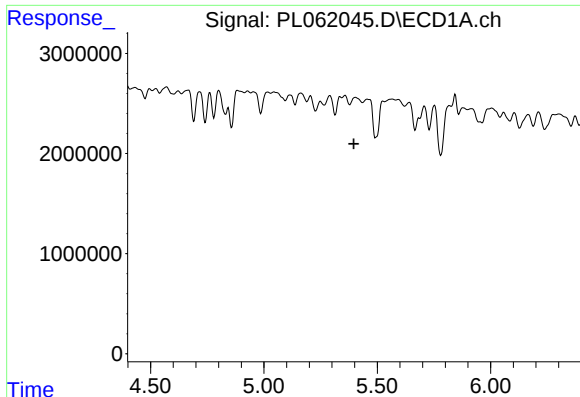

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

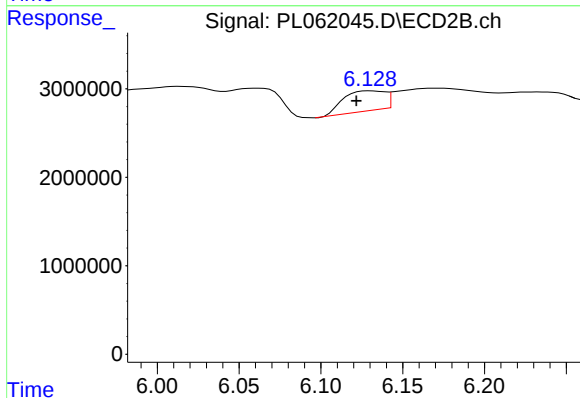


#10 gamma-Chlordane

R.T.: 6.130 min
Delta R.T.: 0.009 min
Response: 3984567
Conc: 1.36 ng/ml

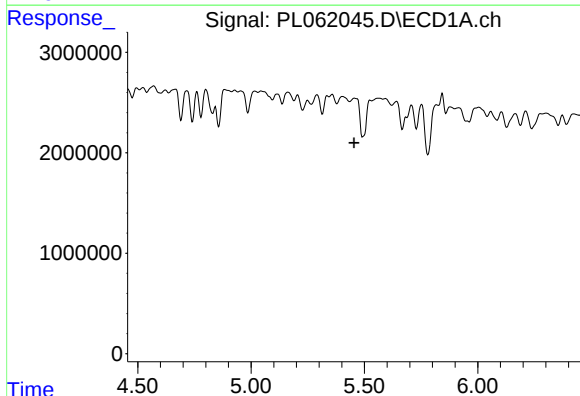


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

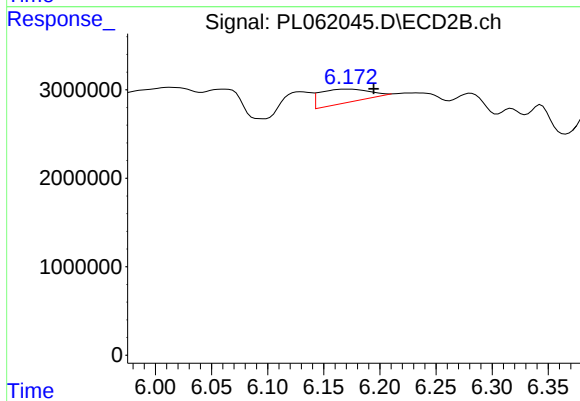

#11 alpha-Chlordane


R.T.: 6.173 min
Delta R.T.: -0.021 min
Response: 4676428
Conc: 1.56 ng/ml

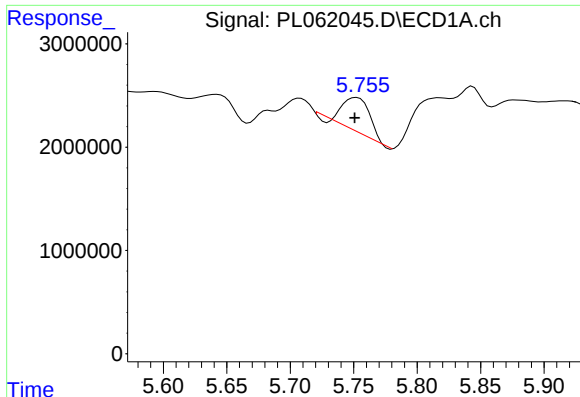

#13 Dieldrin


R.T.: 5.753 min
Delta R.T.: 0.002 min
Response: 4667719
Conc: 2.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

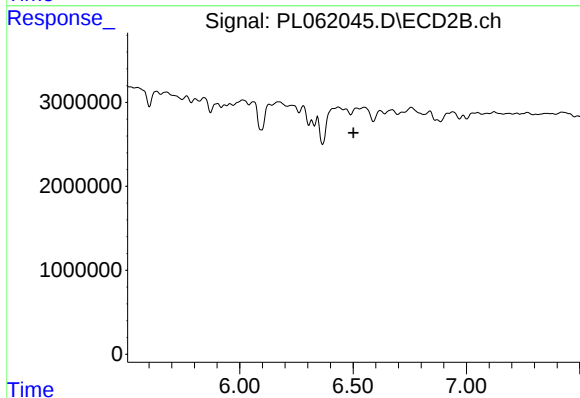


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.502 min
Response: 0
Conc: N.D.

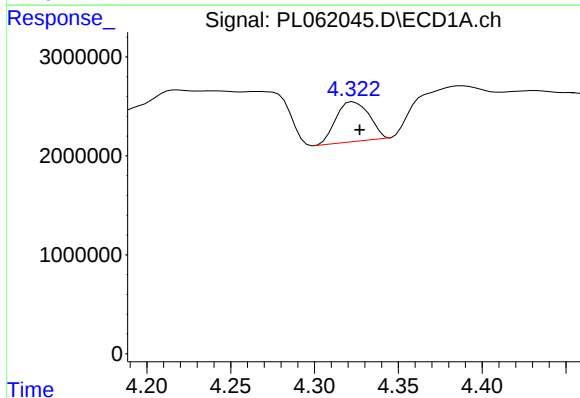


#23 Chlordane-1

R.T.: 4.323 min
Delta R.T.: -0.004 min
Response: 5506921
Conc: 111.22 ng/ml

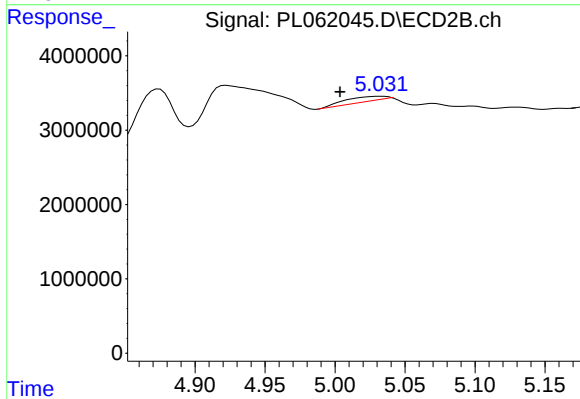

#23 Chlordane-1


R.T.: 5.033 min
Delta R.T.: 0.029 min
Response: 1434523
Conc: 15.24 ng/ml

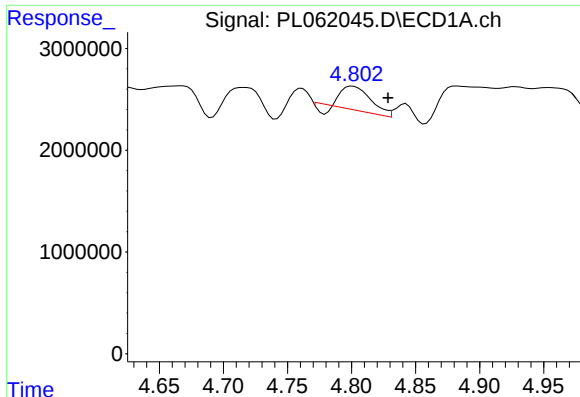

#24 Chlordane-2


R.T.: 4.801 min
Delta R.T.: -0.028 min
Response: 3382286
Conc: 57.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

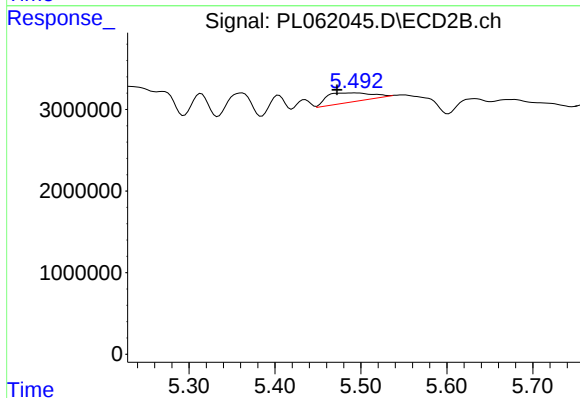


#24 Chlordane-2

R.T.: 5.493 min
Delta R.T.: 0.020 min
Response: 4142558
Conc: 40.26 ng/ml

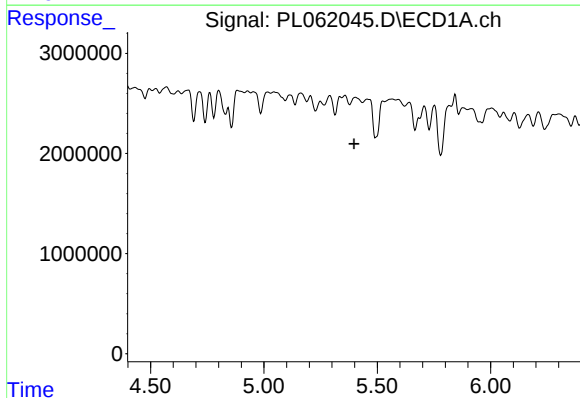


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

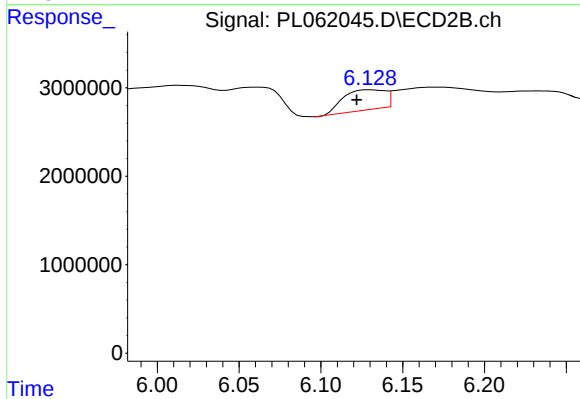

#25 Chlordane-3


R.T.: 6.130 min
Delta R.T.: 0.008 min
Response: 3984567
Conc: 10.87 ng/ml

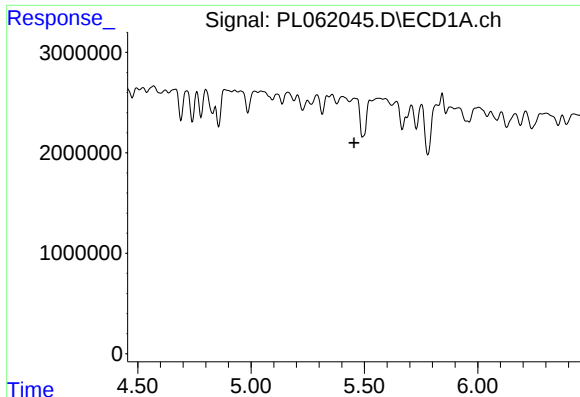

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

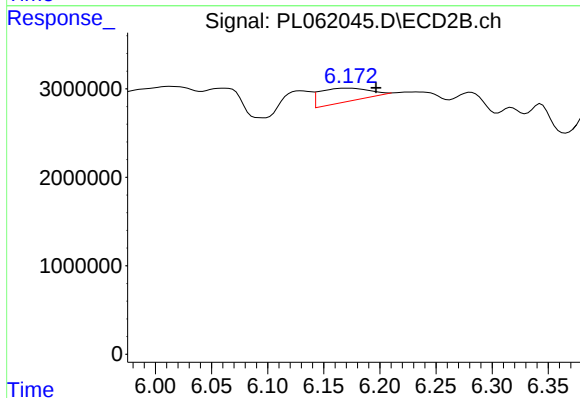


#26 Chlordane-4

R.T.: 6.173 min
Delta R.T.: -0.024 min
Response: 4676428
Conc: 10.42 ng/ml

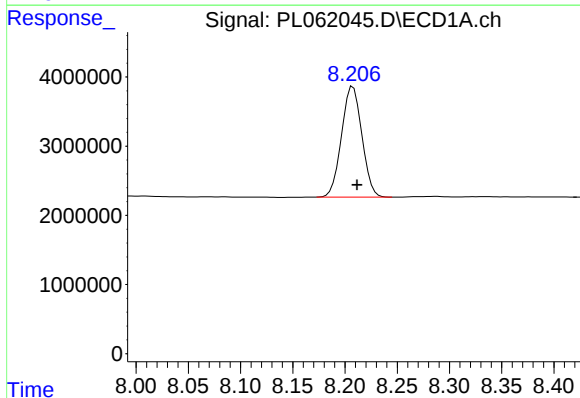

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.004 min
Response: 21686315
Conc: 13.33 ng/ml

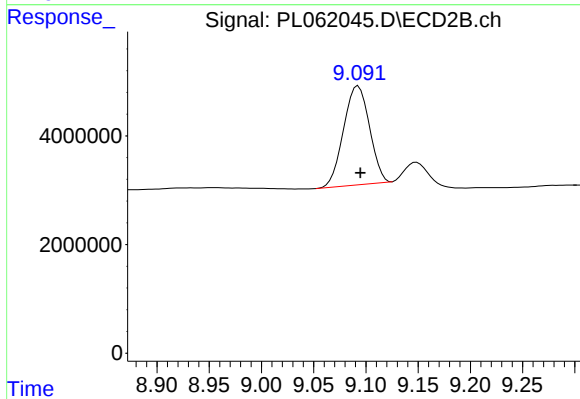

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 31468057
Conc: 14.29 ng/ml