

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
 Data File : PL062046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 01:05
 Operator : DD\AJ
 Sample : L4260-05
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 04:34:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.006	24788682	35298214	14.531	12.938
28)	SA Decachlor...	8.207	9.091	20896443	29065935	12.845	13.204
Target Compounds							
6)	B beta-BHC	0.000	4.880f	0	50700	N.D.	0.034 #
10)	B gamma-Chl...	0.000	6.151f	0	4644168	N.D.	1.581 #
23)	Chlordane-1	4.323	0.000	3448173	0	69.638	N.D. #
25)	Chlordane-3	0.000	6.151f	0	4644168	N.D.	12.674 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
Data File : PL062046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 01:05
Operator : DD\AJ
Sample : L4260-05
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 04:34:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

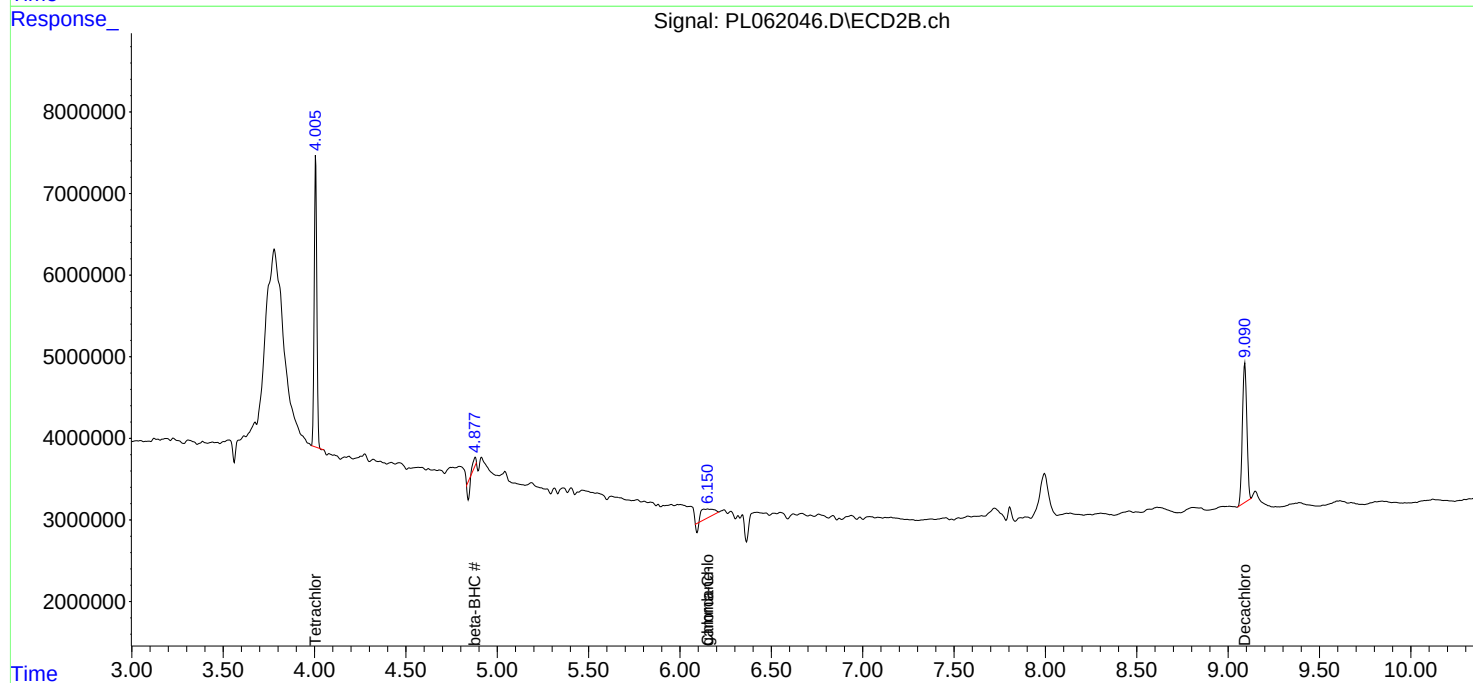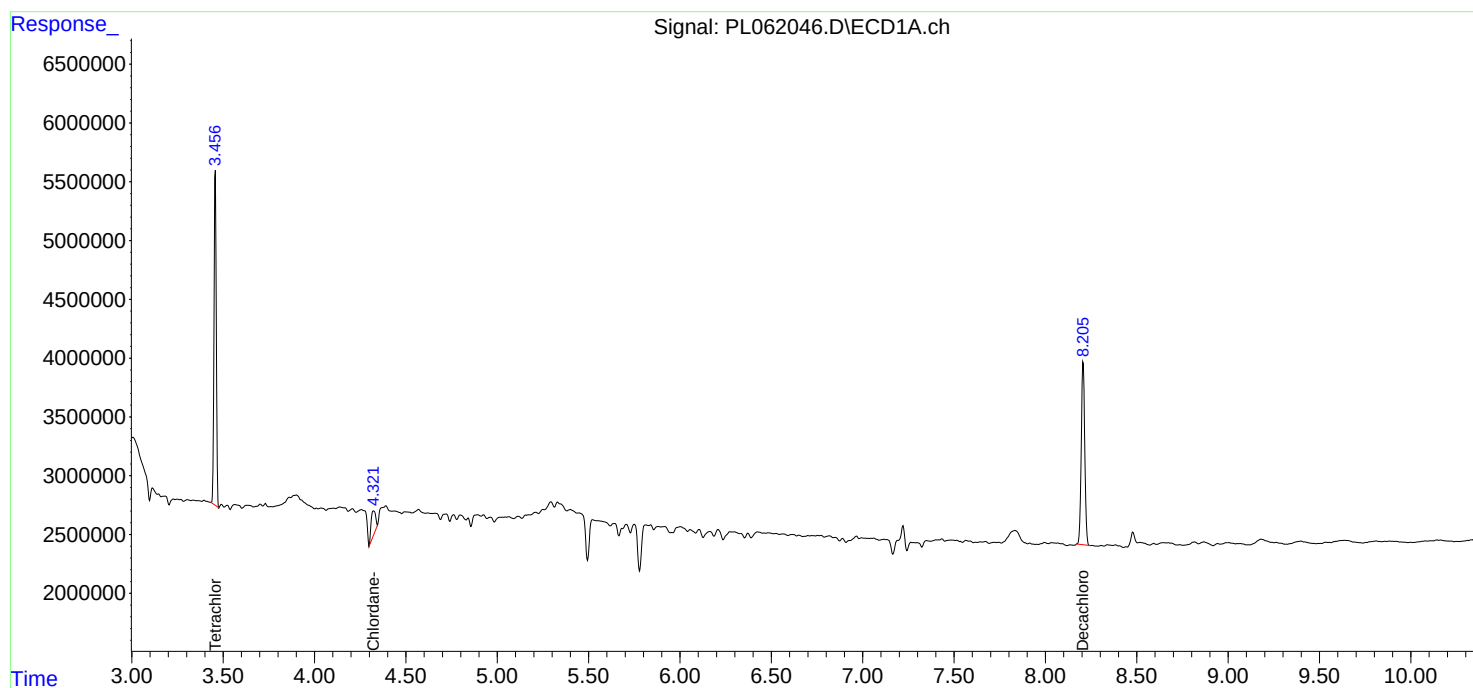


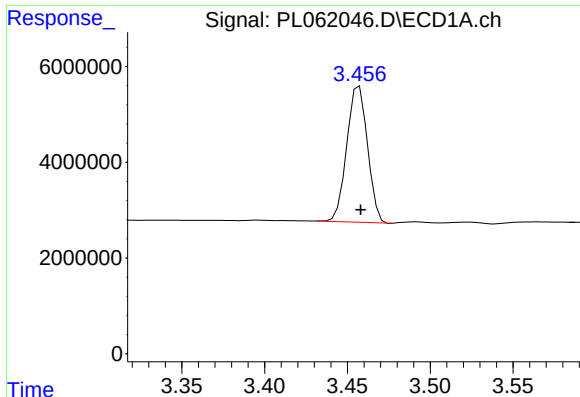

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 24788682
Conc: 14.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

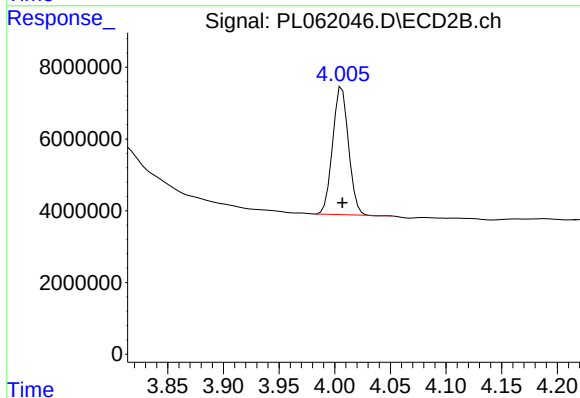


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: 0.000 min
Response: 35298214
Conc: 12.94 ng/ml

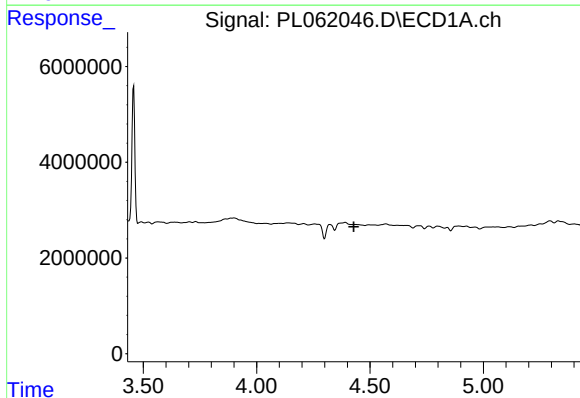


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.428 min
Response: 0
Conc: N.D.

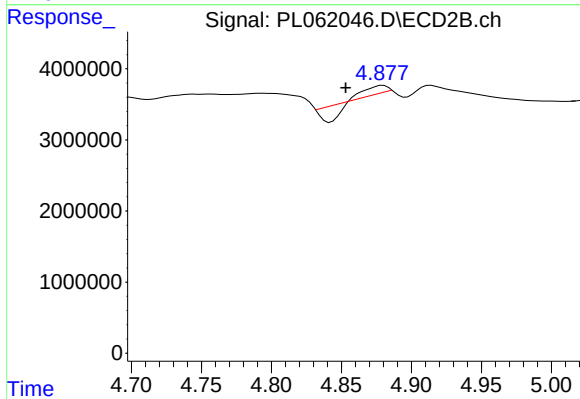

#6 beta-BHC


R.T.: 4.880 min
Delta R.T.: 0.027 min
Response: 50700
Conc: 0.03 ng/ml

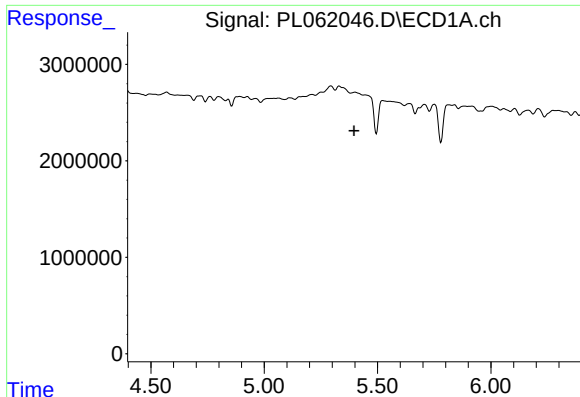

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

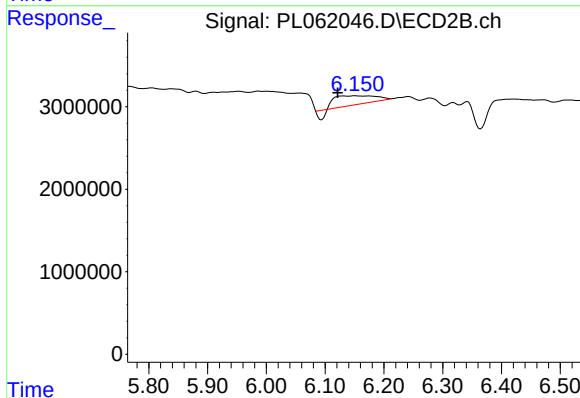


#10 gamma-Chlordane

R.T.: 6.151 min
Delta R.T.: 0.030 min
Response: 4644168
Conc: 1.58 ng/ml

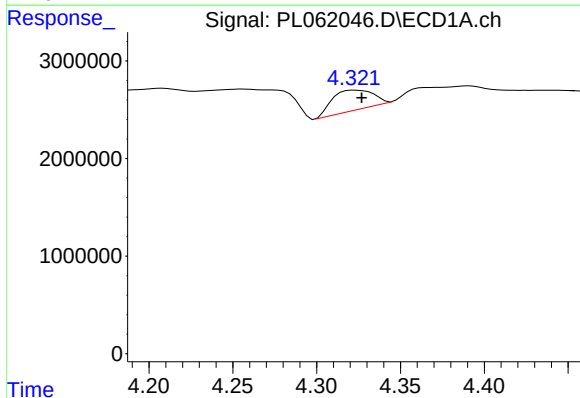


#23 Chlordane-1

R.T.: 4.323 min
Delta R.T.: -0.004 min
Response: 3448173
Conc: 69.64 ng/ml

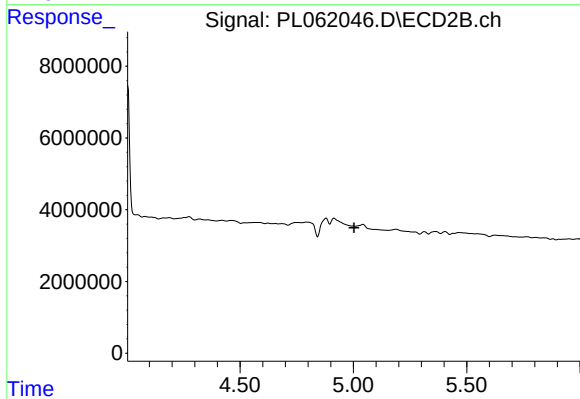

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

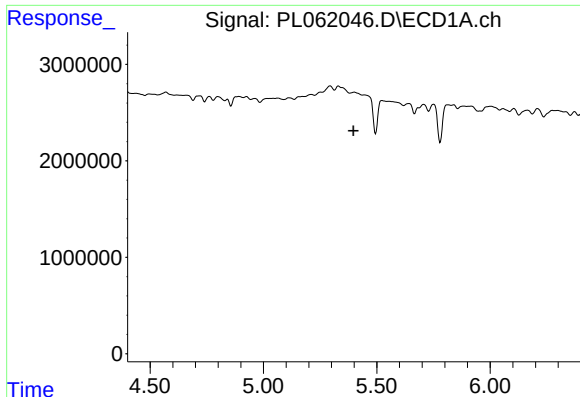

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

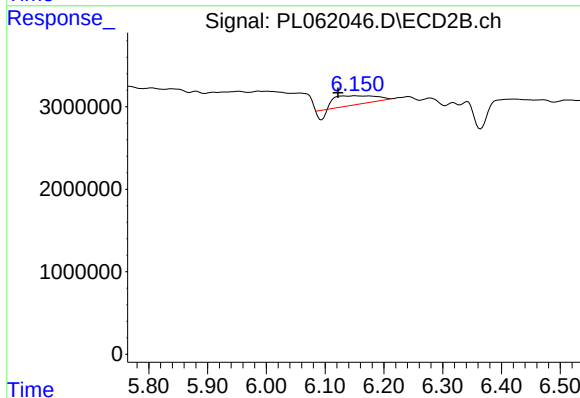


#25 Chlordane-3

R.T.: 6.151 min
Delta R.T.: 0.029 min
Response: 4644168
Conc: 12.67 ng/ml

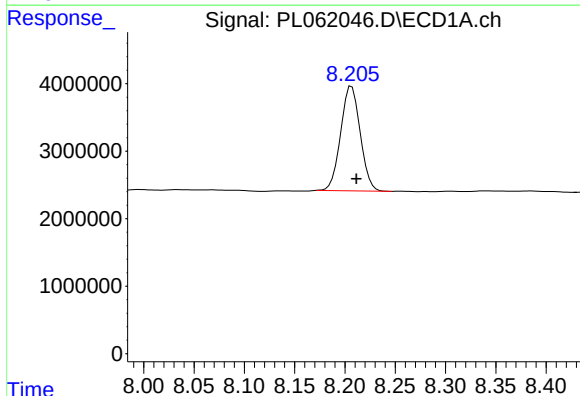

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.005 min
Response: 20896443
Conc: 12.85 ng/ml

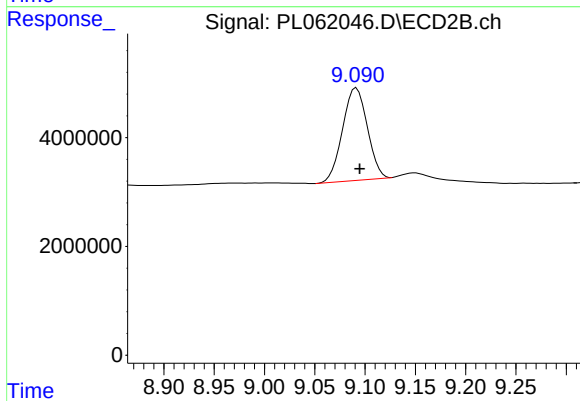

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: -0.003 min
Response: 29065935
Conc: 13.20 ng/ml