

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
 Data File : PL062047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 01:19
 Operator : DD\AJ
 Sample : L4260-11
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 04:34:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.007	25149303	32285720	14.742	11.834
28)	SA Decachlor...	8.208	9.092	22496985	33133201	13.829	15.051
Target Compounds							
9)	A Endosulfan I	5.522	6.241	9956335	7051541	6.144	2.553 #
11)	B alpha-Chl...	0.000	6.175f	0	21863710	N.D.	7.279 #
23)	Chlordane-1	4.322	0.000	5156951	0	104.147	N.D. #
26)	Chlordane-4	0.000	6.175f	0	21863710	N.D.	48.703 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
Data File : PL062047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 01:19
Operator : DD\AJ
Sample : L4260-11
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 04:34:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

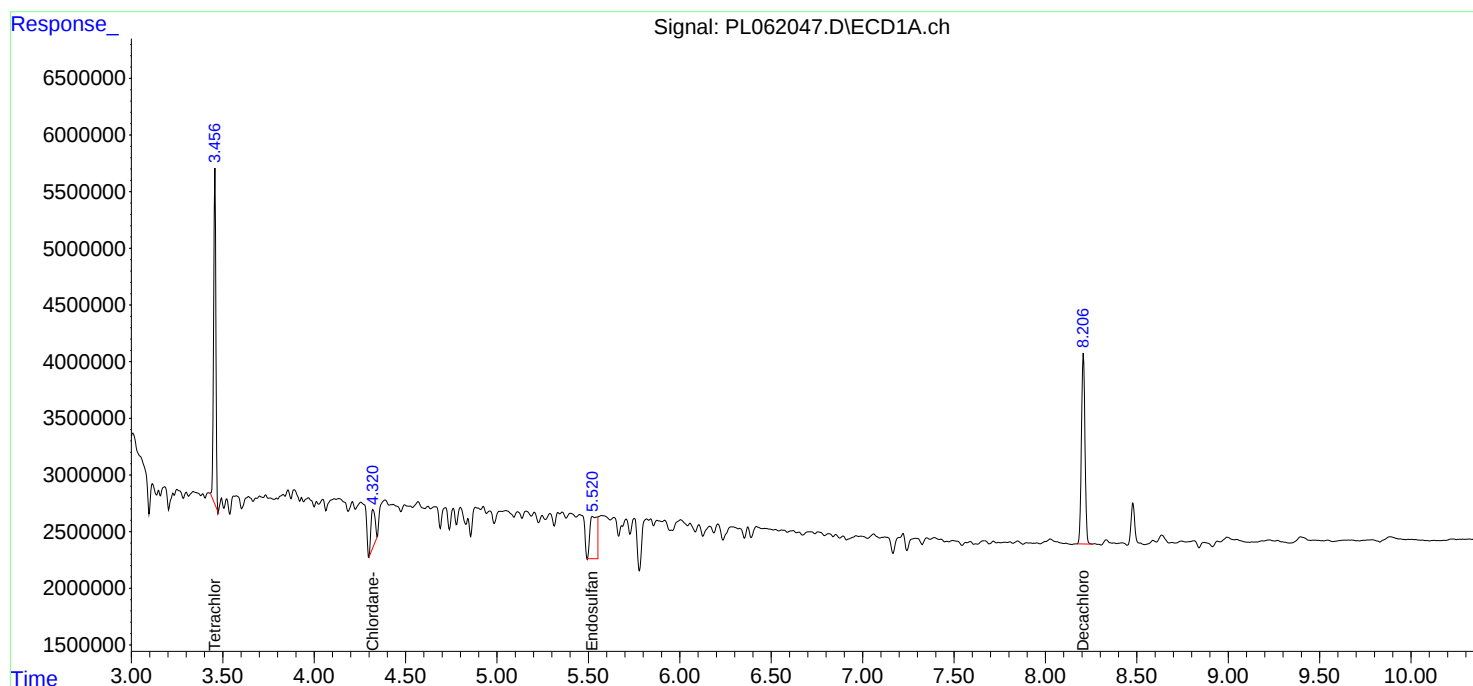


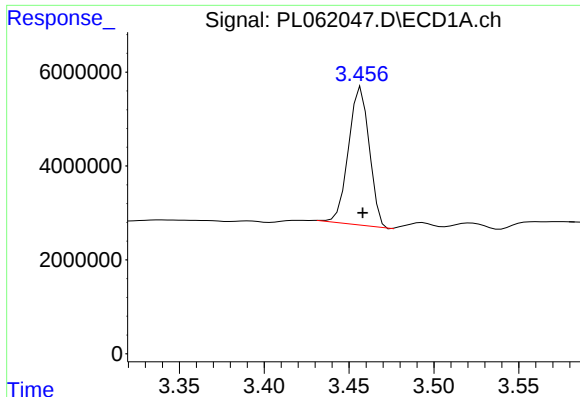

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 25149303
Conc: 14.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

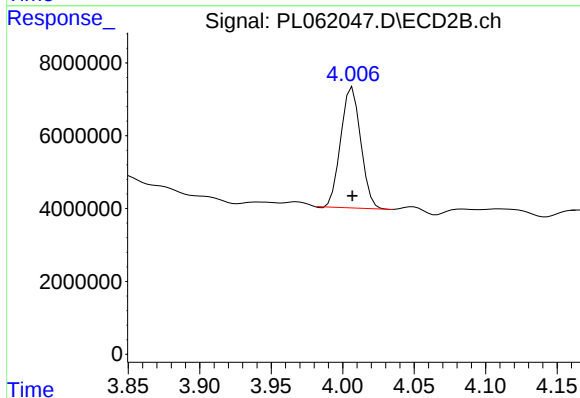


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 32285720
Conc: 11.83 ng/ml

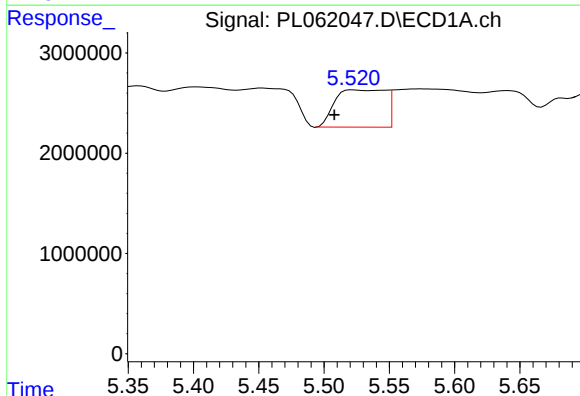


#9 Endosulfan I

R.T.: 5.522 min
Delta R.T.: 0.014 min
Response: 9956335
Conc: 6.14 ng/ml

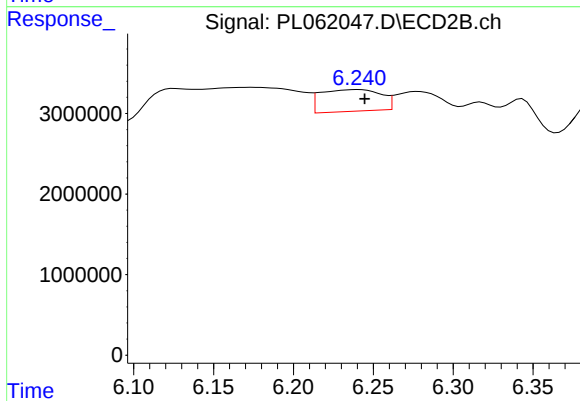

#9 Endosulfan I


R.T.: 6.241 min
Delta R.T.: -0.004 min
Response: 7051541
Conc: 2.55 ng/ml

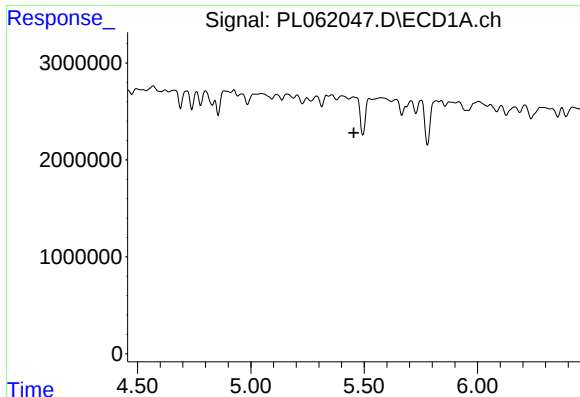

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

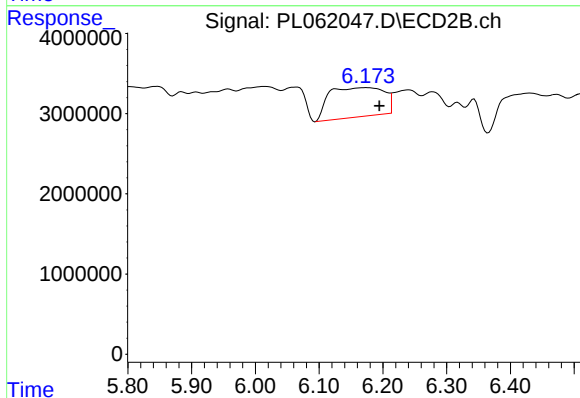


#11 alpha-Chlordane

R.T.: 6.175 min
Delta R.T.: -0.020 min
Response: 21863710
Conc: 7.28 ng/ml

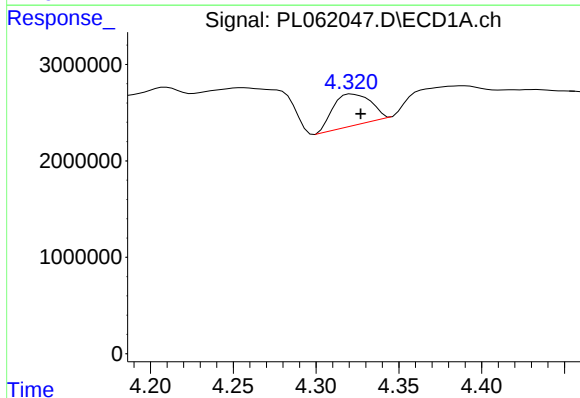


#23 Chlordane-1

R.T.: 4.322 min
Delta R.T.: -0.005 min
Response: 5156951
Conc: 104.15 ng/ml

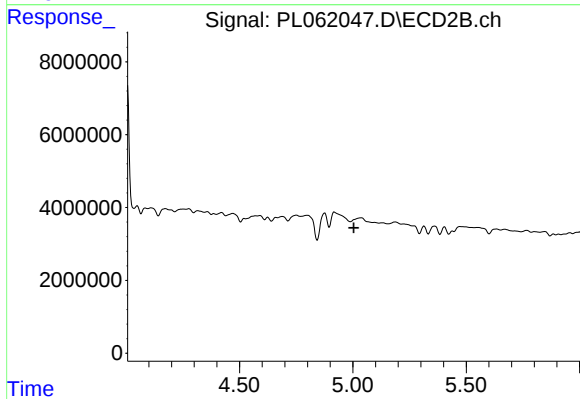

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.004 min
Response: 0
Conc: N.D.

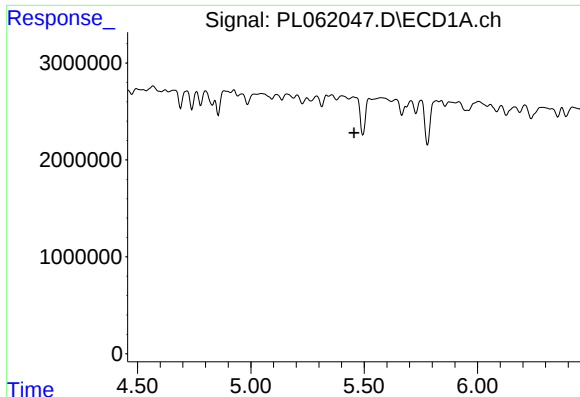

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

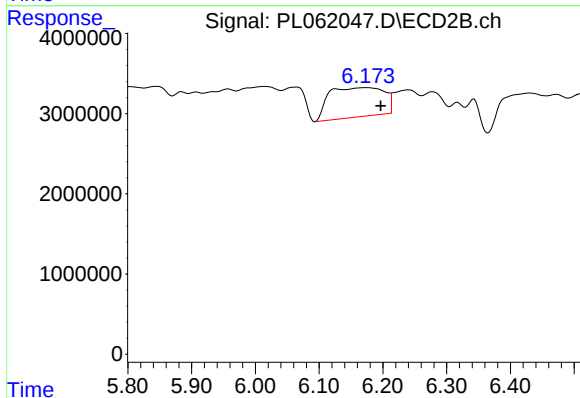


#26 Chlordane-4

R.T.: 6.175 min
Delta R.T.: -0.022 min
Response: 21863710
Conc: 48.70 ng/ml

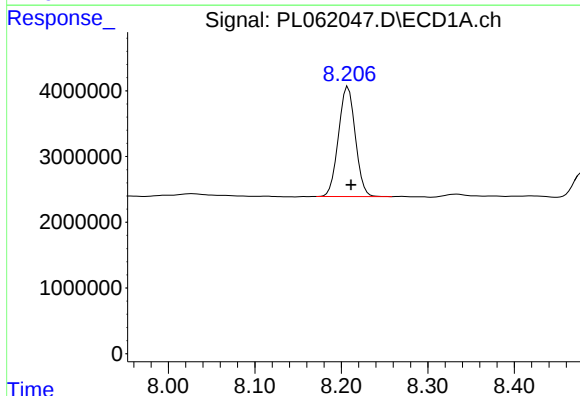

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.004 min
Response: 22496985
Conc: 13.83 ng/ml

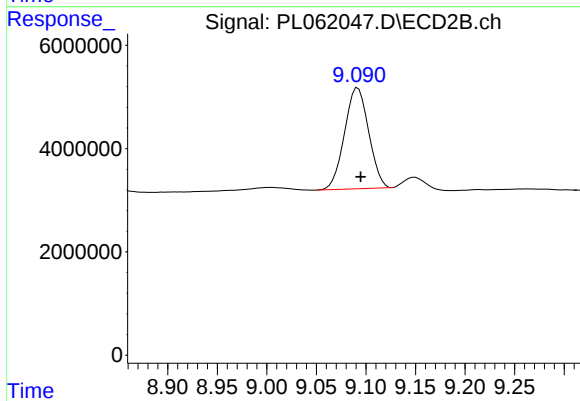

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.003 min
Response: 33133201
Conc: 15.05 ng/ml