

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
 Data File : PL062045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2020 00:51
 Operator : DD\AJ
 Sample : L4260-03
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PAV-B21-100220-0-10

Manual Integrations
 APPROVED

Ankita
 10/6/2020 11:07:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 05:34:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.005	24945527	29709263	14.622	10.890m#
28)	SA Decachlor...	8.208	9.093	21686315	31468057	13.331	14.295

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100520\
Data File : PL062045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2020 00:51
Operator : DD\AJ
Sample : L4260-03
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PAV-B21-100220-0-10


Manual Integrations
APPROVED

Ankita
10/6/2020 11:07:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 05:34:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

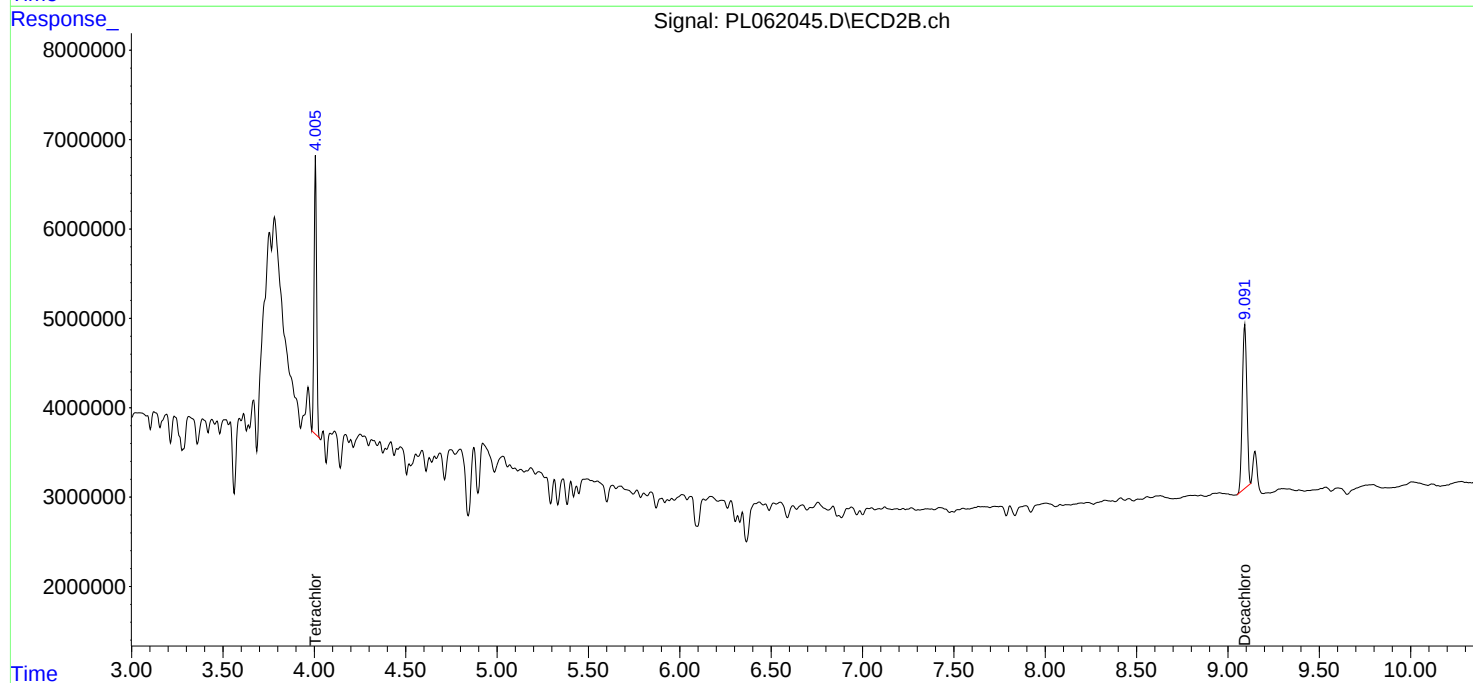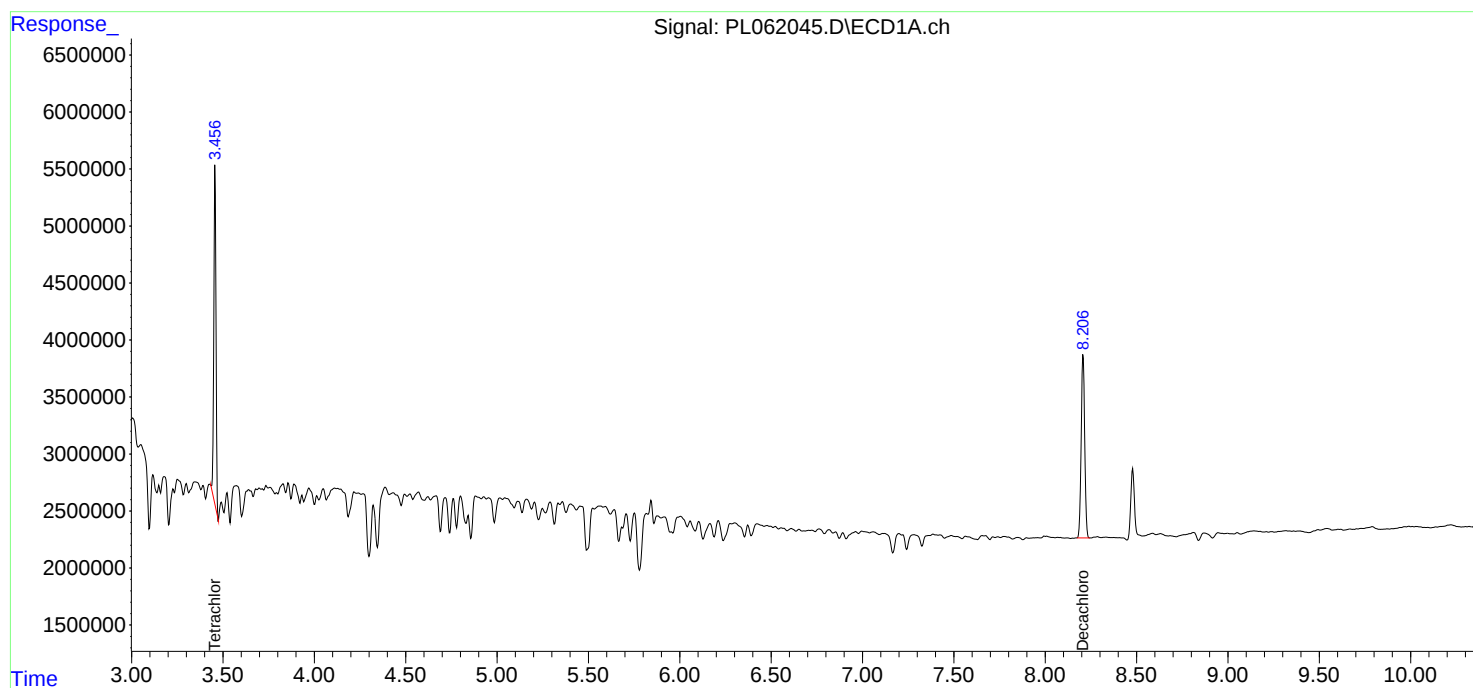

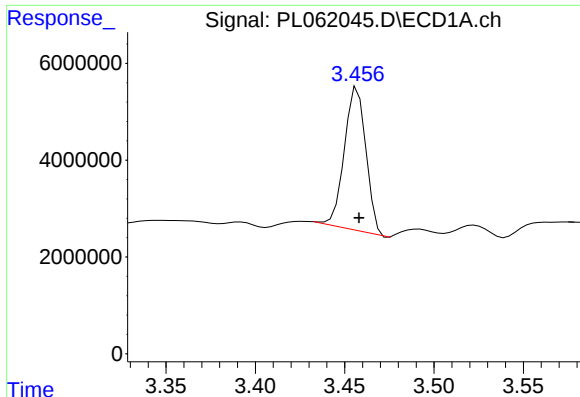


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 24945527
Conc: 14.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PAV-B21-100220-0-10


Manual Integrations
APPROVED

Ankita
10/6/2020 11:07:05 AM

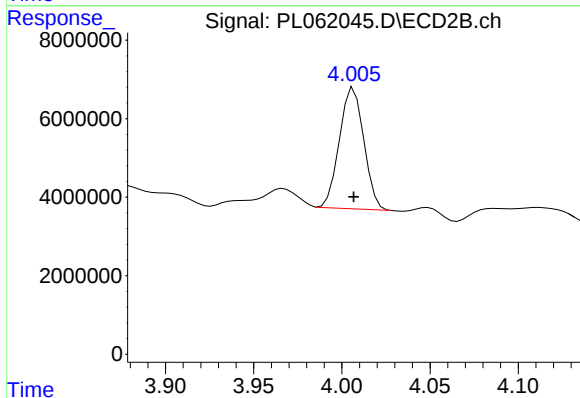


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.001 min
Response: 29709263
Conc: 10.89 ng/ml m

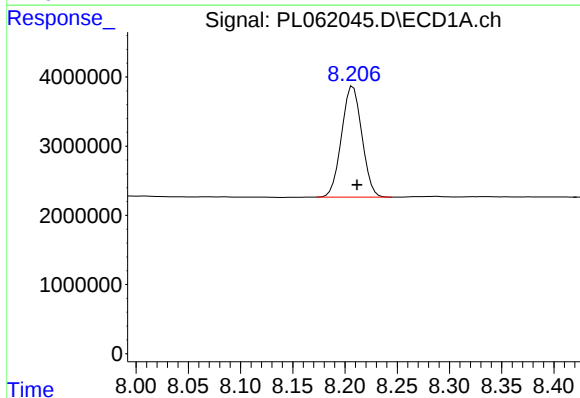

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.004 min
Response: 21686315
Conc: 13.33 ng/ml

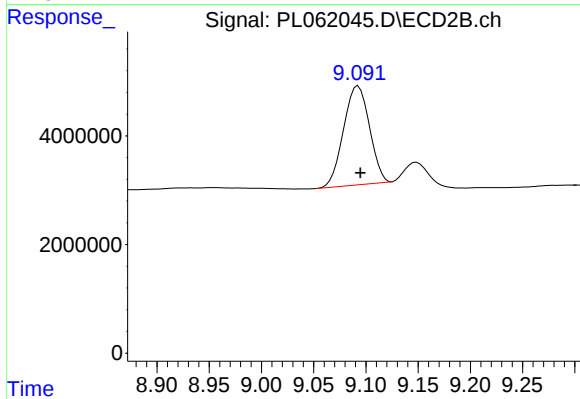

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 31468057
Conc: 14.29 ng/ml