

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100521\
 Data File : PL070153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2021 14:32
 Operator : AR\AJ
 Sample : M4060-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-100421

Manual Integrations
 APPROVED

mohammad
 10/6/2021 9:03:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 01:35:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.626	5.562	7531920	18573164	15.052	14.043
28)	SA Decachlor...	10.390	11.481	9796805	16531942	14.158	13.661
Target Compounds							
12)	B 4,4'-DDE	7.626	8.560	449652	726434	0.706	0.469 #
17)	MA 4,4'-DDT	8.470	9.419	653418	736216	1.068	0.563m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100521\
Data File : PL070153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2021 14:32
Operator : AR\AJ
Sample : M4060-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TR-05-100421


Manual Integrations
APPROVED

mohammad
10/6/2021 9:03:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 01:35:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

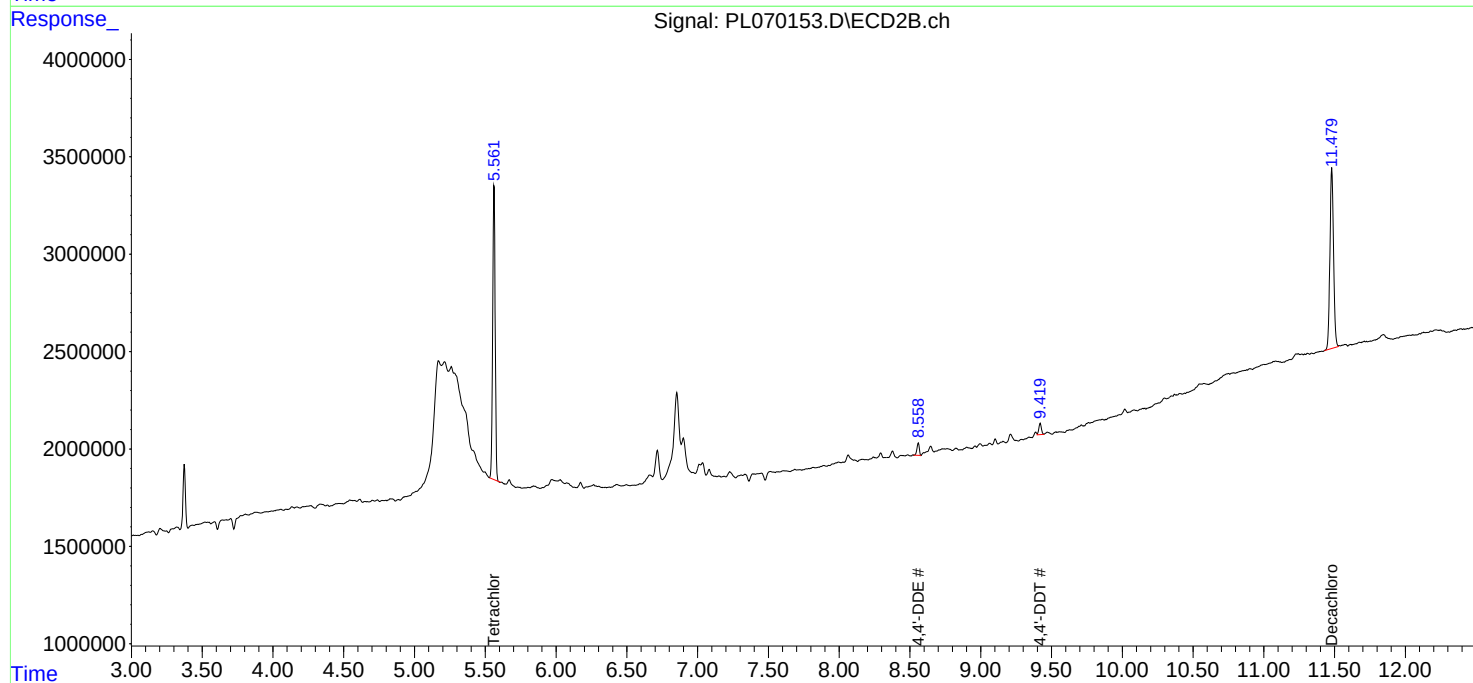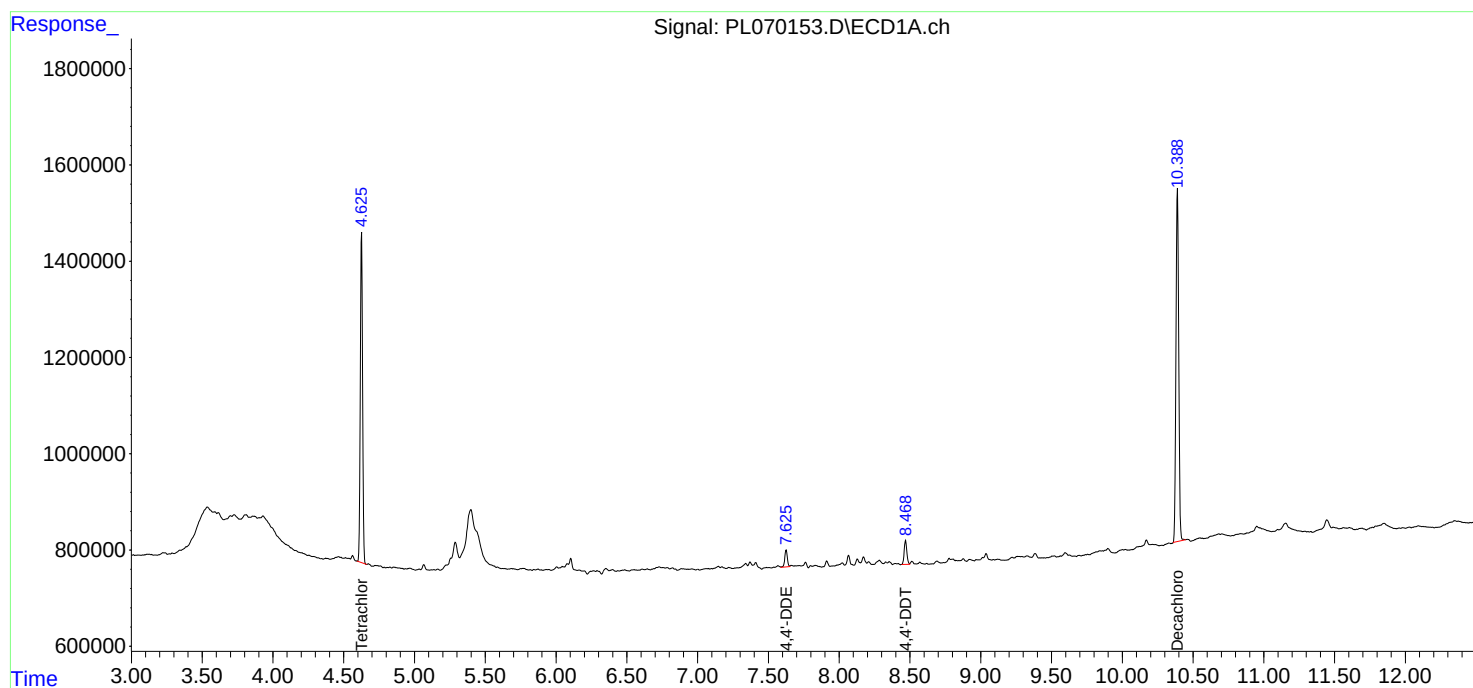

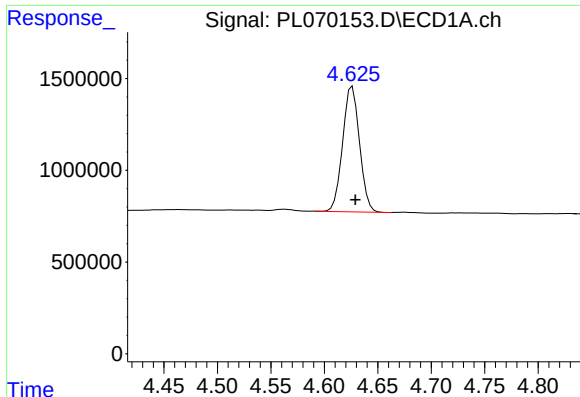


#1 Tetrachloro-m-xylene

R.T.: 4.626 min
Delta R.T.: -0.003 min
Response: 7531920
Conc: 15.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-100421


Manual Integrations
APPROVED

mohammad
10/6/2021 9:03:47 AM

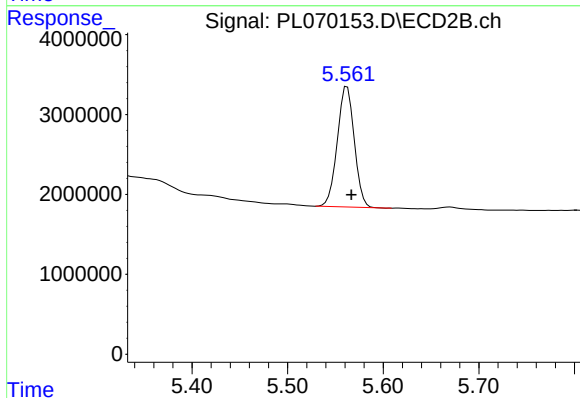


#1 Tetrachloro-m-xylene

R.T.: 5.562 min
Delta R.T.: -0.004 min
Response: 18573164
Conc: 14.04 ng/ml

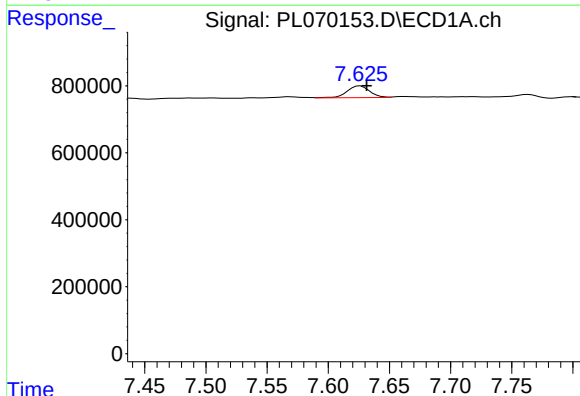


#12 4,4'-DDE

R.T.: 7.626 min
Delta R.T.: -0.005 min
Response: 449652
Conc: 0.71 ng/ml

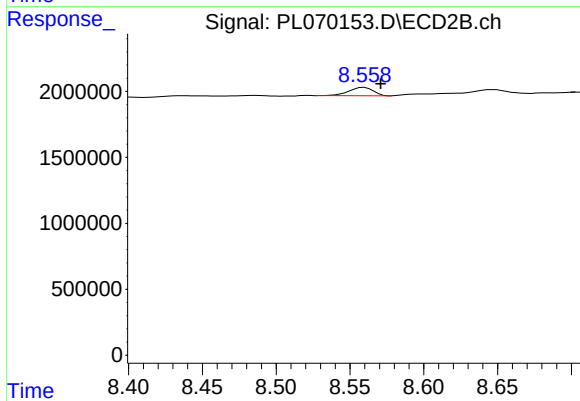

#12 4,4'-DDE

R.T.: 8.560 min
Delta R.T.: -0.011 min
Response: 726434
Conc: 0.47 ng/ml

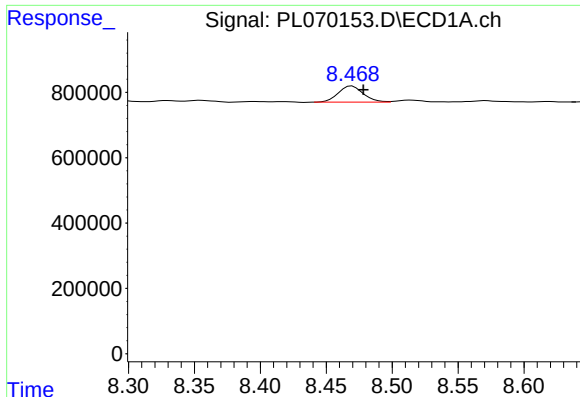


#17 4,4'-DDT

R.T.: 8.470 min
Delta R.T.: -0.009 min
Response: 653418
Conc: 1.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-100421


Manual Integrations
APPROVED

mohammad
10/6/2021 9:03:47 AM

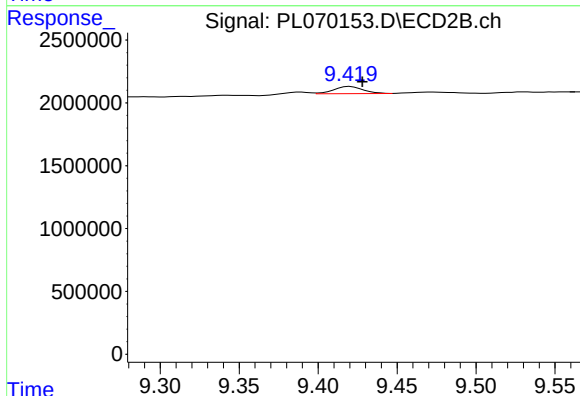


#17 4,4'-DDT

R.T.: 9.419 min
Delta R.T.: -0.009 min
Response: 736216
Conc: 0.56 ng/ml m

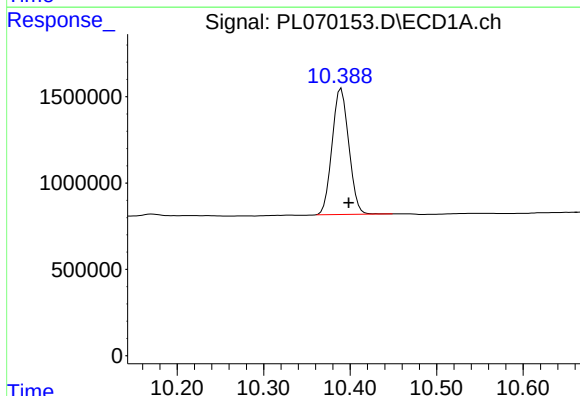

#28 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: -0.008 min
Response: 9796805
Conc: 14.16 ng/ml

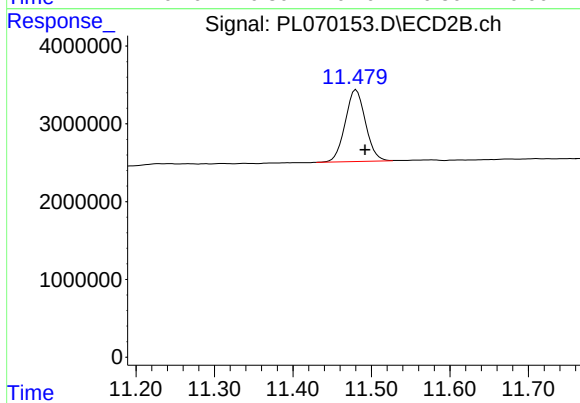

#28 Decachlorobiphenyl

R.T.: 11.481 min
Delta R.T.: -0.011 min
Response: 16531942
Conc: 13.66 ng/ml