

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100522\
 Data File : PL078109.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Oct 2022 21:53
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 23:17:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 04 23:06:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	18202347	33673409	10.238	10.503
27)	SA Decachlor...	8.903	7.719	31572732	52331634	21.642	21.530
Target Compounds							
22)	Toxaphene-1	6.117	5.140	13945359	16721054	999.599	1049.200
23)	Toxaphene-2	6.942	6.404	40792988	66850244	993.564	993.051
24)	Toxaphene-3	7.031	6.531	31808383	90983566	987.496	1007.142
25)	Toxaphene-4	7.122	6.842	14489635	55291634	676.459	1017.400 #
26)	Toxaphene-5	7.819	6.975	23677832	32113588	982.422	966.279

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100522\
Data File : PL078109.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Oct 2022 21:53
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 23:17:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Tue Oct 04 23:06:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

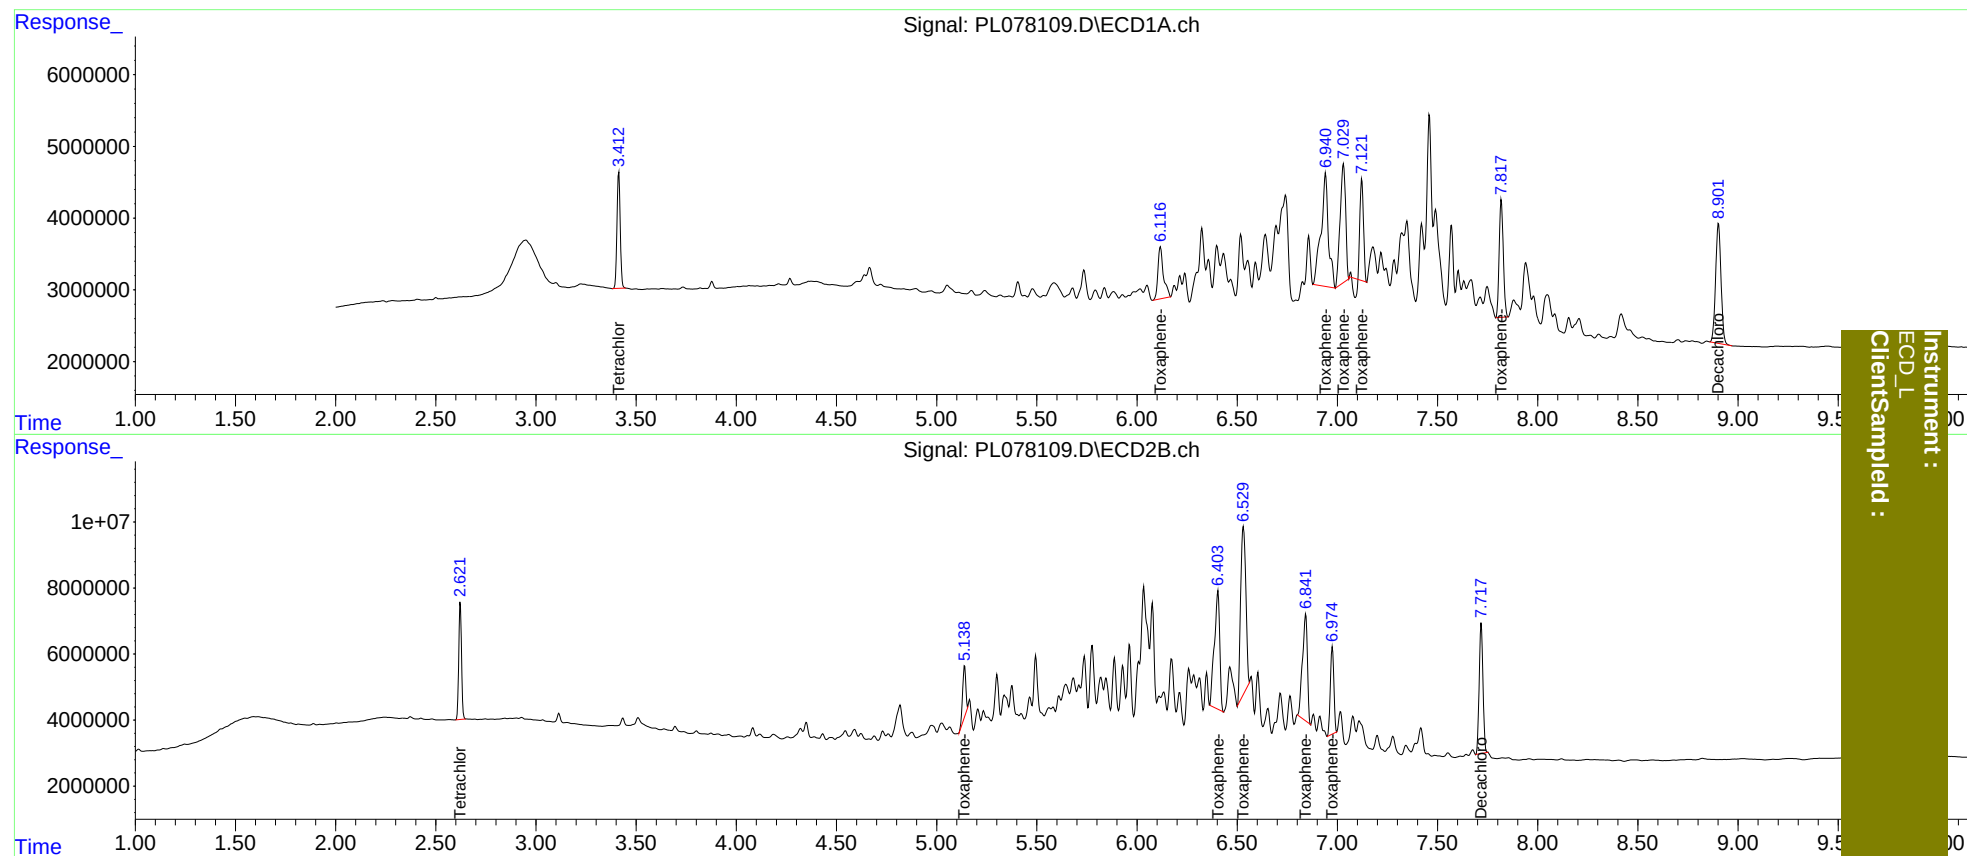

Instrument :
ECD_L
ClientSampled :
PL100522CLP.M Tue Oct 04 23:17:37 2022