

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100522\
 Data File : PL078119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 00:11
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 00:29:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 00:23:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	66103967	123.3E6	39.414	38.948
27)	SA Decachlor...	8.902	7.719	109.1E6	194.1E6	77.373	77.269
Target Compounds							
2)	A alpha-BHC	3.879	3.115	97222138	188.5E6	40.258	39.372
3)	MA gamma-BHC...	4.214	3.439	91995891	172.4E6	39.942	39.409
4)	MA Heptachlor	4.789	3.770	91414895	170.7E6	39.725	39.230
9)	A Endosulfan I	5.950	4.908	66829428	132.3E6	39.609	38.992
13)	MA Dieldrin	6.227	5.172	143.5E6	288.1E6	80.248	78.302
14)	MA Endrin	6.458	5.444	121.9E6	238.2E6	79.689	77.907
16)	A 4,4'-DDD	6.599	5.601	104.4E6	225.4E6	80.244	78.688
17)	MA 4,4'-DDT	6.910	5.849	111.5E6	226.4E6	80.093	78.242
20)	A Methoxychlor	7.392	6.426	277.5E6	534.8E6	392.091	384.185

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100522\
Data File : PL078119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 00:11
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 00:29:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 00:23:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

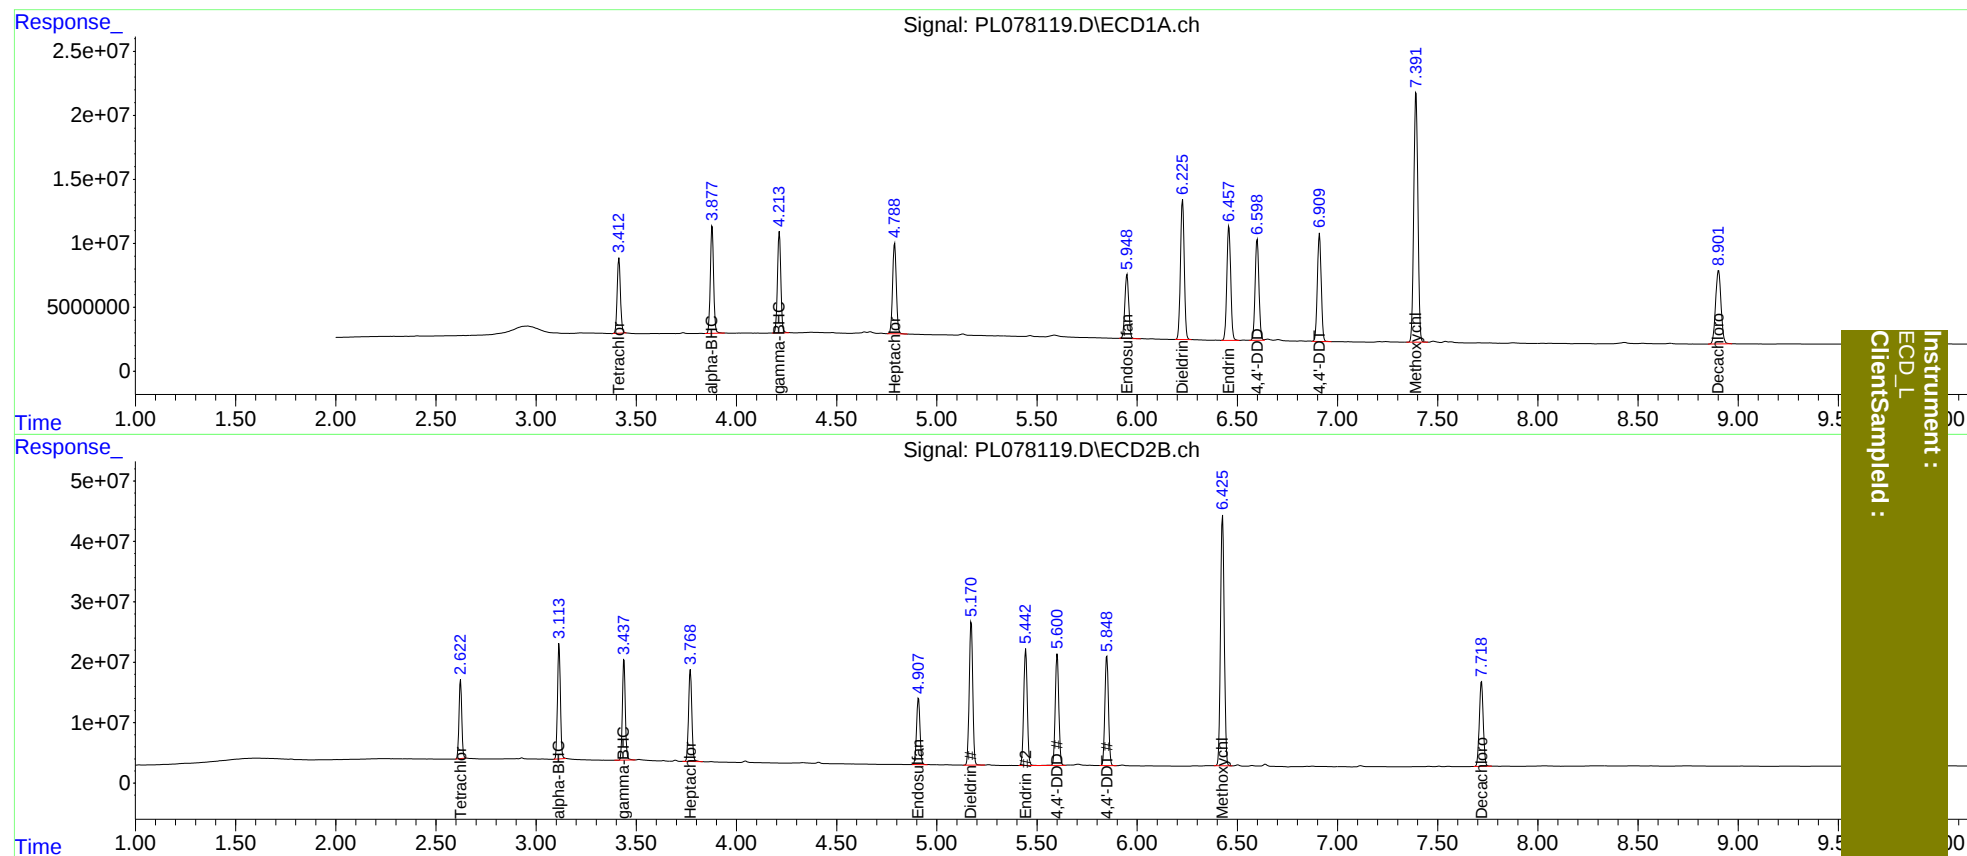

Instrument :
ECD_L
ClientSampled :
PL100522CLP.M