

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100523\
 Data File : PL085725.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2023 16:11
 Operator : AR\AJ
 Sample : 04769-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-06-10-4-2023

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/06/2023
 Supervised By : Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 21:22:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.623	31430231	10557661	10.568	11.302
28)	SA Decachlor...	8.859	7.774	25752790	9800071	11.824	10.618
Target Compounds							
12)	B 4,4'-DDE	6.021	5.080	1743794	432663	0.624	0.527m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100523\
Data File : PL085725.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2023 16:11
Operator : AR\AJ
Sample : 04769-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AU-06-10-4-2023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/06/2023
Supervised By : Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 21:22:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

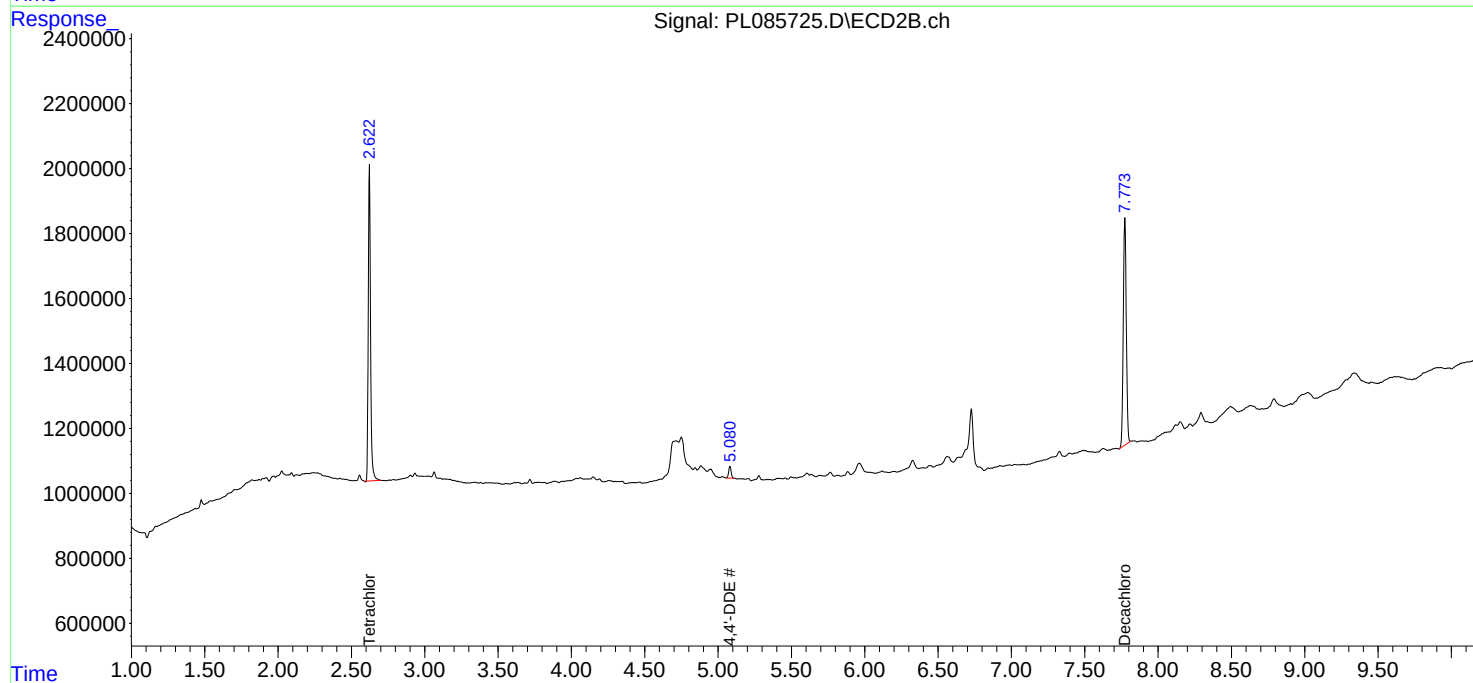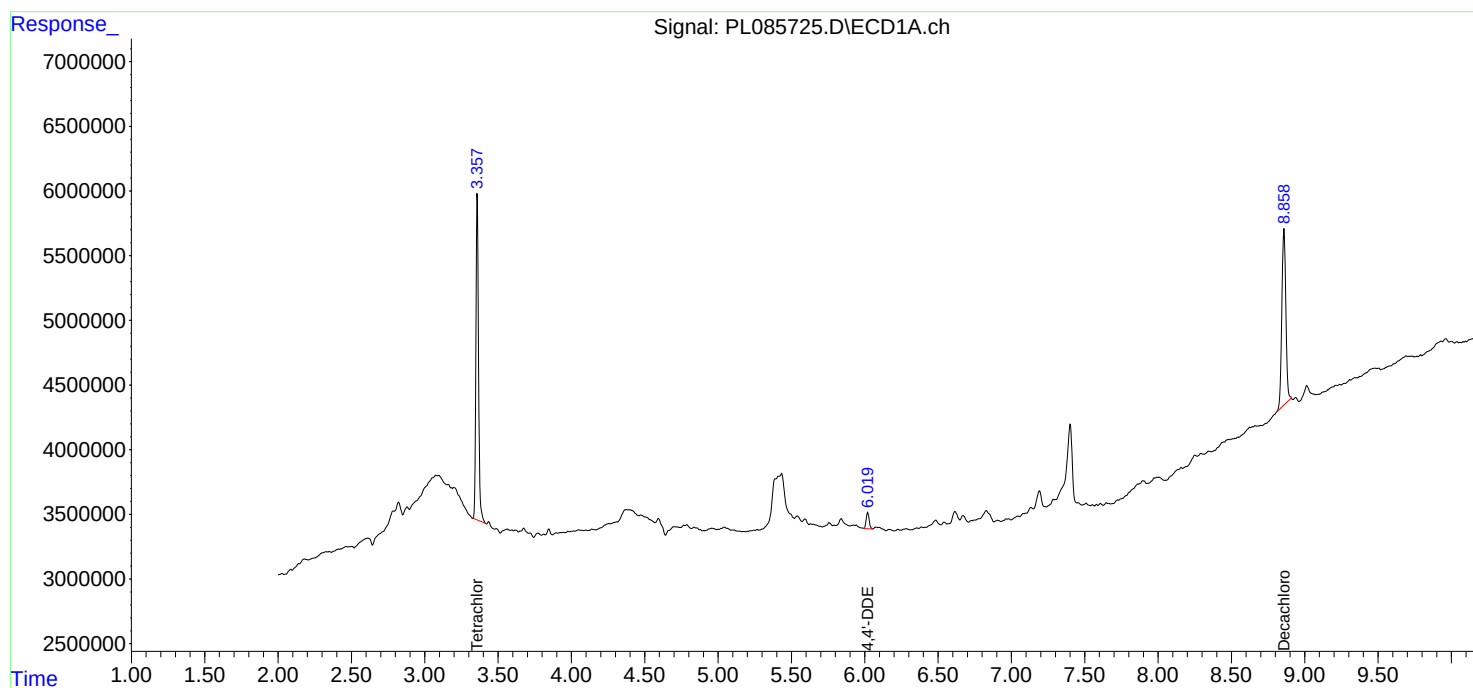

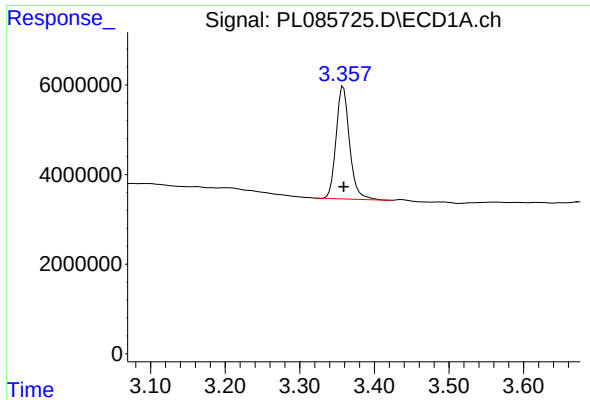


#1 Tetrachloro-m-xylene

R.T.: 3.358 min
Delta R.T.: 0.000 min
Response: 31430231
Conc: 10.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-10-4-2023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

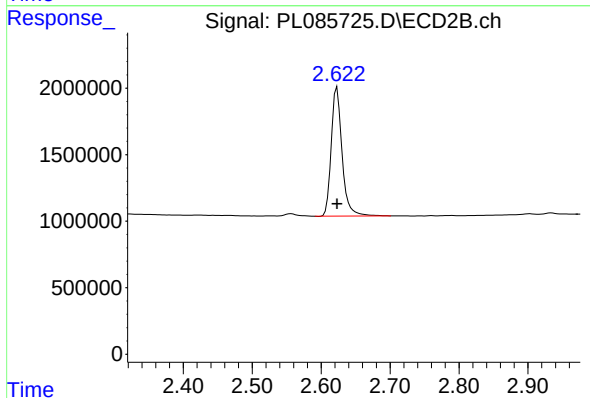


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 10557661
Conc: 11.30 ng/ml

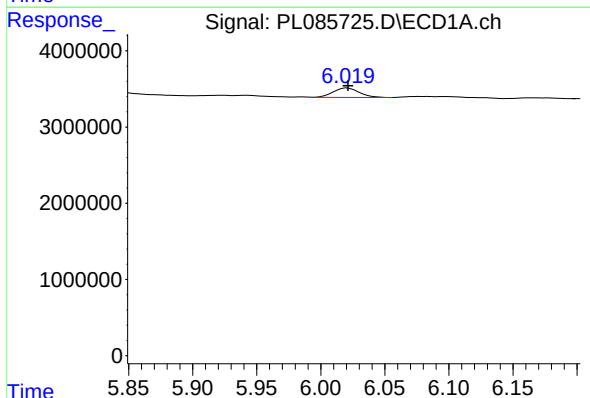


#12 4,4'-DDE

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 1743794
Conc: 0.62 ng/ml

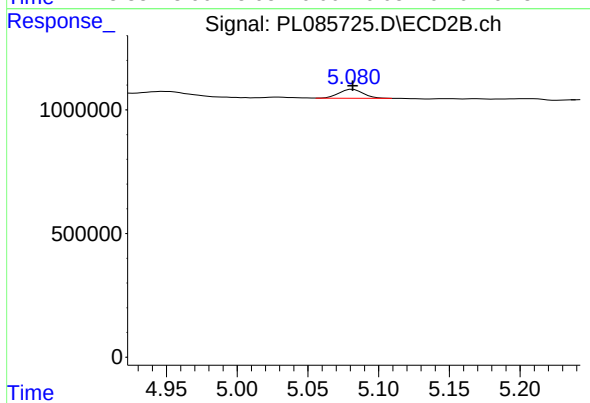

#12 4,4'-DDE

R.T.: 5.080 min
Delta R.T.: -0.001 min
Response: 432663
Conc: 0.53 ng/ml m

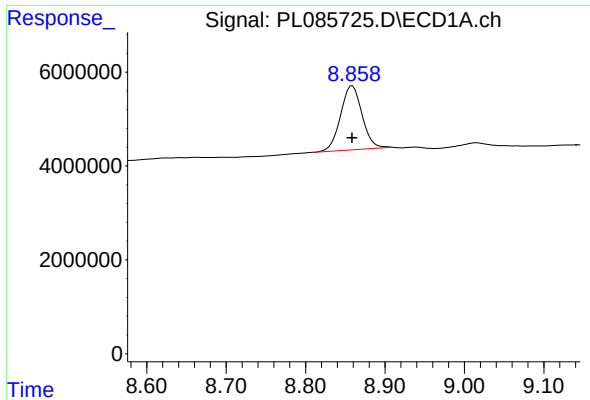


#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 25752790
Conc: 11.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-10-4-2023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

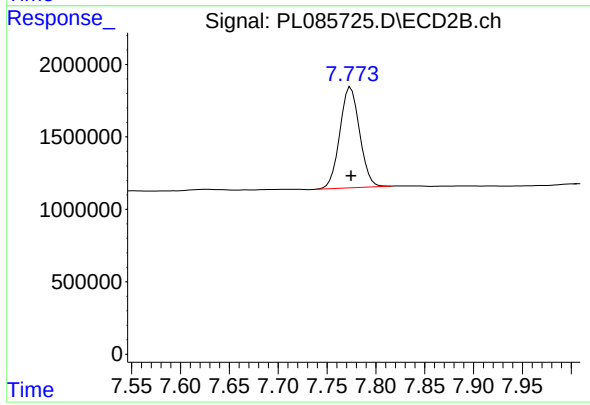

#28 Decachlorobiphenyl

R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 9800071
Conc: 10.62 ng/ml