

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100523\
 Data File : PL085742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2023 20:08
 Operator : AR\AJ
 Sample : 04767-09
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 Q-1(5-10)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/06/2023
 Supervised By : Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 21:28:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.357	2.623	28436067	11036910	9.561m	11.815
28) SA Decachlor...	8.859	7.774	51381022	12815052	23.590m	13.884 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100523\
Data File : PL085742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2023 20:08
Operator : AR\AJ
Sample : 04767-09
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
Q-1(5-10)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/06/2023
Supervised By : Ankita Jodhani 10/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 21:28:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

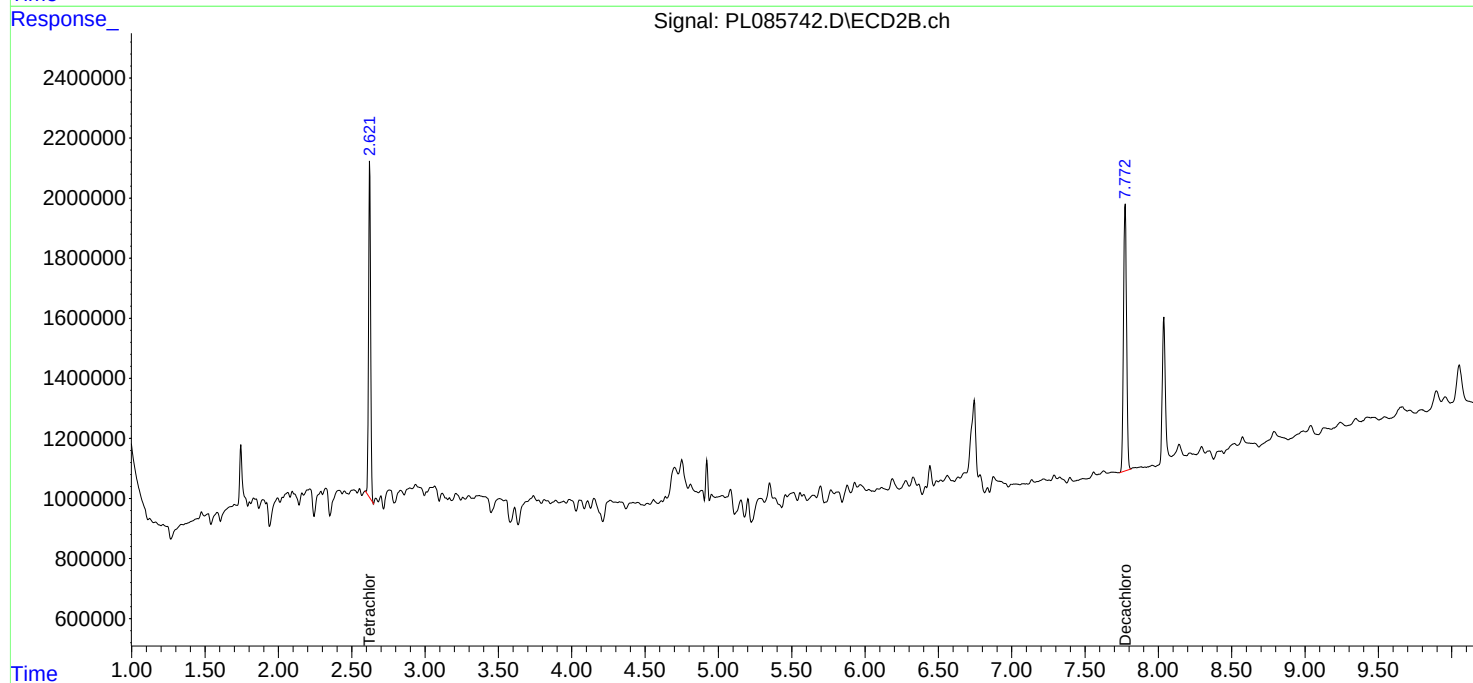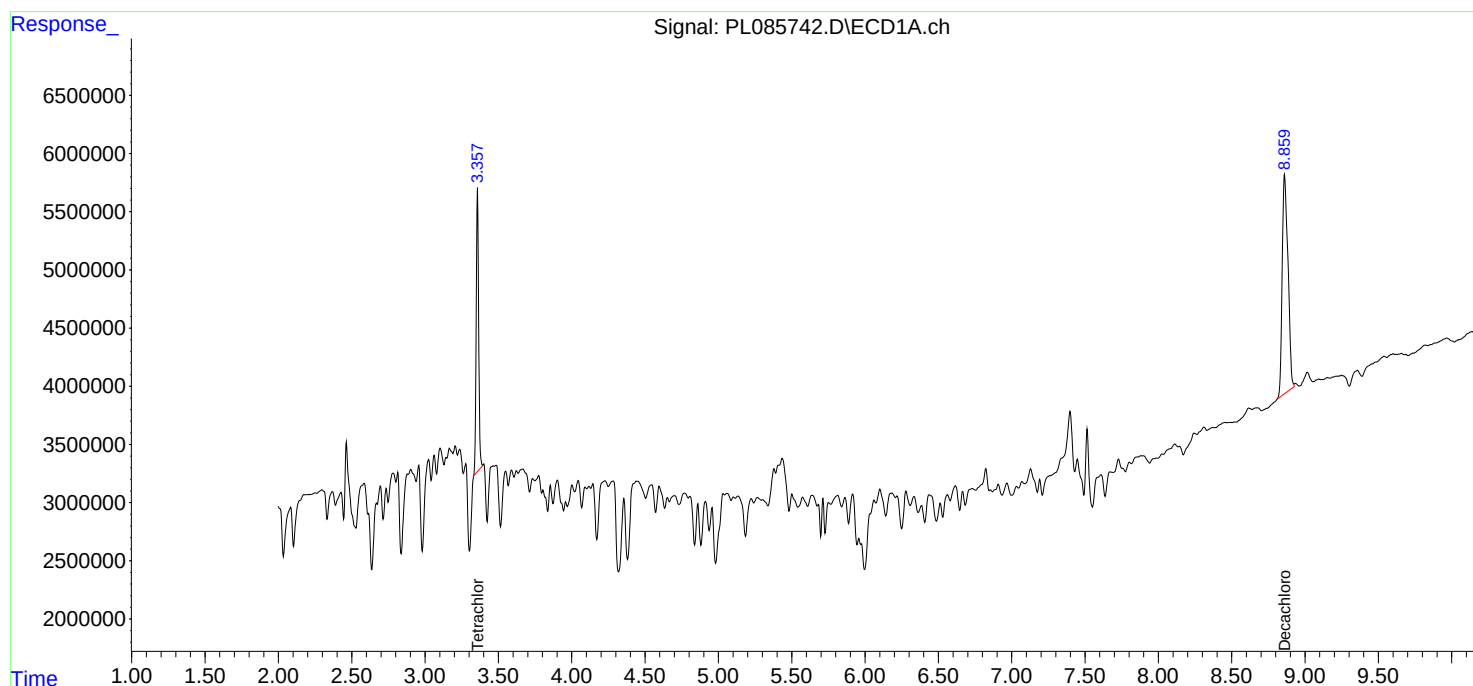

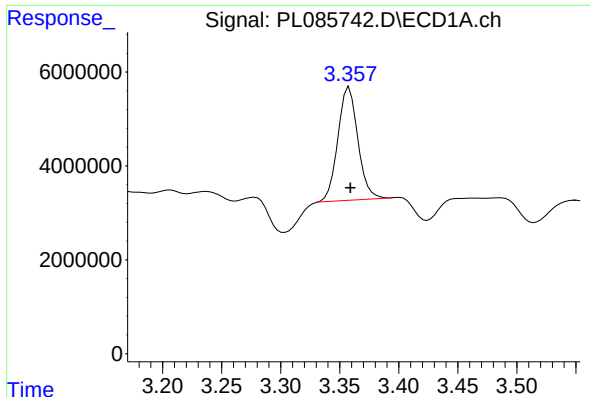


#1 Tetrachloro-m-xylene

R.T.: 3.357 min
Delta R.T.: -0.002 min
Response: 28436067
Conc: 9.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
Q-1(5-10)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/06/2023
Supervised By :Ankita Jodhani 10/06/2023

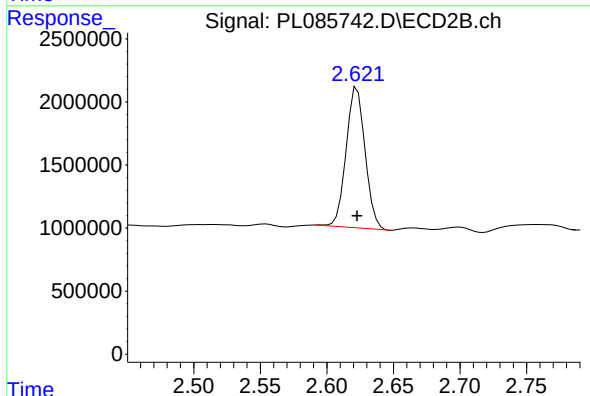


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 11036910
Conc: 11.82 ng/ml

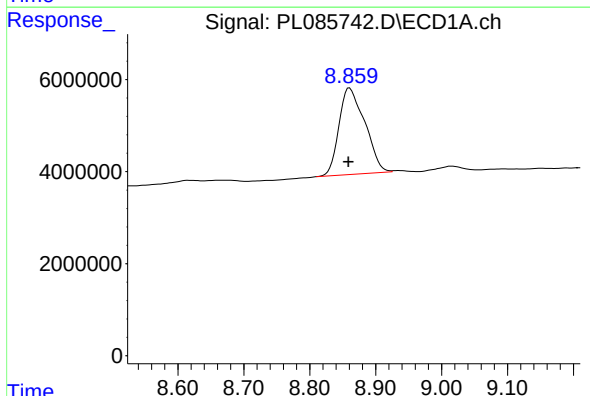

#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 51381022
Conc: 23.59 ng/ml m

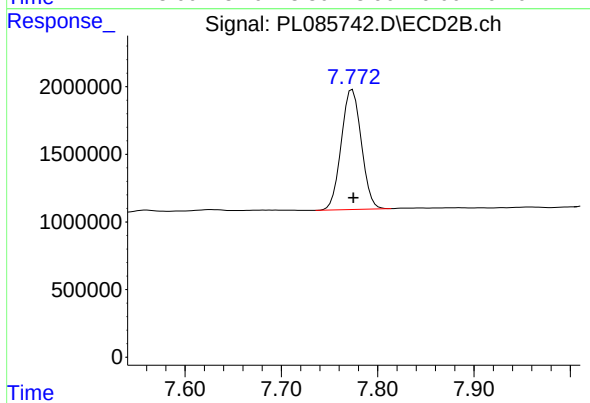

#28 Decachlorobiphenyl

R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 12815052
Conc: 13.88 ng/ml