

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100524\
 Data File : PL092225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Oct 2024 17:49
 Operator : AR\AJ
 Sample : P4258-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 Chamberlain Ave

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/04/2024
 Supervised By :Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 04 02:54:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.781	39305469	45781255	17.668	18.254
28) SA Decachlor...	9.057	7.921	15692554	23482824	9.579m	9.386

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100524\
Data File : PL092225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Oct 2024 17:49
Operator : AR\AJ
Sample : P4258-04
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
Chamberlain Ave


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/04/2024
Supervised By : Ankita Jodhani 10/04/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 04 02:54:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

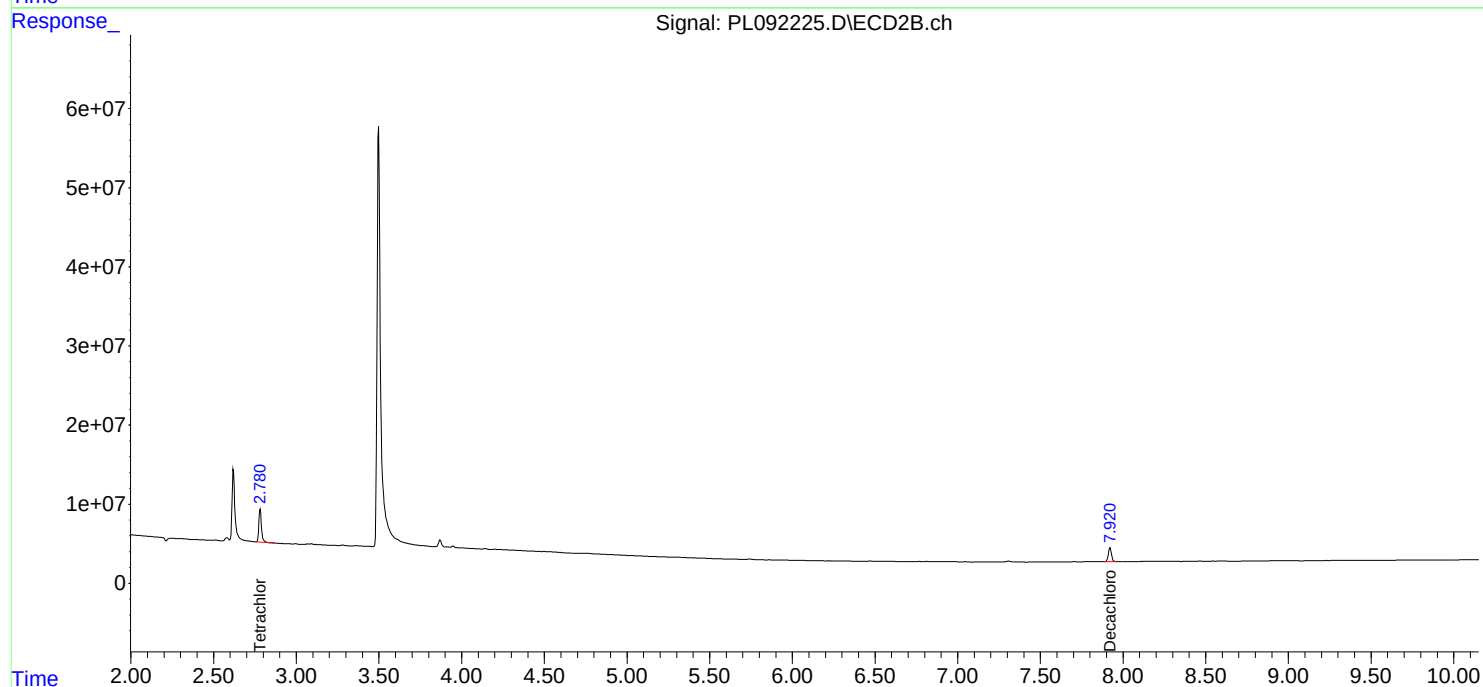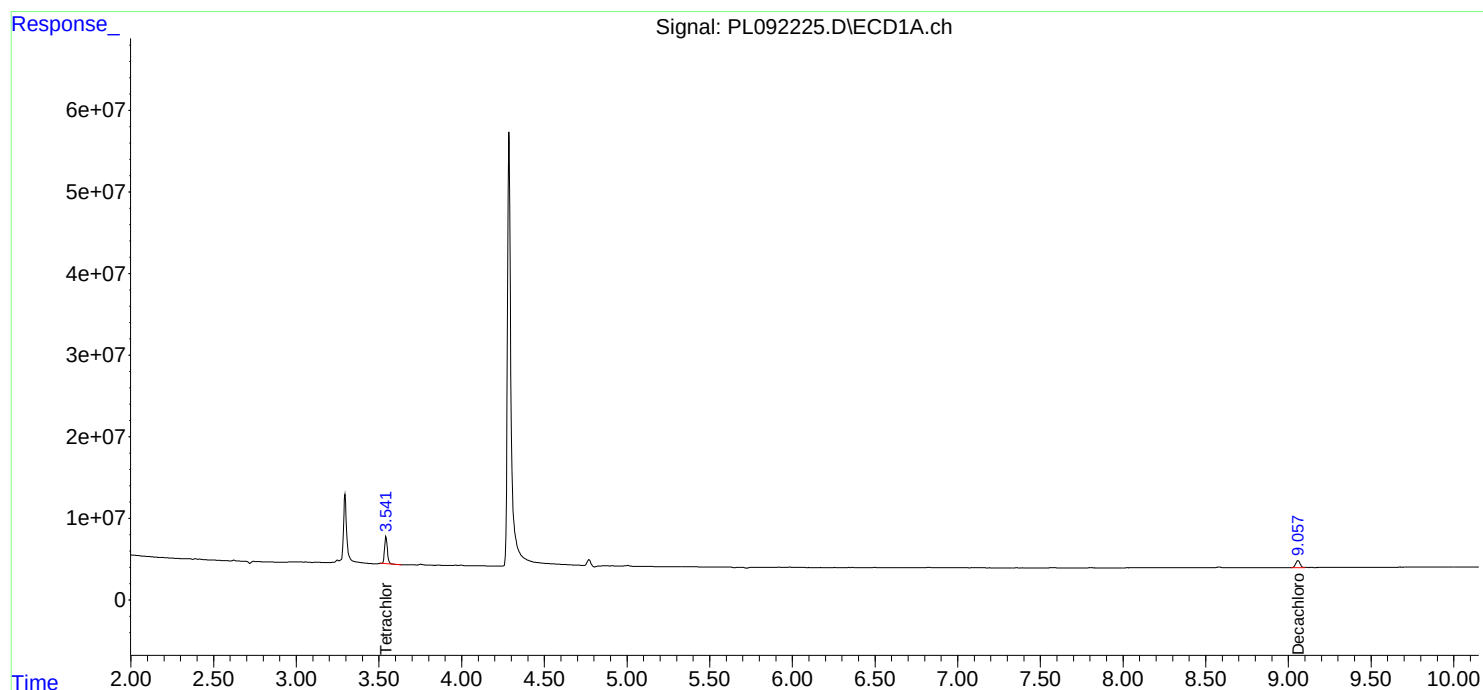

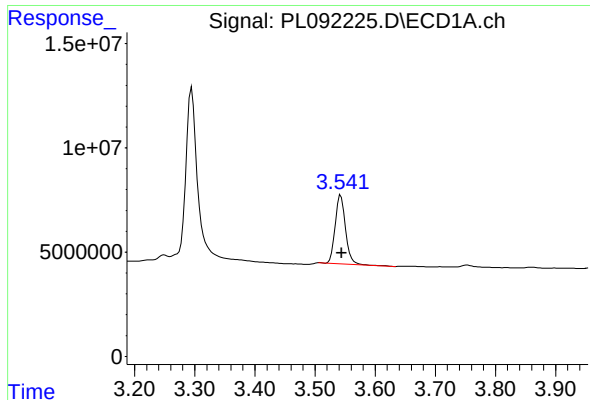

#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 39305469
Conc: 17.67 ng/ml


Instrument :

ECD_L

ClientSampleId :
Chamberlain Ave


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/04/2024
Supervised By :Ankita Jodhani 10/04/2024

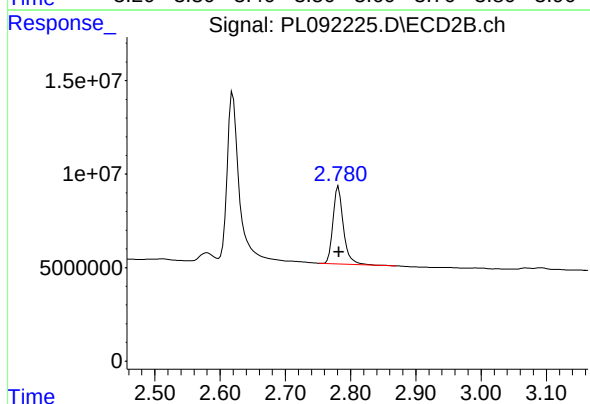


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: 0.000 min
Response: 45781255
Conc: 18.25 ng/ml

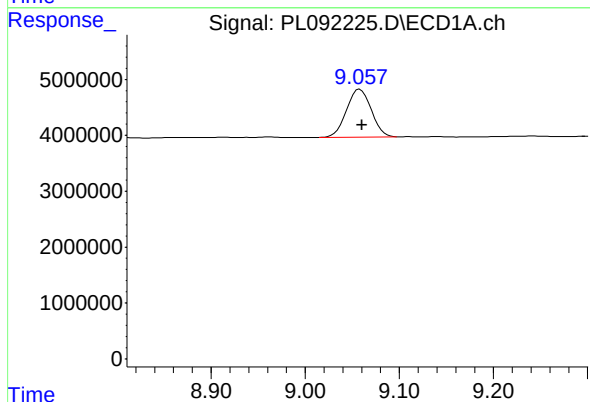

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.004 min
Response: 15692554
Conc: 9.58 ng/ml m

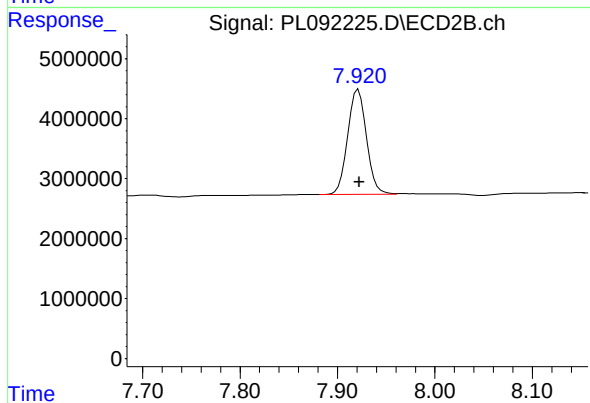

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: -0.001 min
Response: 23482824
Conc: 9.39 ng/ml