

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
 Data File : PL078130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 10:47
 Operator : AR\AJ
 Sample : N4519-01
 Misc : PEST MDL 1PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT4-2022-07

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:02:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.415	2.623	29999081	60299267	17.007	17.922
2)	SA Decachlor...	8.904	7.719	53925847	100.4E6	35.577	37.095
Target Compounds							
2)	A alpha-BHC	3.880	3.115	1967274	4911846	0.783	0.979 #
3)	MA gamma-BHC...	4.215	3.438	1894226	4464456	0.785	0.975
4)	MA Heptachlor	4.791	3.769	1929976	5212022	0.800	1.135 #
5)	MB Aldrin	5.131	4.043	2038773	4722043	0.934	1.058
6)	B beta-BHC	4.429	3.739	1218195	2573192	1.036	1.296 #
7)	B delta-BHC	4.670	3.961	4772258	4660942	1.954	0.992 #
8)	B Heptachlo...	5.565	4.541	1947017	4207637	0.920	1.067
9)	A Endosulfan I	5.950	4.907	1744290	3821077	0.982	1.057
10)	B trans-Chl...	5.819	4.791	1870545	4379892	0.958	1.084
11)	B cis-Chlor...	5.896	4.854	1827198	4182647	0.968	1.085
12)	B 4,4'-DDE	6.076	5.047	1729705	3709467	0.923	0.988
13)	MA Dieldrin	6.228	5.170	1500324	3998188	0.807	1.028 #
14)	MA Endrin	6.459	5.443	1410879	3546247	0.875	1.100 #
15)	B Endosulfa...	6.689	5.739	2172233	3496342	1.346	1.106
16)	A 4,4'-DDD	6.600	5.600	1241256	3350152	0.915	1.109
17)	MA 4,4'-DDT	6.912	5.849	1309669	2652627	0.900	0.878
18)	B Endrin al...	6.820	5.918	1199613	2862241	0.891	1.107
19)	B Endosulfa...	7.052	6.142	1469029	3647178	0.989	1.177
20)	A Methoxychlor	7.392	6.426	777944	1729508	1.037	1.162
21)	B Endrin ke...	7.541	6.640	1632979	3368977	1.016	1.014

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
Data File : PL078130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 10:47
Operator : AR\AJ
Sample : N4519-01
Misc : PEST MDL 1PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:02:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

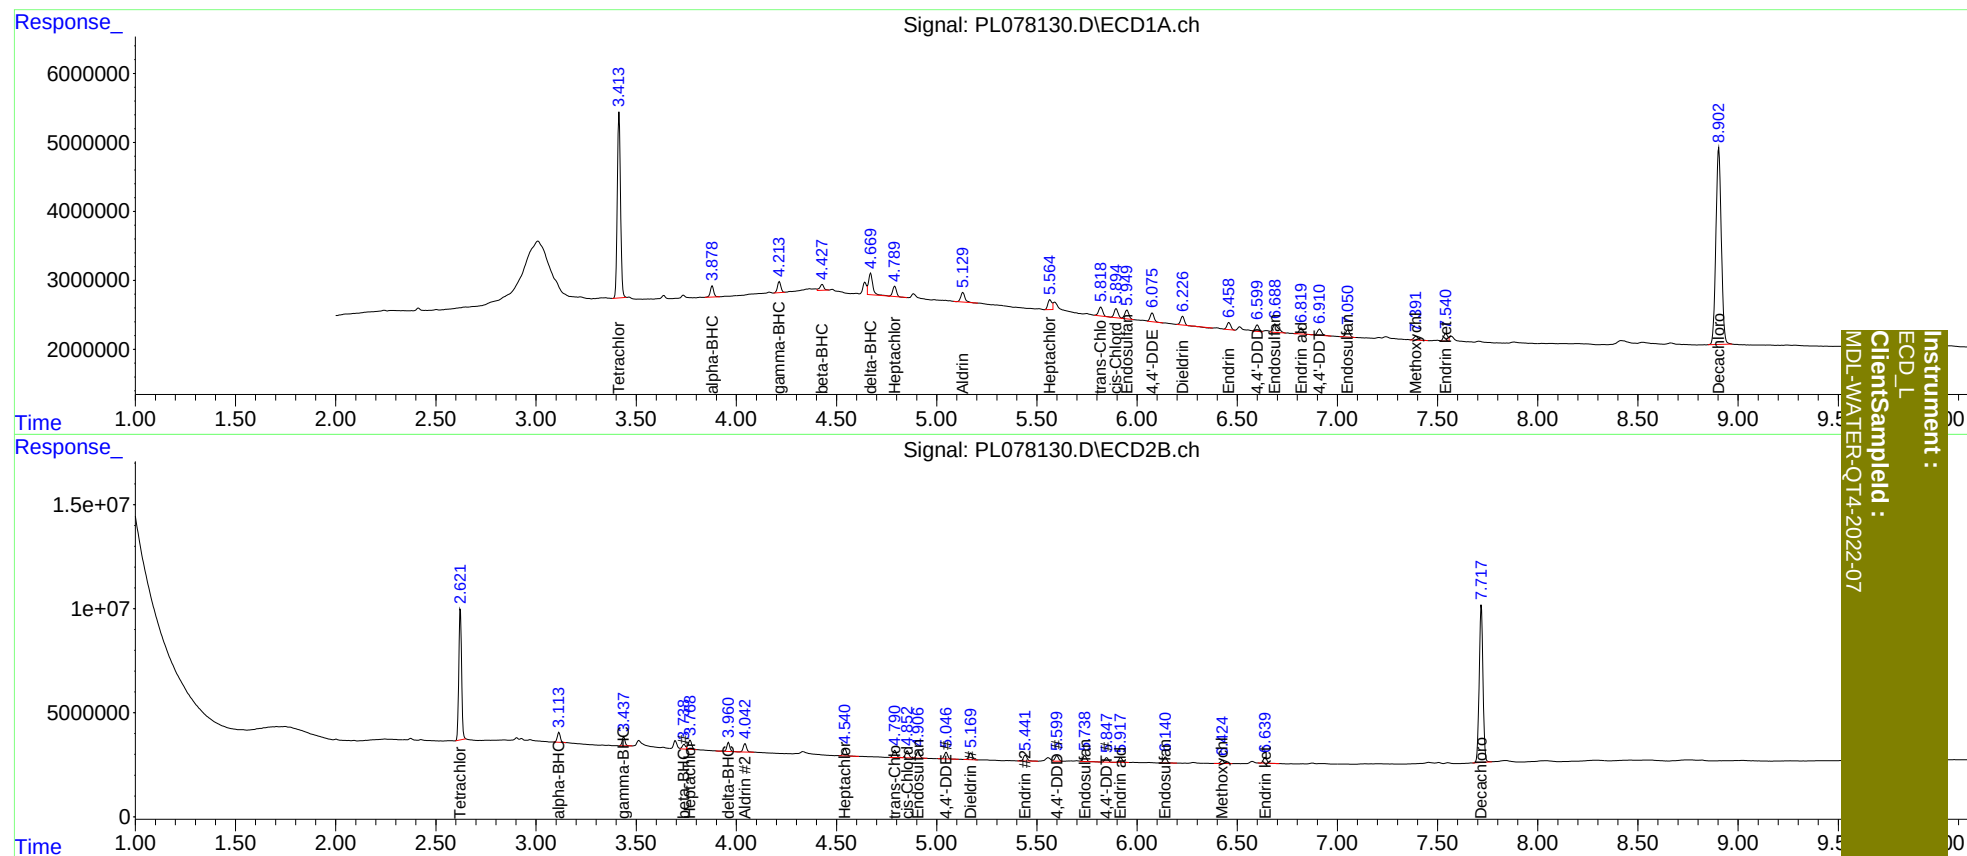

Instrument :
ECD_L
ClientSample :
MDL-WATER-QT4-2022-07