

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
 Data File : PL078148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 16:33
 Operator : AR\AJ
 Sample : N4847-02MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB8P5MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:25:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	33632721	60804168	19.067	18.073
2)	SA Decachlor...	8.901	7.717	50895892	97624203	33.578	36.053
Target Compounds							
2)	A alpha-BHC	3.879	3.115	113.8E6	239.3E6	45.274	47.679
3)	MA gamma-BHC...	4.214	3.438	110.8E6	228.0E6	45.906	49.790
4)	MA Heptachlor	4.789	3.769	108.3E6	219.3E6	44.901	47.732
5)	MB Aldrin	5.130	4.043	102.9E6	221.1E6	47.130	49.569
6)	B beta-BHC	4.427	3.739	49101145	92162177	41.741	46.421
7)	B delta-BHC	4.671	3.961	49333036	108.3E6	20.194	23.033
8)	B Heptachlo...	5.563	4.542	93791752	196.9E6	44.331	49.903
9)	A Endosulfan I	5.949	4.907	84037637	183.7E6	47.305	50.803
10)	B trans-Chl...	5.818	4.791	90748686	194.7E6	46.469	48.169
11)	B cis-Chlor...	5.895	4.854	89018555	189.2E6	47.182	49.062
12)	B 4,4'-DDE	6.075	5.048	181.5E6	376.1E6	96.850	100.170
13)	MA Dieldrin	6.227	5.170	186.5E6	396.0E6	100.262	101.816
14)	MA Endrin	6.458	5.443	159.6E6	346.6E6	98.944	107.474
15)	B Endosulfa...	6.686	5.739	154.8E6	322.1E6	95.931	101.844
16)	A 4,4'-DDD	6.600	5.600	134.4E6	304.2E6	99.020	100.732
17)	MA 4,4'-DDT	6.910	5.849	144.3E6	320.0E6	99.153	105.913
18)	B Endrin al...	6.817	5.918	122.0E6	252.1E6	90.625	97.513
19)	B Endosulfa...	7.050	6.141	123.0E6	267.8E6	82.853	86.391
20)	A Methoxychlor	7.392	6.426	361.4E6	730.6E6	481.868	490.879
21)	B Endrin ke...	7.539	6.640	161.2E6	346.8E6	100.254	104.374

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
Data File : PL078148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 16:33
Operator : AR\AJ
Sample : N4847-02MS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:25:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

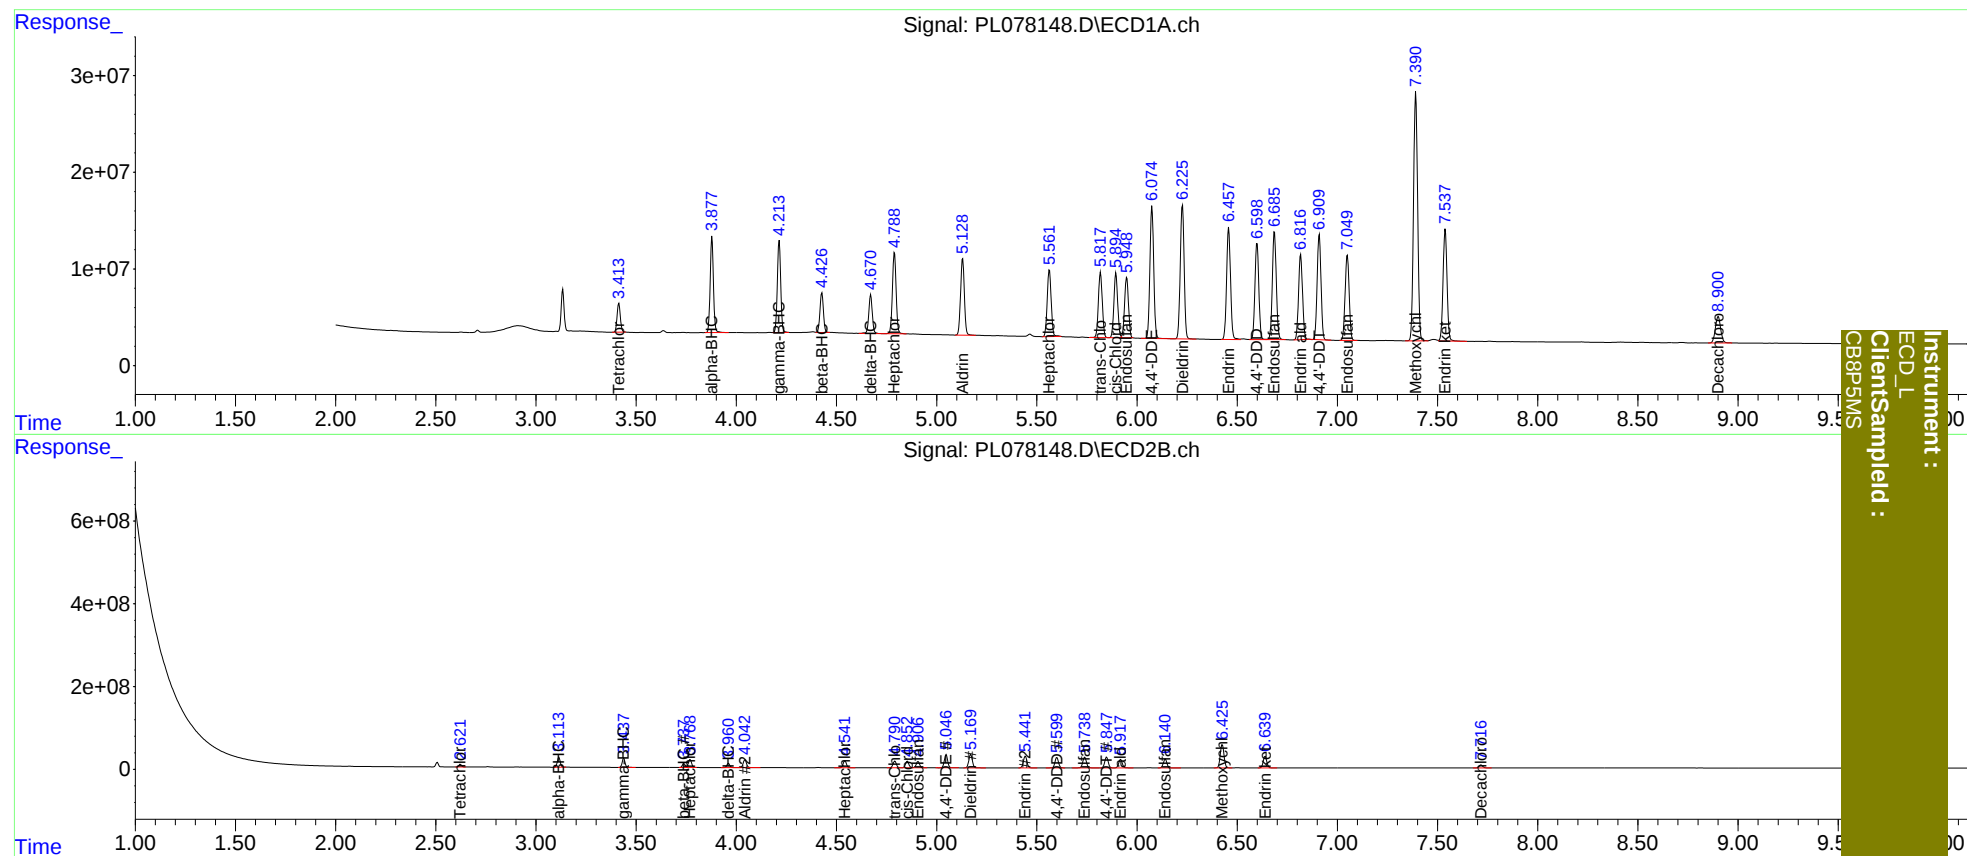

Instrument :
ECD_L
ClientSampled :
CB8P5MS