

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
 Data File : PL078149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 16:47
 Operator : AR\AJ
 Sample : N4847-03MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB8P5MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:26:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	2.622	33727786	61151918	19.121	18.176
2)	SA Decachlor...	8.902	7.717	50637302	98115225	33.408	36.234
Target Compounds							
2)	A alpha-BHC	3.878	3.114	113.8E6	241.0E6	45.278	48.018
3)	MA gamma-BHC...	4.213	3.438	110.5E6	229.4E6	45.808	50.114
4)	MA Heptachlor	4.789	3.769	108.0E6	220.2E6	44.800	47.936
5)	MB Aldrin	5.129	4.043	102.7E6	222.3E6	47.043	49.833
6)	B beta-BHC	4.426	3.738	52746451	92577551	44.840	46.631
7)	B delta-BHC	4.670	3.960	49657558	108.7E6	20.327	23.131
8)	B Heptachlo...	5.562	4.541	94081815	198.3E6	44.468	50.255
9)	A Endosulfan I	5.949	4.906	84425567	185.1E6	47.523	51.184
10)	B trans-Chl...	5.818	4.790	90825284	196.0E6	46.508	48.493
11)	B cis-Chlor...	5.895	4.852	89216085	190.6E6	47.287	49.422
12)	B 4,4'-DDE	6.074	5.046	181.6E6	379.2E6	96.877	100.997
13)	MA Dieldrin	6.226	5.169	186.9E6	399.0E6	100.489	102.590
14)	MA Endrin	6.457	5.442	160.1E6	349.7E6	99.259	108.426
15)	B Endosulfa...	6.686	5.738	155.5E6	324.0E6	96.368	102.439
16)	A 4,4'-DDD	6.599	5.599	134.7E6	306.4E6	99.278	101.447
17)	MA 4,4'-DDT	6.910	5.848	144.7E6	322.6E6	99.407	106.772
18)	B Endrin al...	6.817	5.917	122.5E6	253.5E6	91.020	98.065
19)	B Endosulfa...	7.051	6.140	123.5E6	268.9E6	83.173	86.761
20)	A Methoxychlor	7.391	6.425	362.3E6	733.1E6	483.094	492.565
21)	B Endrin ke...	7.538	6.640	161.9E6	349.0E6	100.713	105.017

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
Data File : PL078149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 16:47
Operator : AR\AJ
Sample : N4847-03MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:26:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

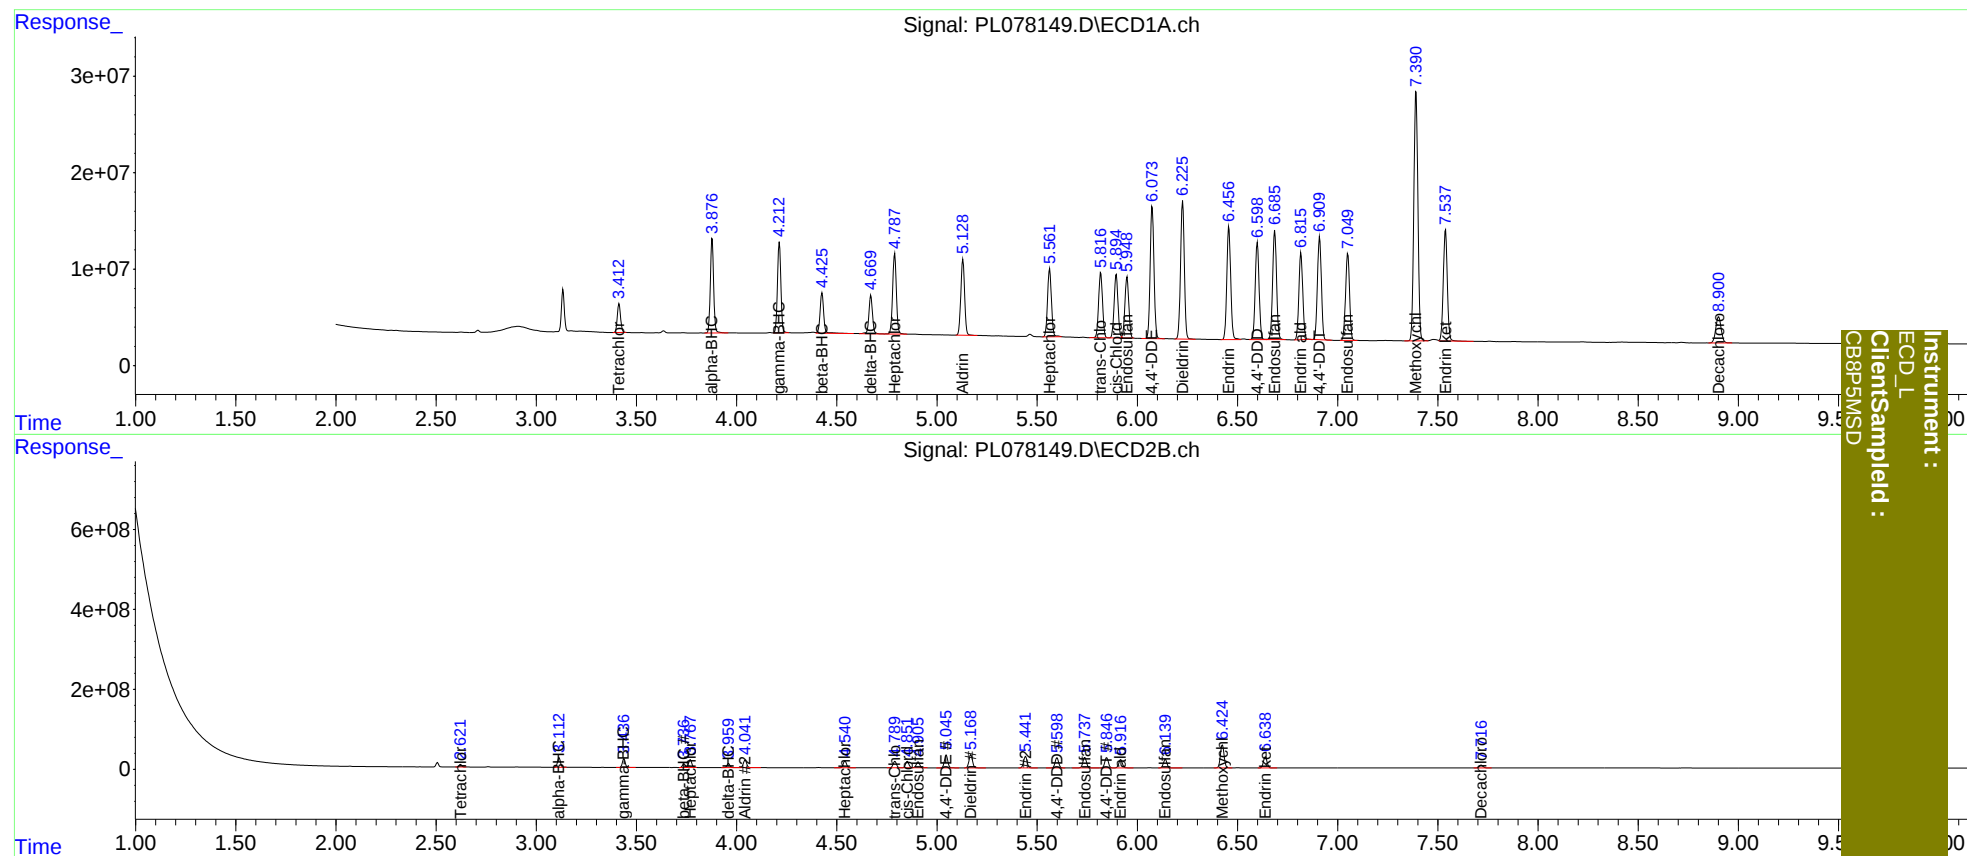

Instrument :
ECD_L
ClientSampled :
CB8P5MSD