

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
 Data File : PL078151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 17:15
 Operator : AR\AJ
 Sample : N4847-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB8Q5

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/07/2022
 Supervised By : Ankita Jodhani 10/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 05 23:28:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.623	25069528	51915087	14.213	15.430
2)	SA Decachlor...	8.904	7.720	37297495	67154783	24.607m	24.801
Target Compounds							
7)	B delta-BHC	4.668	3.967	2910256	2100726	1.191	0.447 #
20)	A Methoxychlor	7.390	6.425	1002773	4562499	1.337	3.066 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
Data File : PL078151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 17:15
Operator : AR\AJ
Sample : N4847-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 05 23:28:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

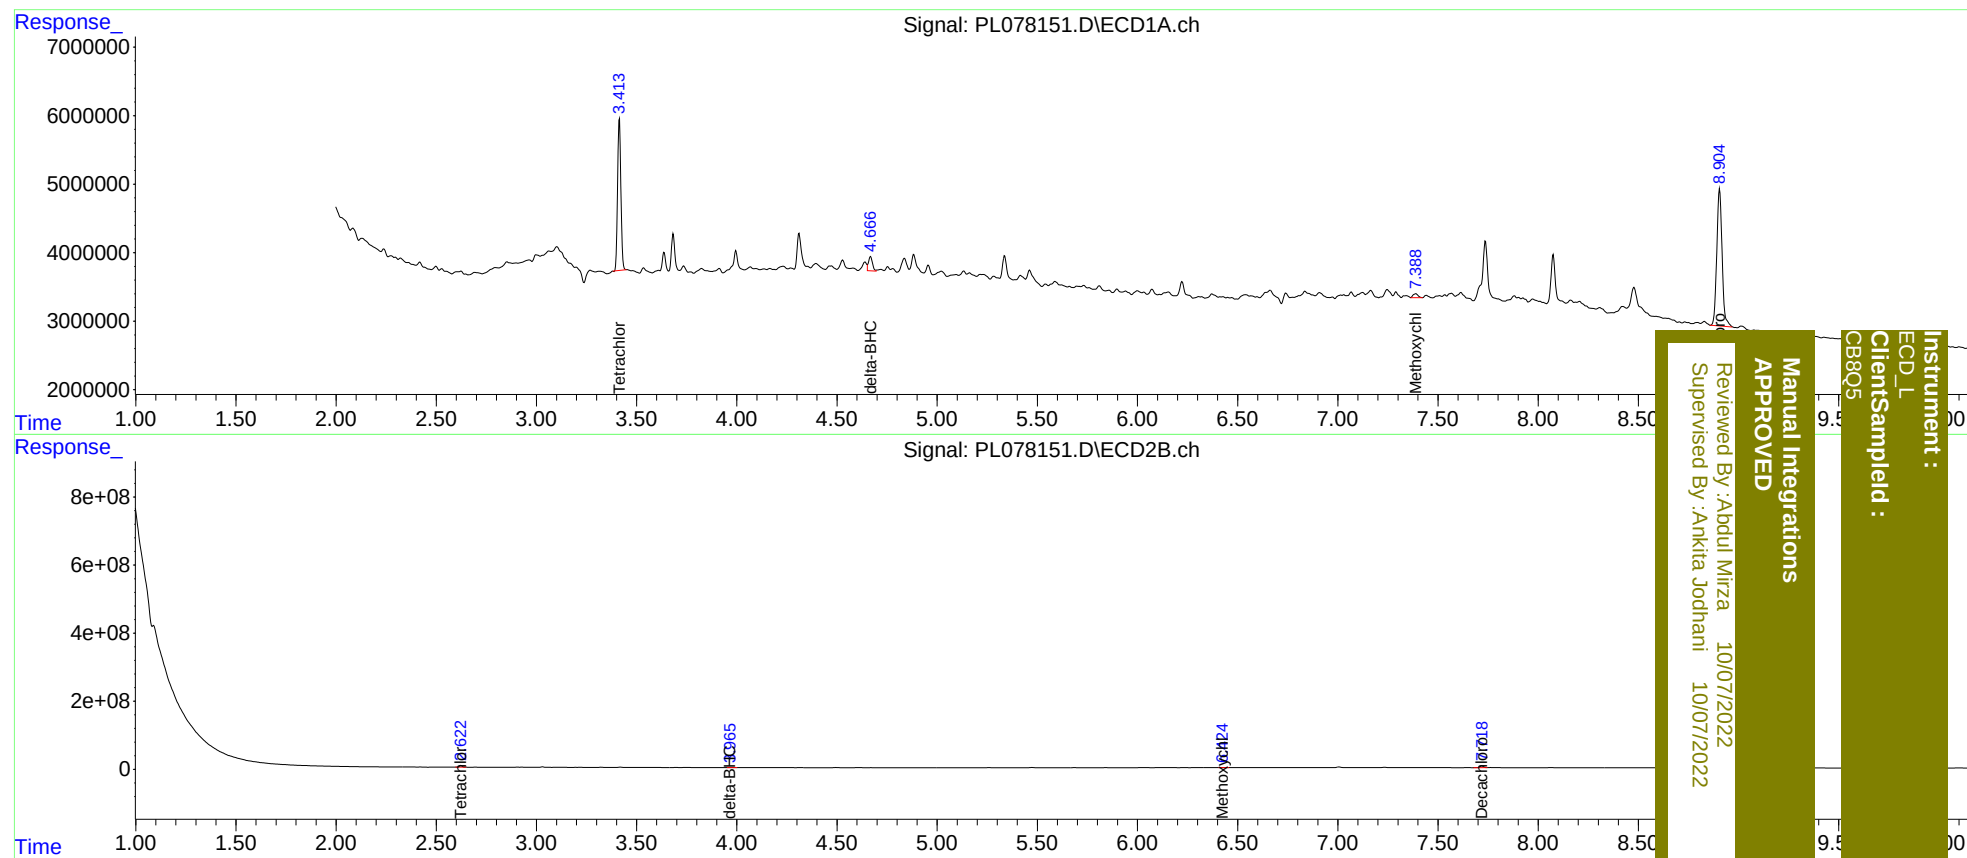

Reviewed By: Abdul Mirza 10/07/2022
Supervised By: Ankita Jodhani 10/07/2022

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
CB805