

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
 Data File : PL078162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 20:56
 Operator : AR\AJ
 Sample : N4956-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB8R8

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/07/2022
 Supervised By :Ankita Jodhani 10/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 06:52:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	2.623	29465737	52398006	16.705	15.574
2)	SA Decachlor...	8.901	7.718	49425897	78335129	32.609	28.930
Target Compounds							
13)	MA Dieldrin	6.224	5.170	3787786	7387202	2.036m	1.899
17)	MA 4,4'-DDT	6.901	5.876	748271	10642653	0.514m	3.523m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
Data File : PL078162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 20:56
Operator : AR\AJ
Sample : N4956-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 06:52:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

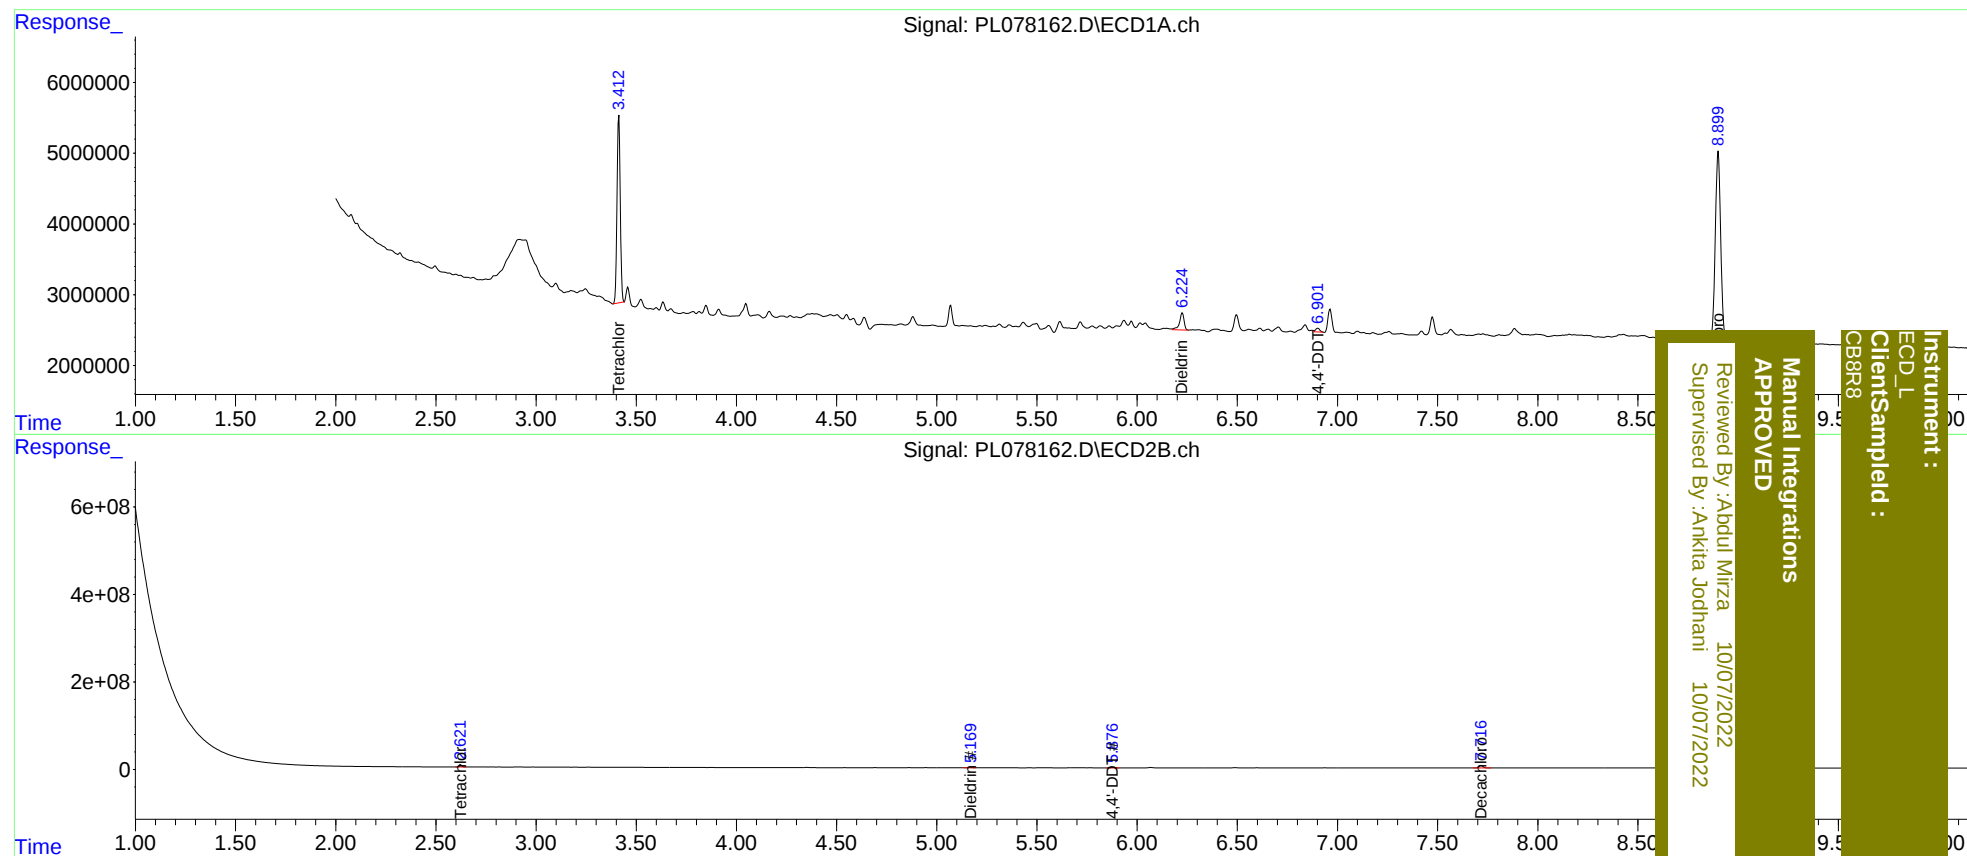

Reviewed By: Abdul Mirza 10/07/2022
Supervised By: Ankita Jodhani 10/07/2022

Manual Integrations
APPROVED

Instrument :
ECD_L
ClientSampled :
CB8R8