

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
 Data File : PL078165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Oct 2022 21:37
 Operator : AR\AJ
 Sample : N4956-12
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CB8W3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/07/2022
 Supervised By : Ankita Jodhani 10/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 07:15:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 05 01:39:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.413	2.623	28459999	50558117	16.135	15.027
2) SA Decachlor...	8.901	7.718	49362458	77868202	32.567	28.757
Target Compounds						
9) A Endosulfan I	5.935	4.896	900951	1772068	0.507	0.490
13) MA Dieldrin	6.224	5.168	4145609	9193782	2.229m	2.364m
17) MA 4,4'-DDT	6.903	5.876	1142551	11359744	0.785	3.760m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100622\
Data File : PL078165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Oct 2022 21:37
Operator : AR\AJ
Sample : N4956-12
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 07:15:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100522CLP.M
Quant Title : GC Extractables
QLast Update : Wed Oct 05 01:39:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

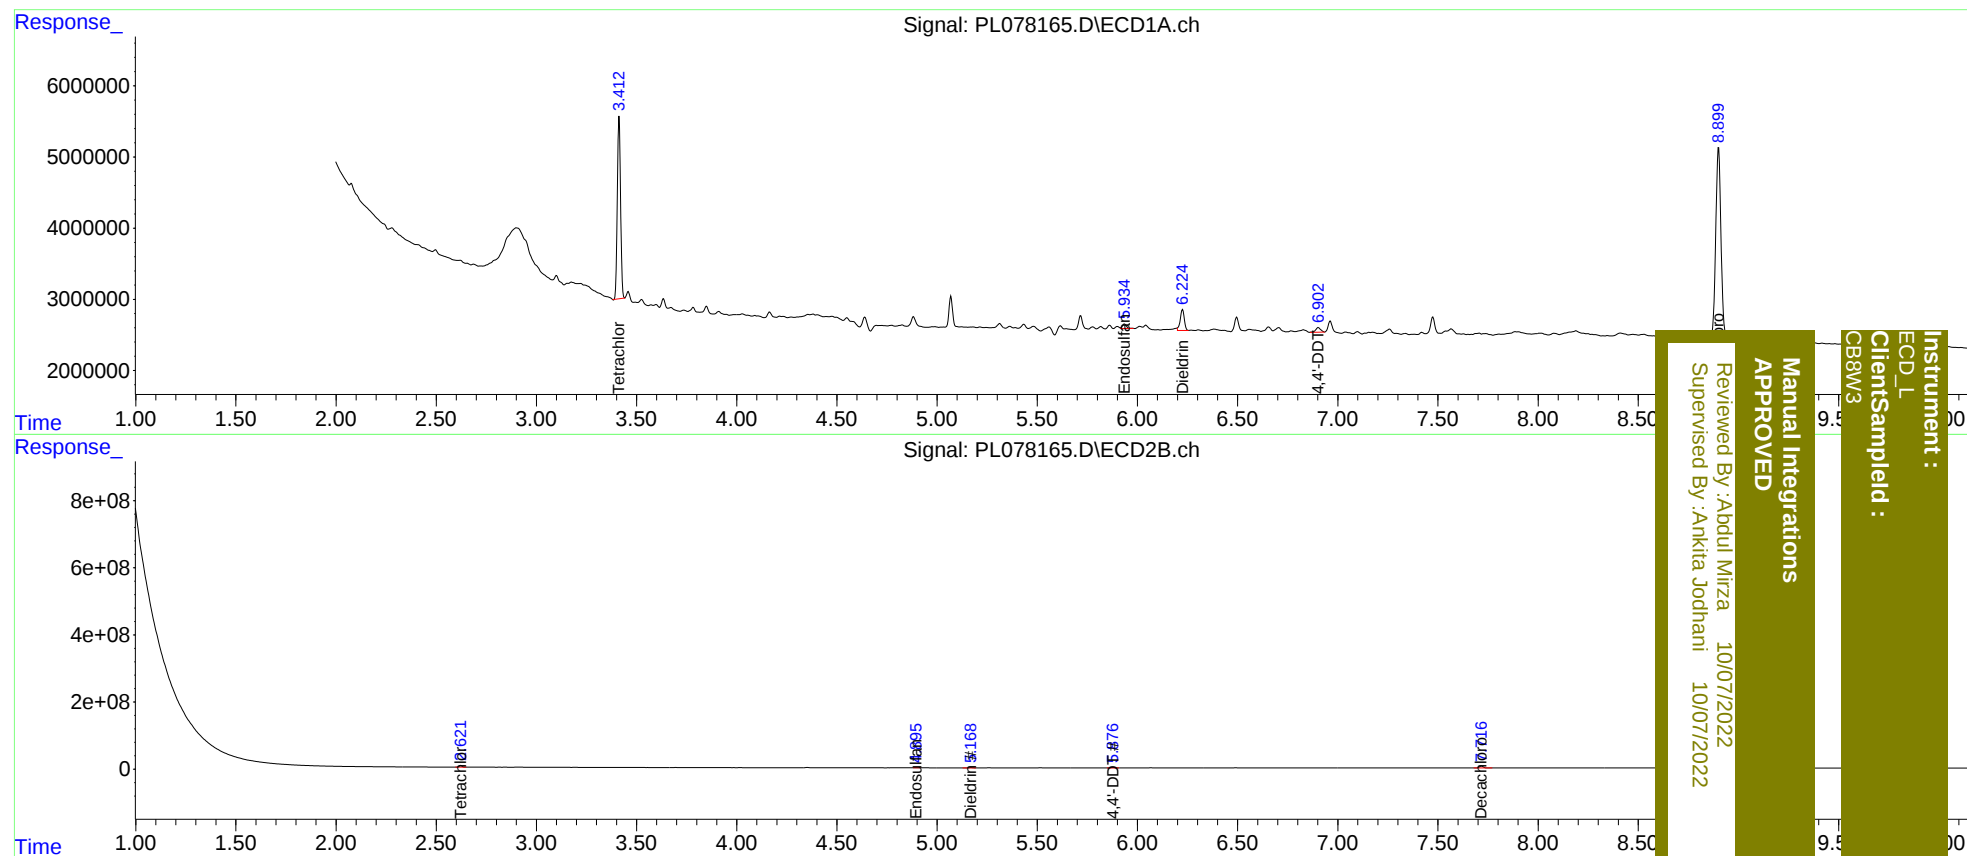

Reviewed By: Abdul Mirza 10/07/2022
Supervised By: Ankita Jodhani 10/07/2022

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sampled :
CB8W3