

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100623\
 Data File : PL085758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2023 15:04
 Operator : AR\AJ
 Sample : PEST,PCB,SUR/SPIK200PPB
 Misc :
 ALS Vial : 100 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PEST,PCB,SUR/SPIK200PPB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 16:05:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.623	553.1E6	183.9E6	185.966	196.898
28)	SA Decachlor...	8.858	7.774	447.0E6	184.2E6	205.245	199.566

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100623\
Data File : PL085758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2023 15:04
Operator : AR\AJ
Sample : PEST,PCB,SUR/SPIK200PPB
Misc :
ALS Vial : 100 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PEST,PCB,SUR/SPIK200PPB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 16:05:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

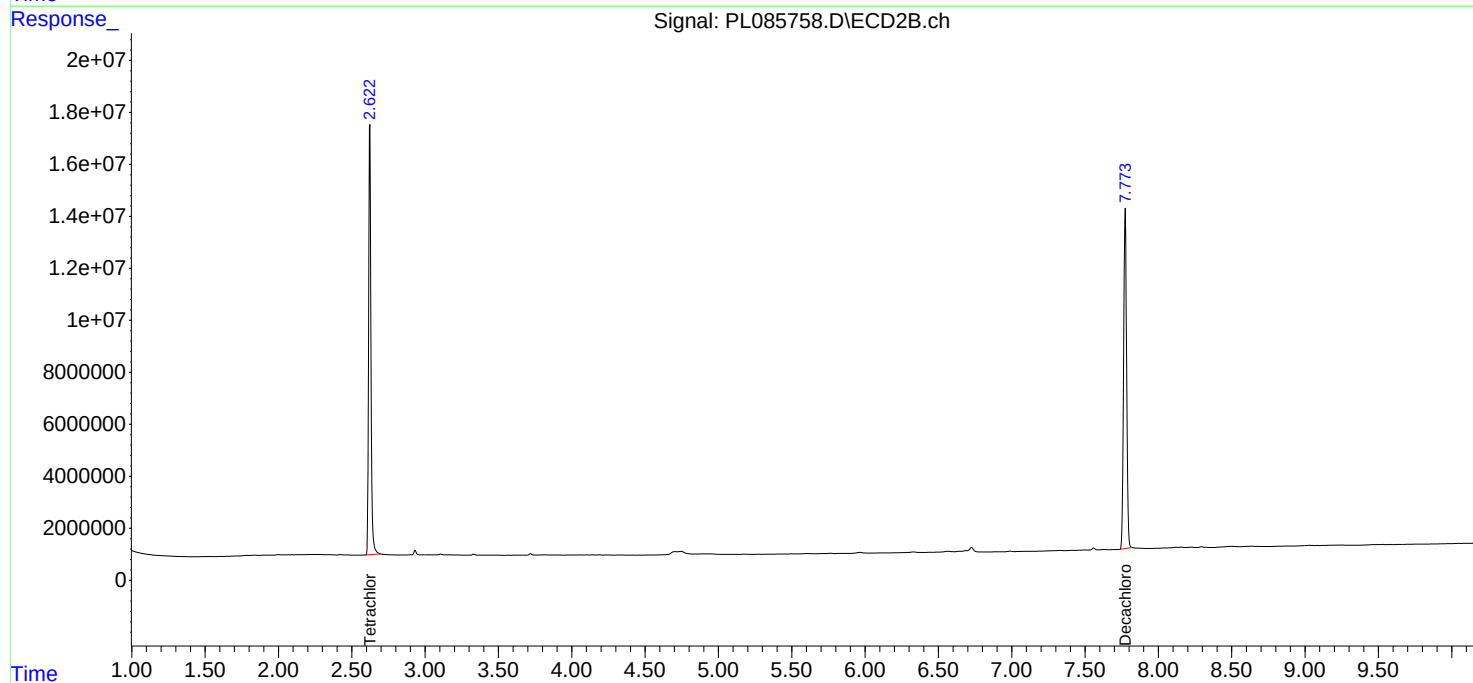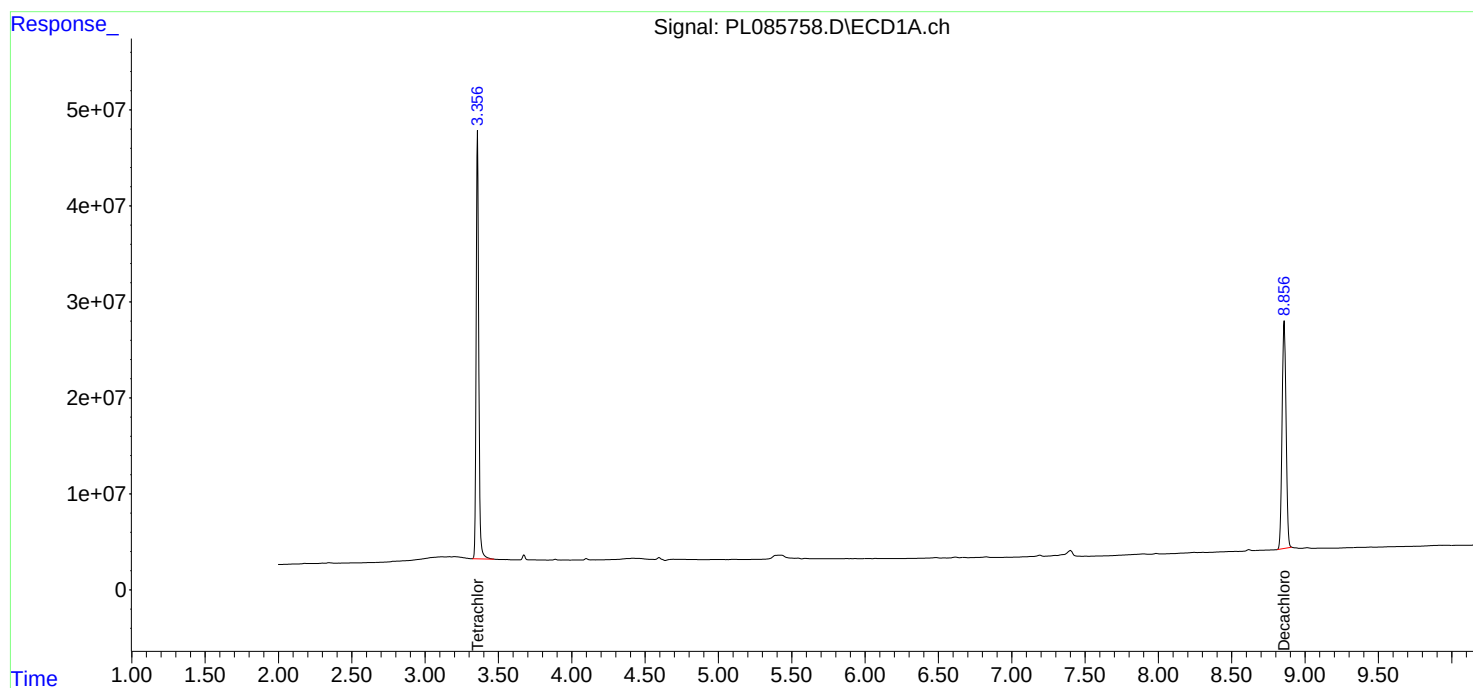


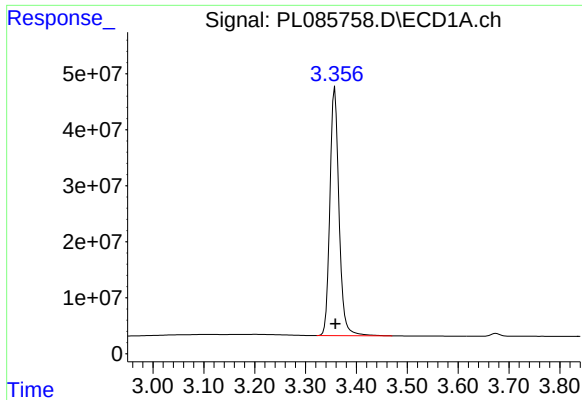

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.001 min
Response: 553090802
Conc: 185.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEST,PCB,SUR/SPIK200PPB

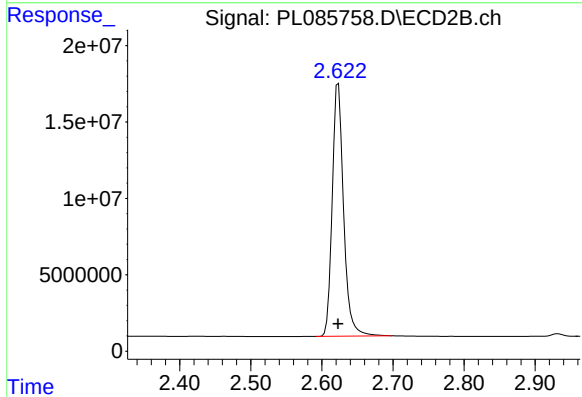


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 183924911
Conc: 196.90 ng/ml

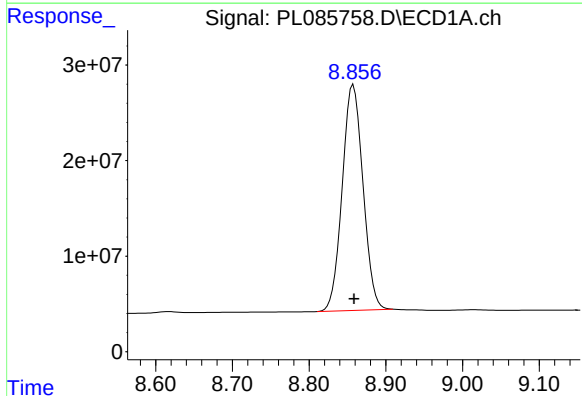

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: -0.001 min
Response: 447035473
Conc: 205.25 ng/ml

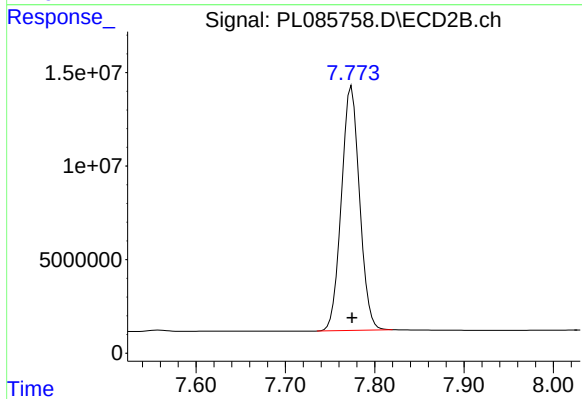

#28 Decachlorobiphenyl

R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 184196473
Conc: 199.57 ng/ml