

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100623\
 Data File : PL085759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Oct 2023 15:18
 Operator : AR\AJ
 Sample : 04784-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-10052023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/09/2023
 Supervised By :Ankita Jodhani 10/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 06 16:06:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	2.623	35042327	11679655	11.782	12.503
2)	SA Decachlor...	8.859	7.774	28724890	11006851	13.188	11.925
Target Compounds							
11)	B alpha-Chl...	5.840	4.880	2527719	495018	0.740m	0.454m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100623\
Data File : PL085759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Oct 2023 15:18
Operator : AR\AJ
Sample : 04784-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-10052023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/09/2023
Supervised By : Ankita Jodhani 10/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 06 16:06:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

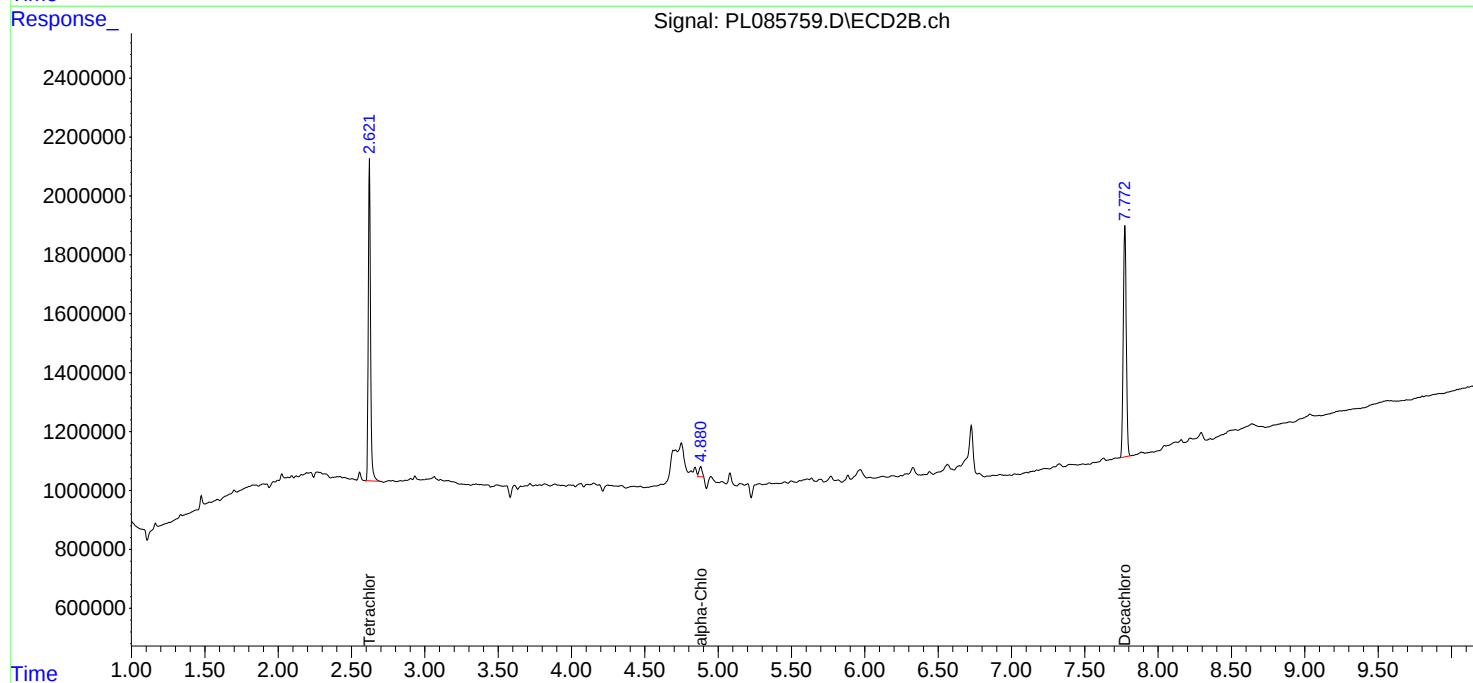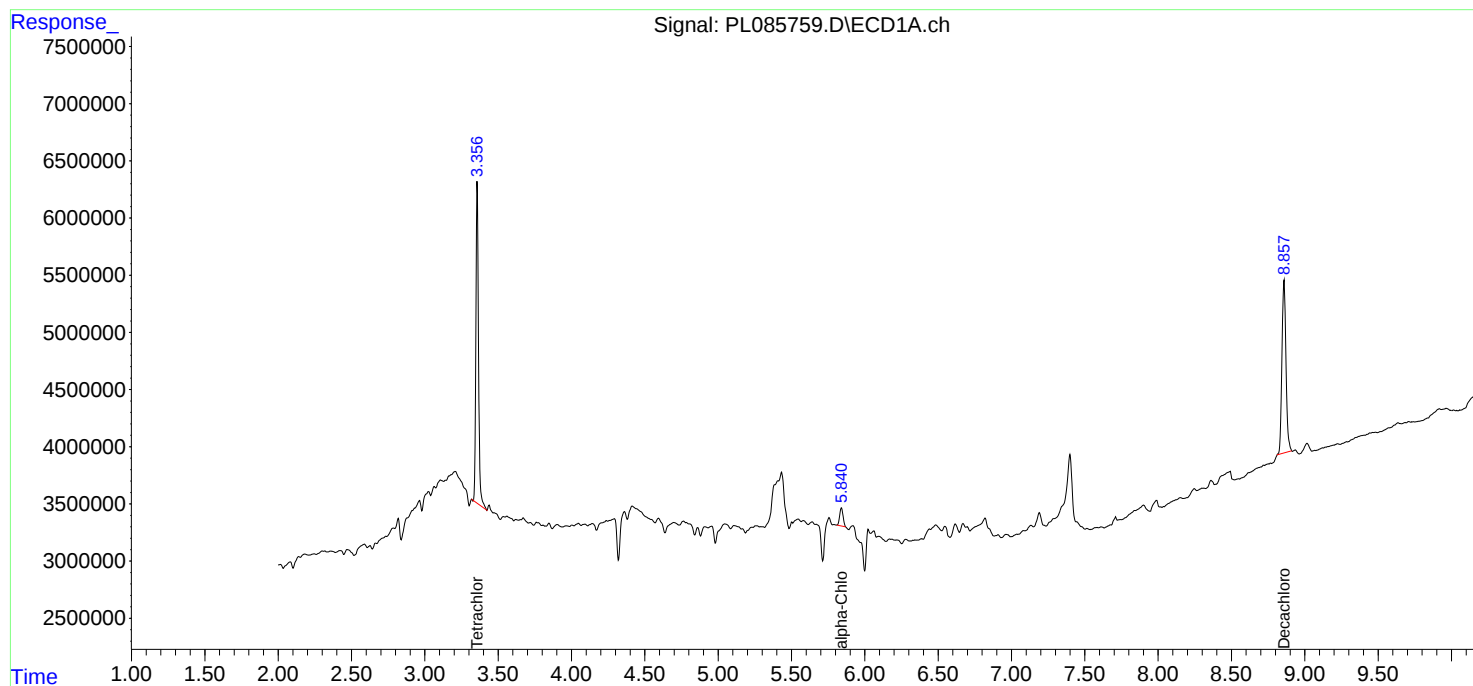

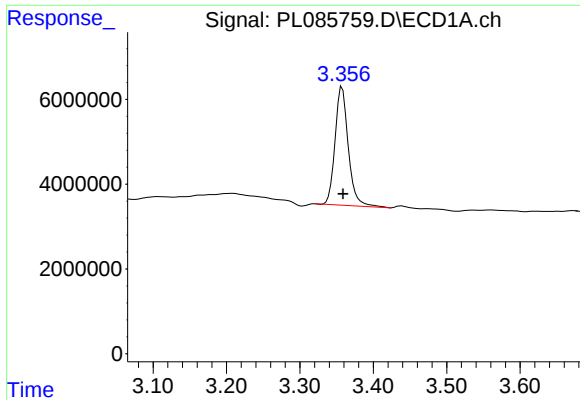


#1 Tetrachloro-m-xylene

R.T.: 3.358 min
Delta R.T.: -0.001 min
Response: 35042327
Conc: 11.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-10052023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/09/2023
Supervised By :Ankita Jodhani 10/09/2023

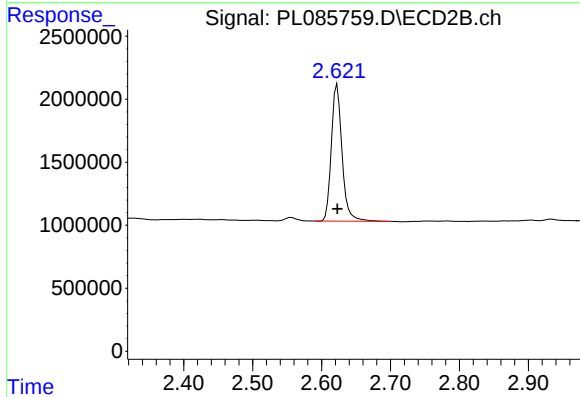


#1 Tetrachloro-m-xylene

R.T.: 2.623 min
Delta R.T.: 0.000 min
Response: 11679655
Conc: 12.50 ng/ml

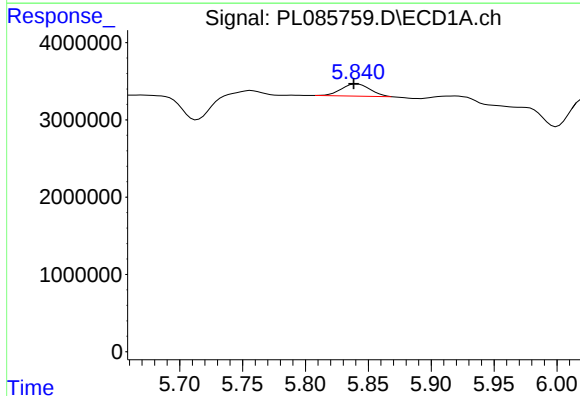


#11 alpha-Chlordane

R.T.: 5.840 min
Delta R.T.: 0.001 min
Response: 2527719
Conc: 0.74 ng/ml m

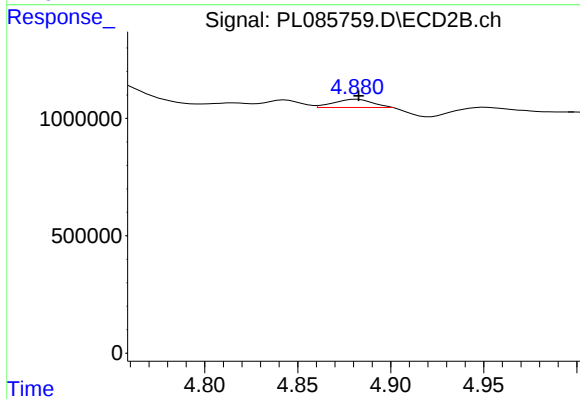

#11 alpha-Chlordane

R.T.: 4.880 min
Delta R.T.: -0.002 min
Response: 495018
Conc: 0.45 ng/ml m

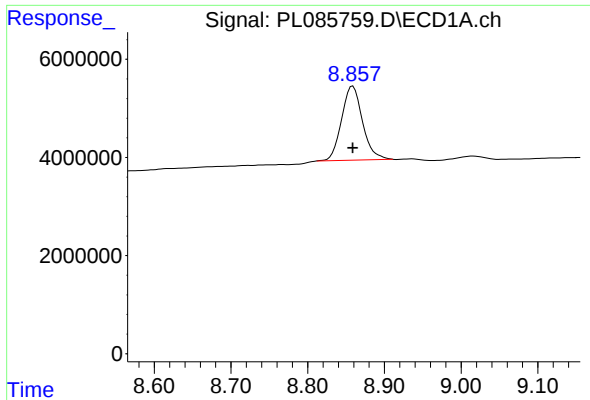


#28 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 28724890
Conc: 13.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-10052023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/09/2023
Supervised By :Ankita Jodhani 10/09/2023

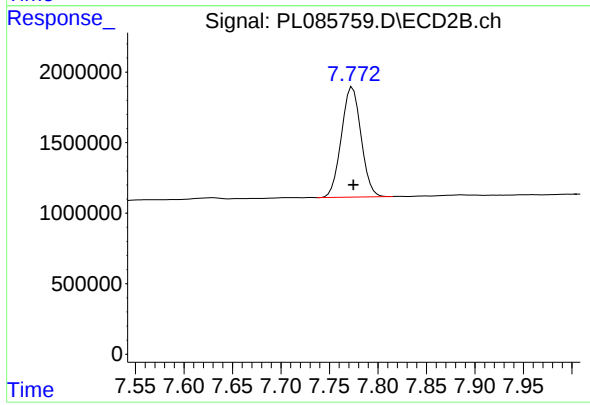

#28 Decachlorobiphenyl

R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 11006851
Conc: 11.93 ng/ml