

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100719\
 Data File : PL053098.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2019 12:58
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 05:36:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	0.000	5.233	0	1719346	N.D.	0.451 #
5) MB	Aldrin	0.000	5.554	0	209760	N.D.	0.061 #
7) B	delta-BHC	0.000	5.101	0	10144196	N.D.	2.802 #
8) B	Heptachlo...	0.000	5.929	0	5388403	N.D.	1.608 #
9) A	Endosulfan I	0.000	6.280	0	228569	N.D.	0.073 #
17) MA	4,4'-DDT	0.000	7.150f	0	10205270	N.D.	3.921 #
18) B	Endrin al...	6.569	7.087	39604943	2150255	4.217	0.877 #
23)	Chlordane-1	0.000	5.027f	0	1962947	N.D.	19.353 #
24)	Chlordane-2	0.000	5.495f	0	2563692	N.D.	22.906 #
27)	Chlordane-5	0.000	7.059f	0	1895201	N.D.	21.485 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100719\
Data File : PL053098.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2019 12:58
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 05:36:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

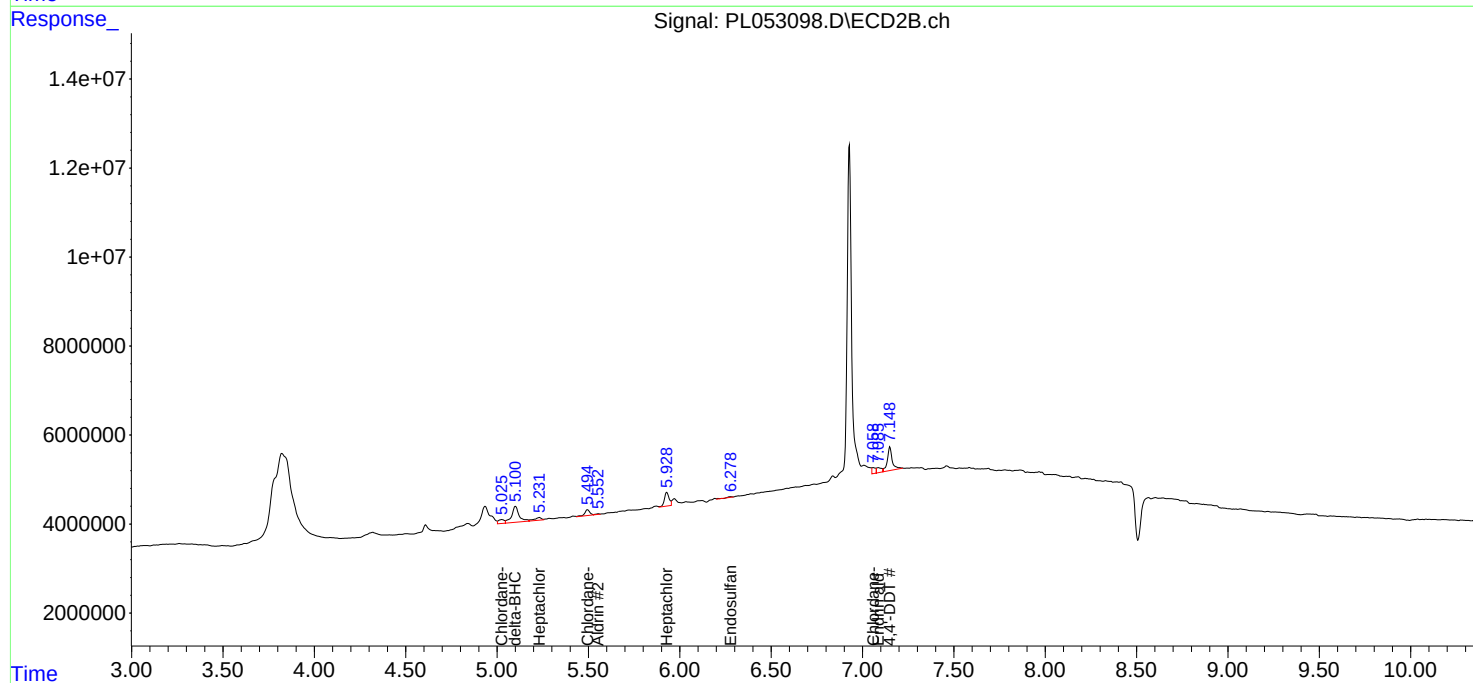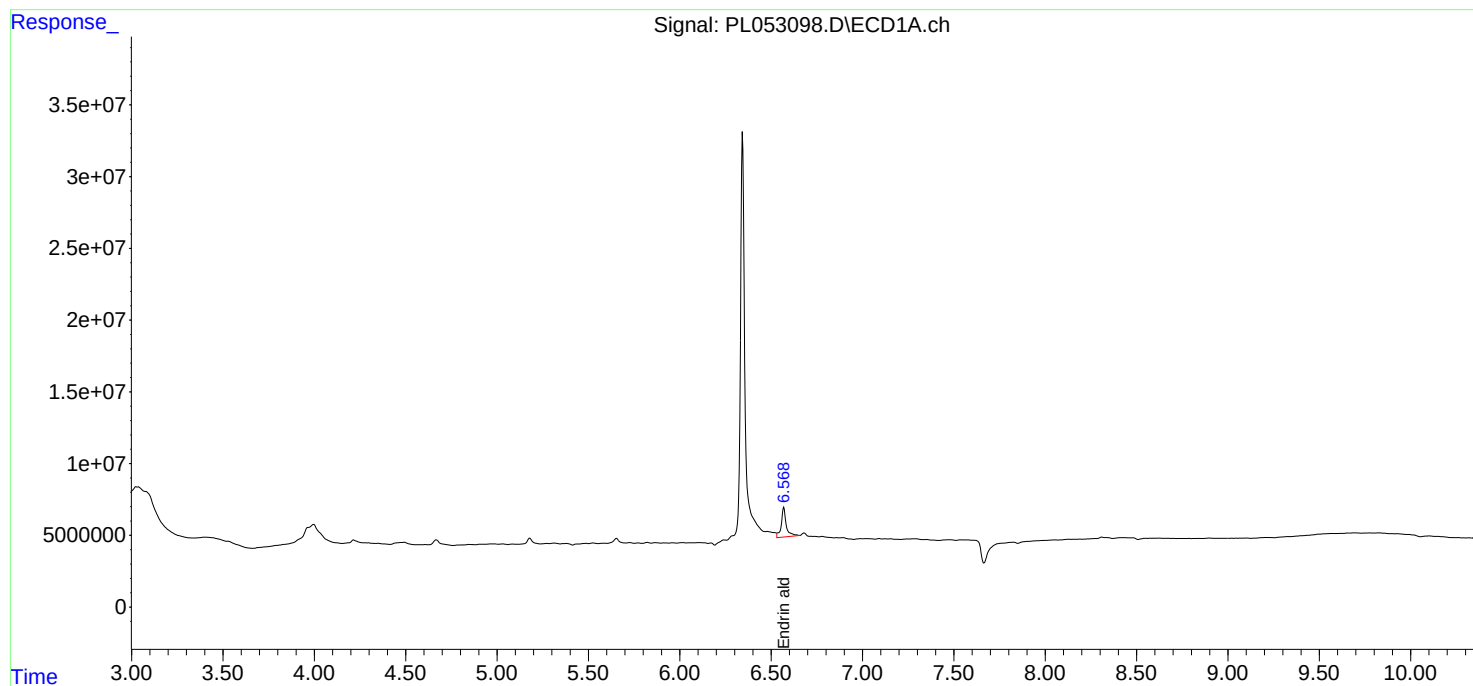


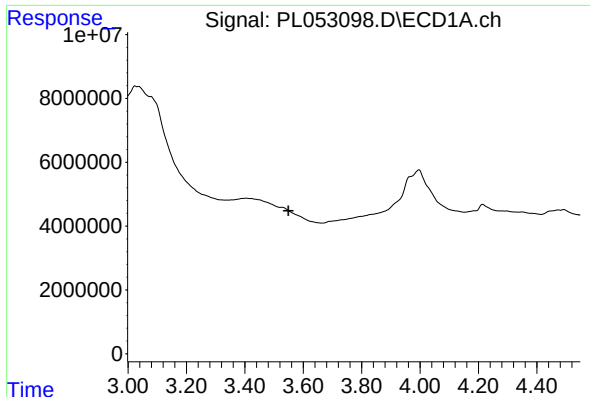

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.549 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

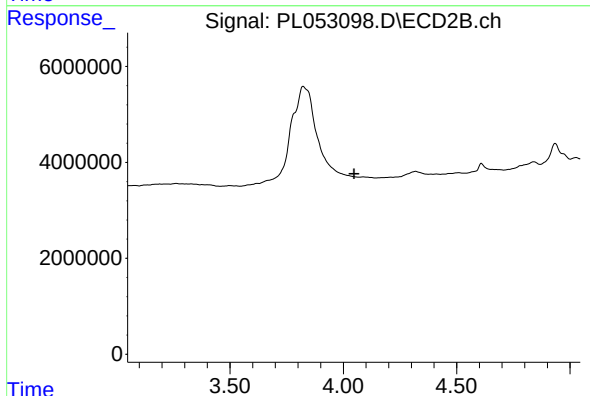


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.047 min
Response: 0
Conc: N.D.

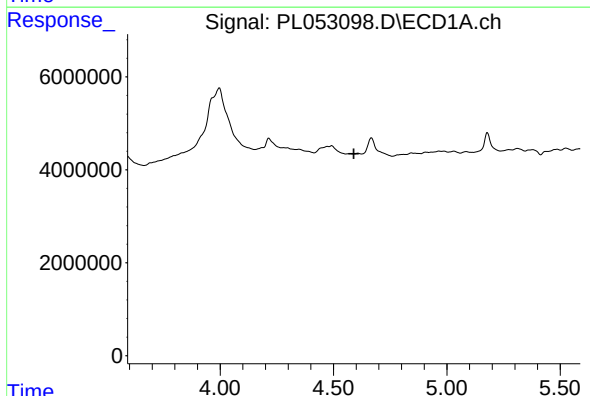


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.590 min
Response: 0
Conc: N.D.

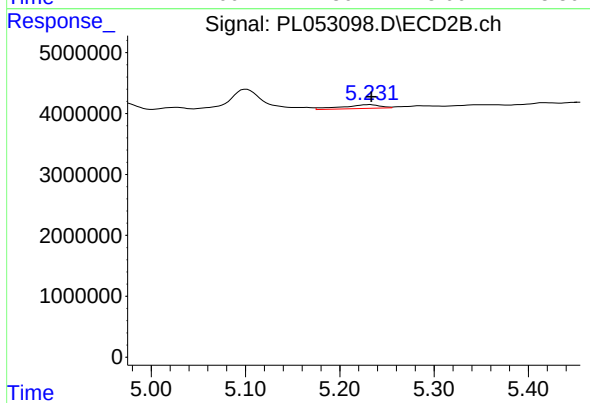

#4 Heptachlor


R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 1719346
Conc: 0.45 ng/ml

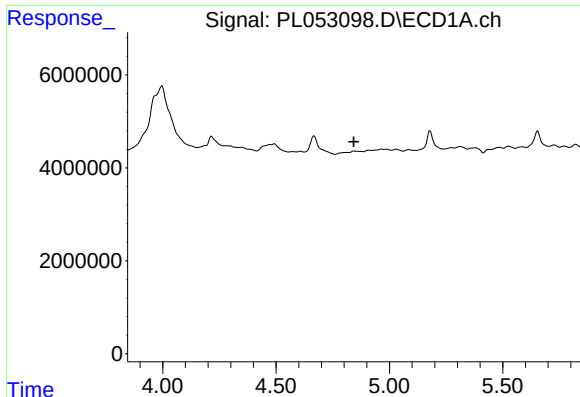

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.843 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

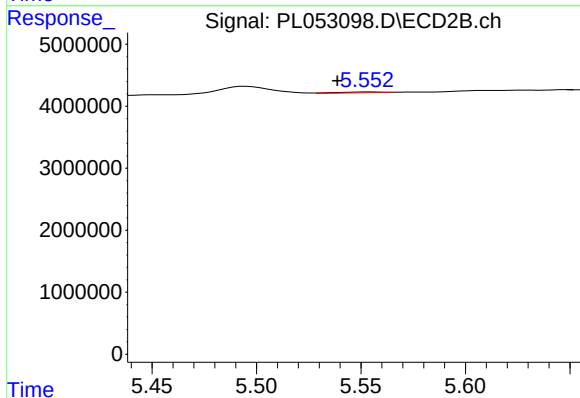


#5 Aldrin

R.T.: 5.554 min
Delta R.T.: 0.015 min
Response: 209760
Conc: 0.06 ng/ml

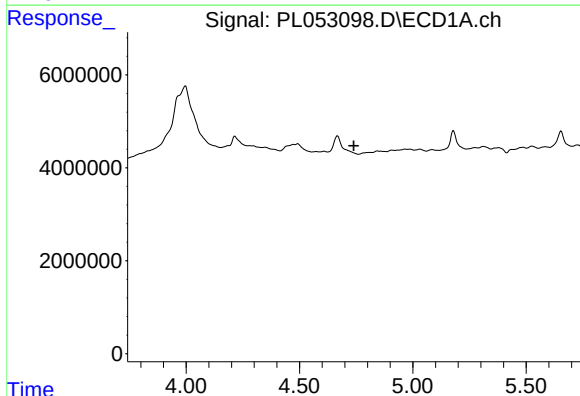


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

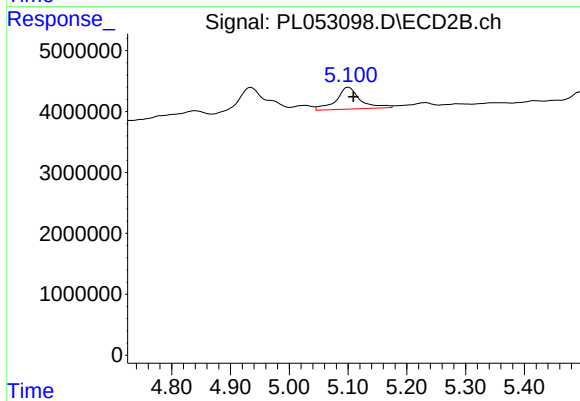

#7 delta-BHC


R.T.: 5.101 min
Delta R.T.: -0.008 min
Response: 10144196
Conc: 2.80 ng/ml

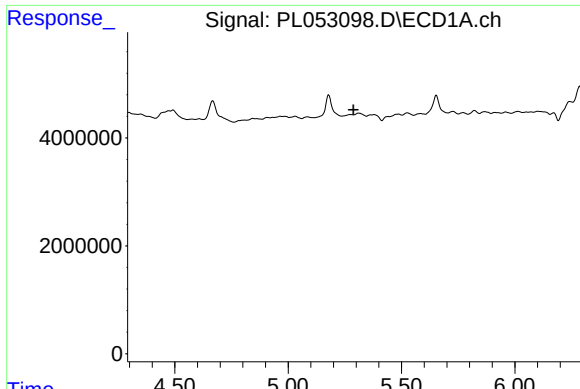

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

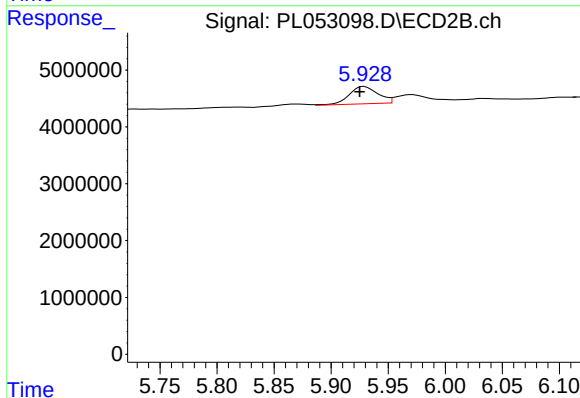


#8 Heptachlor epoxide

R.T.: 5.929 min
Delta R.T.: 0.004 min
Response: 5388403
Conc: 1.61 ng/ml

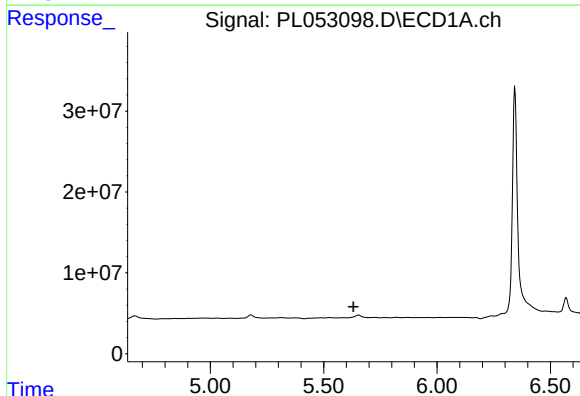


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.632 min
Response: 0
Conc: N.D.

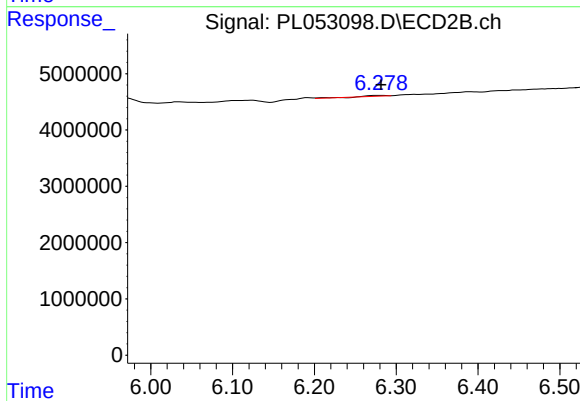

#9 Endosulfan I


R.T.: 6.280 min
Delta R.T.: -0.002 min
Response: 228569
Conc: 0.07 ng/ml

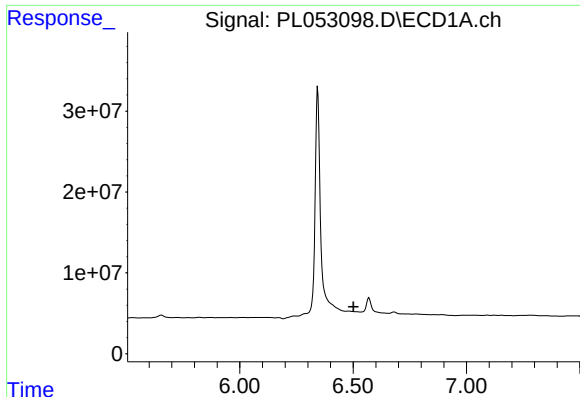

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

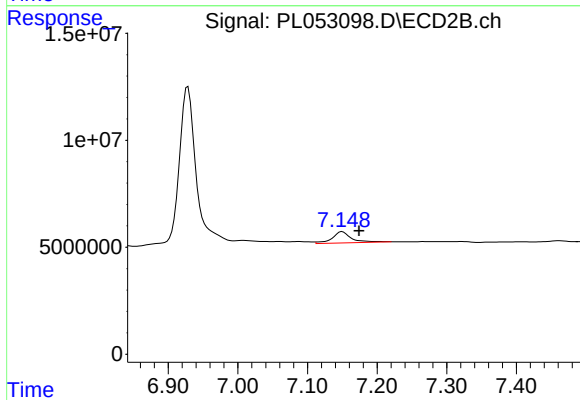


#17 4,4'-DDT

R.T.: 7.150 min
Delta R.T.: -0.024 min
Response: 10205270
Conc: 3.92 ng/ml

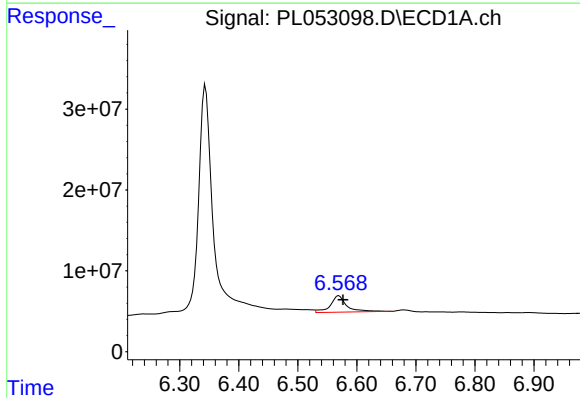


#18 Endrin aldehyde

R.T.: 6.569 min
Delta R.T.: -0.007 min
Response: 39604943
Conc: 4.22 ng/ml

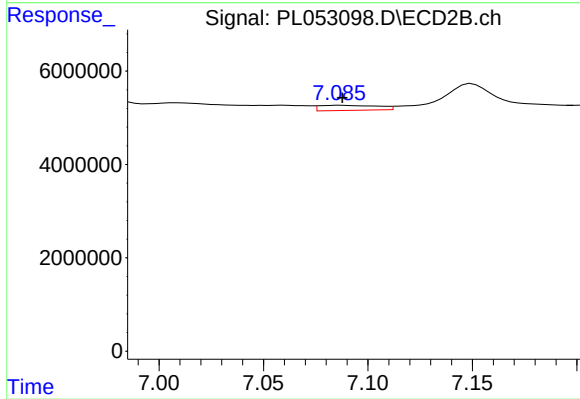

#18 Endrin aldehyde


R.T.: 7.087 min
Delta R.T.: 0.000 min
Response: 2150255
Conc: 0.88 ng/ml

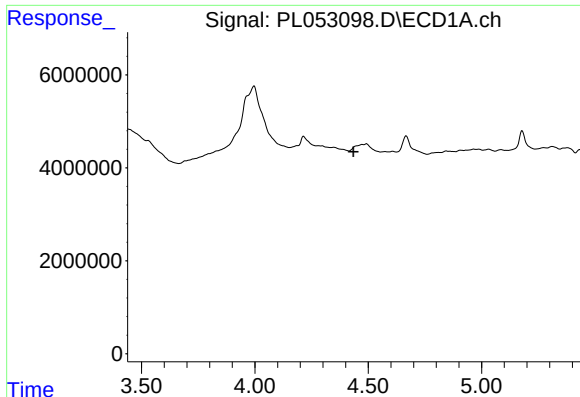

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

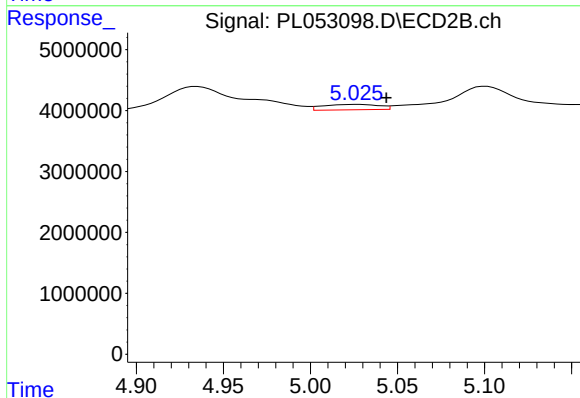


#23 Chlordane-1

R.T.: 5.027 min
Delta R.T.: -0.017 min
Response: 1962947
Conc: 19.35 ng/ml

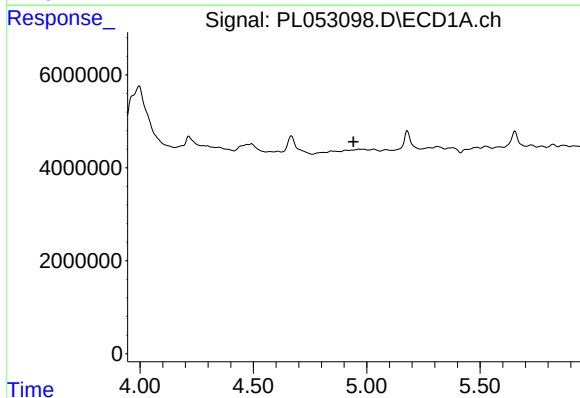


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

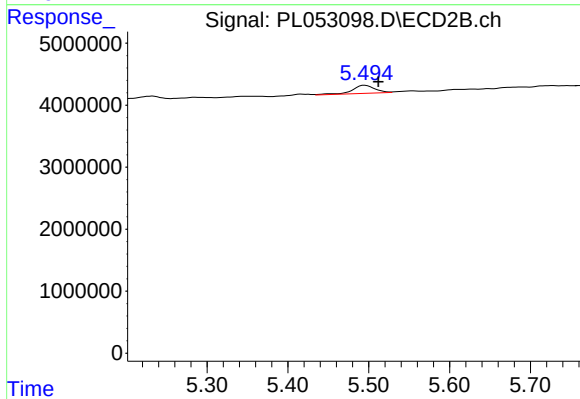

#24 Chlordane-2


R.T.: 5.495 min
Delta R.T.: -0.017 min
Response: 2563692
Conc: 22.91 ng/ml

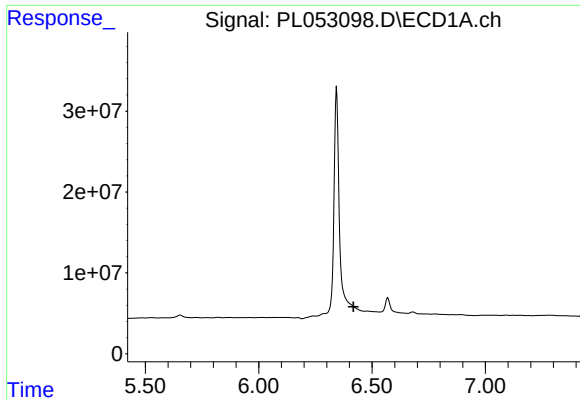

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

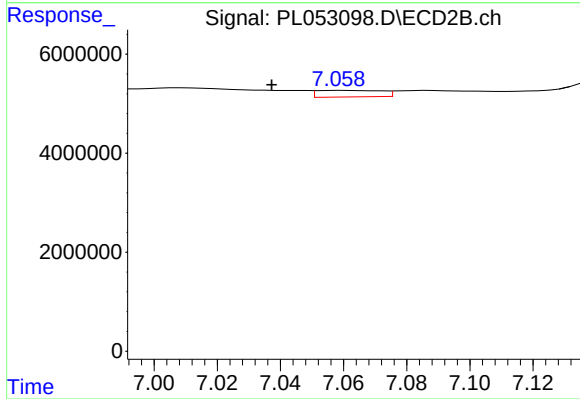


#27 Chlordane-5

R.T.: 7.059 min
Delta R.T.: 0.022 min
Response: 1895201
Conc: 21.49 ng/ml

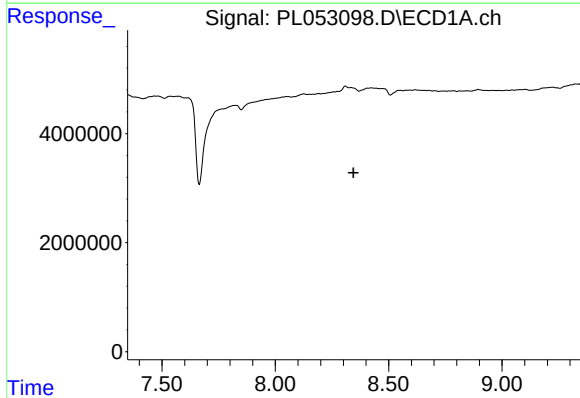

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

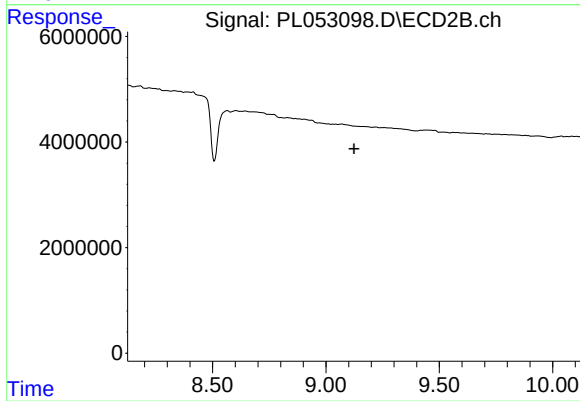

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.124 min
Response: 0
Conc: N.D.