

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100719\
 Data File : PL053103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2019 14:31
 Operator : SG\AJ
 Sample : PB123679BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB123679BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 07 16:42:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	4.048	203.3E6	52592395	20.437	19.586
28)	SA Decachlor...	8.339	9.127	204.1E6	62277907	20.380	21.228
Target Compounds							
2)	A alpha-BHC	0.000	4.410f	0	1505400	N.D.	0.392 #
3)	MA gamma-BHC...	0.000	4.726	0	212149	N.D.	0.059 #
7)	B delta-BHC	0.000	5.105	0	8932616	N.D.	2.468 #
8)	B Heptachlo...	0.000	5.930	0	2480200	N.D.	0.740 #
15)	B Endosulfa...	0.000	6.973	0	2644990	N.D.	0.891 #
17)	MA 4,4'-DDT	0.000	7.151f	0	2859438	N.D.	1.099 #
20)	A Methoxychlor	0.000	7.648f	0	5844467	N.D.	4.151 #
21)	B Endrin ke...	0.000	7.775	0	14964373	N.D.	5.245 #
23)	Chlordane-1	0.000	5.035	0	1499176	N.D.	14.780 #
24)	Chlordane-2	0.000	5.483f	0	209.1E6	N.D.	1868.099 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100719\
Data File : PL053103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2019 14:31
Operator : SG\AJ
Sample : PB123679BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB123679BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 07 16:42:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

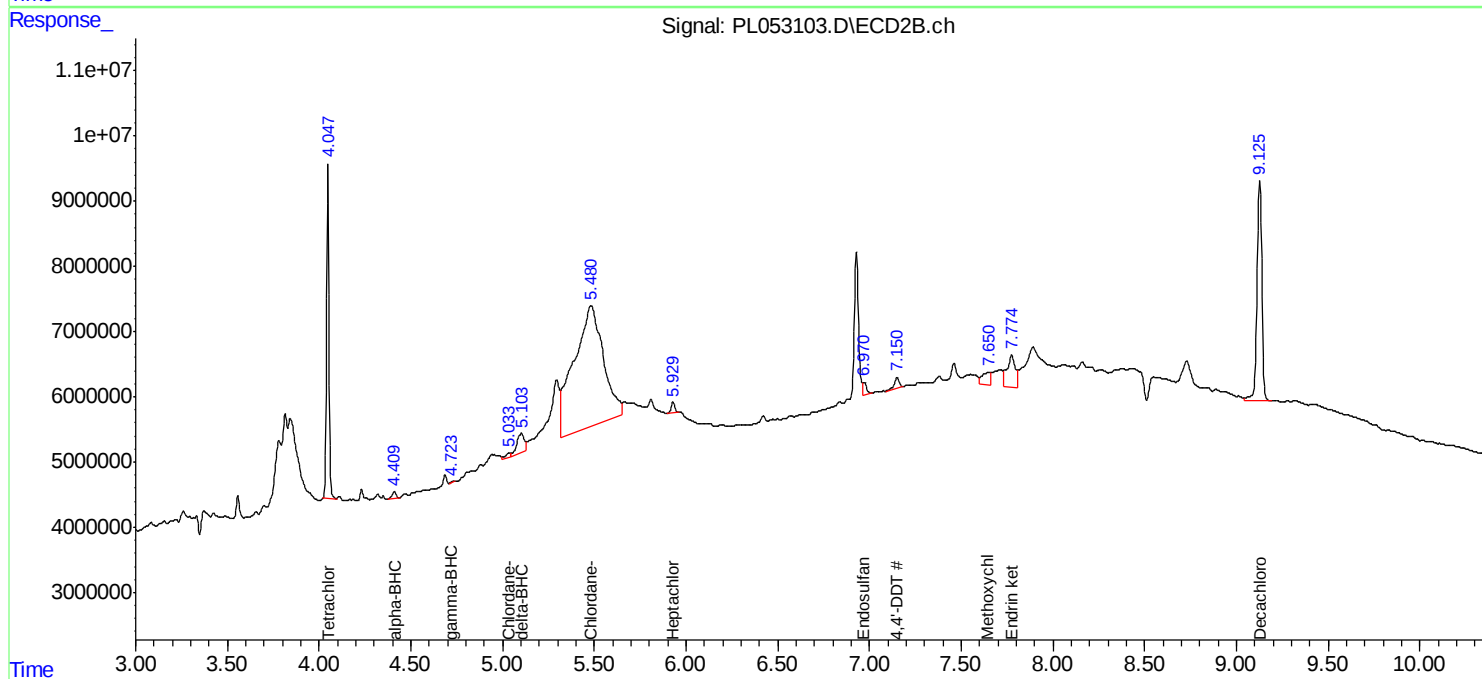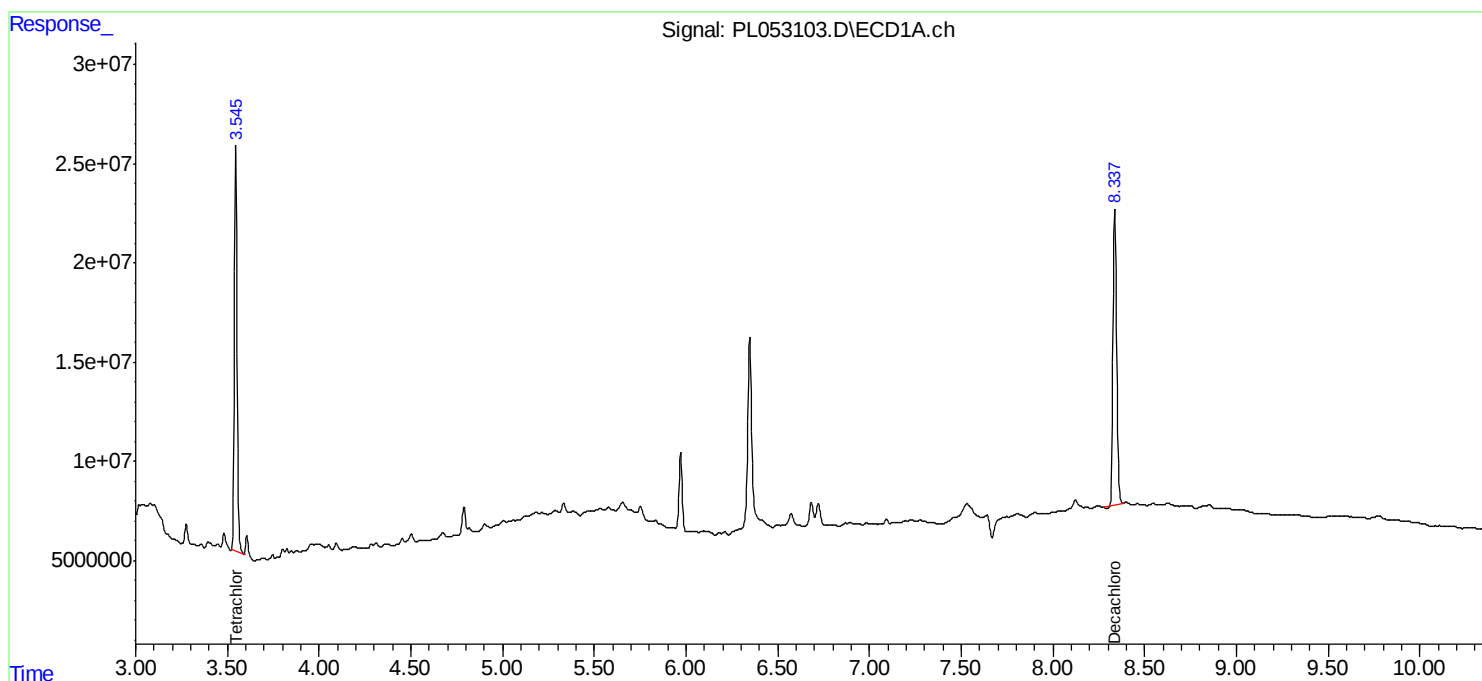


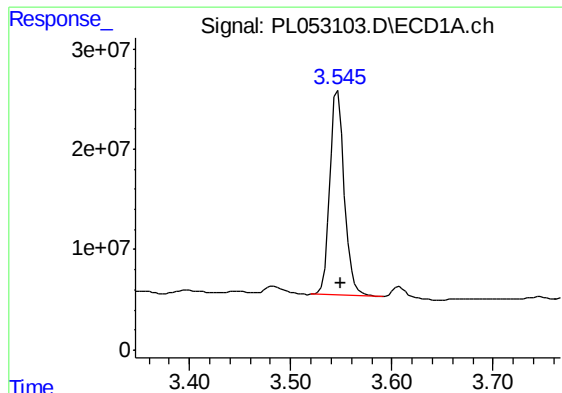

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: -0.002 min
Response: 203284907
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB123679BL

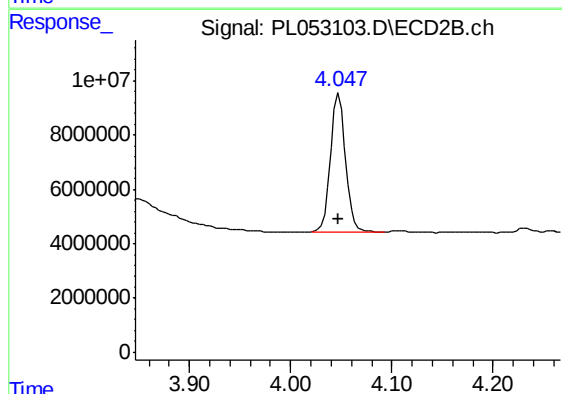


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 52592395
Conc: 19.59 ng/ml

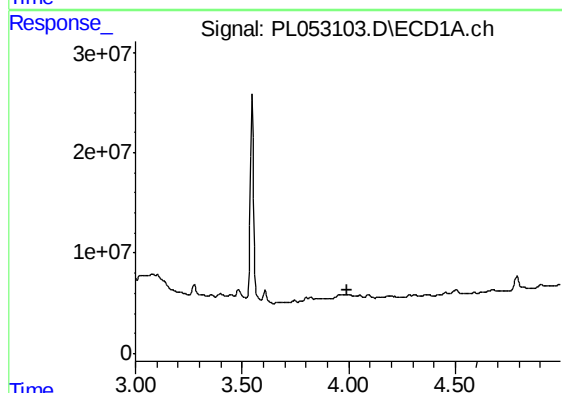


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.994 min
Response: 0
Conc: N.D.

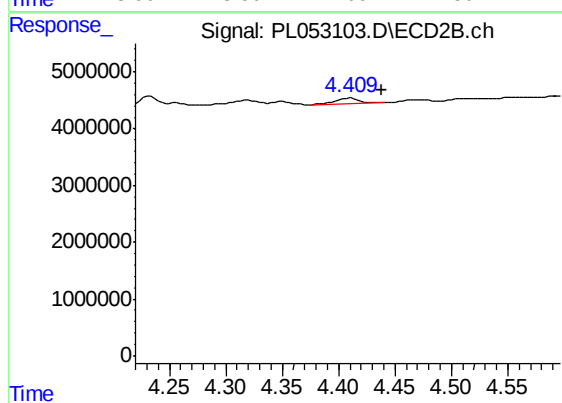

#2 alpha-BHC


R.T.: 4.410 min
Delta R.T.: -0.028 min
Response: 1505400
Conc: 0.39 ng/ml

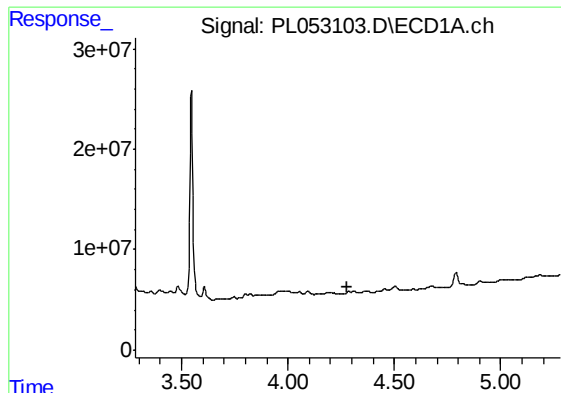

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB123679BL

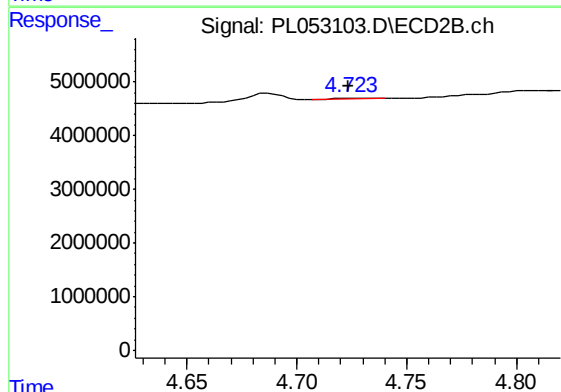


#3 gamma-BHC (Lindane)

R.T.: 4.726 min
Delta R.T.: 0.003 min
Response: 212149
Conc: 0.06 ng/ml

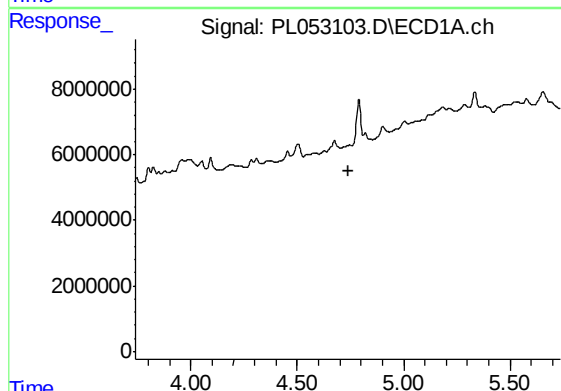


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.740 min
Response: 0
Conc: N.D.

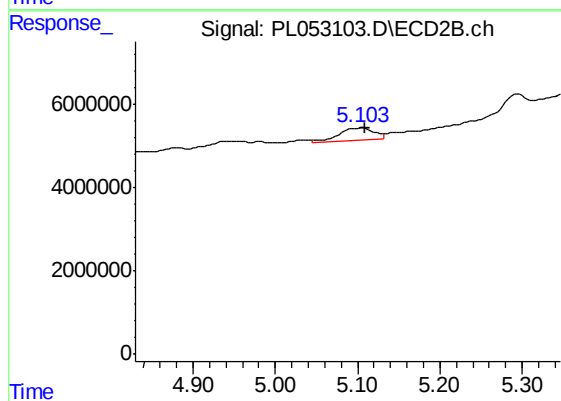

#7 delta-BHC


R.T.: 5.105 min
Delta R.T.: -0.004 min
Response: 8932616
Conc: 2.47 ng/ml

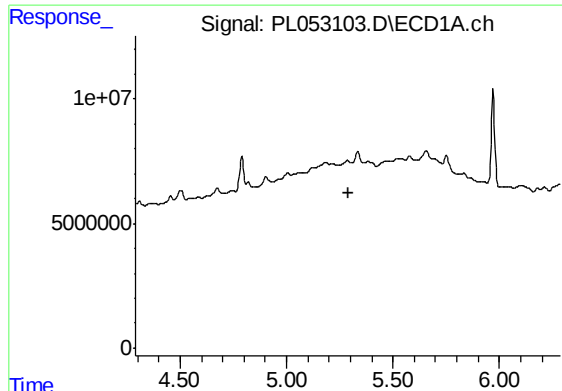

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB123679BL

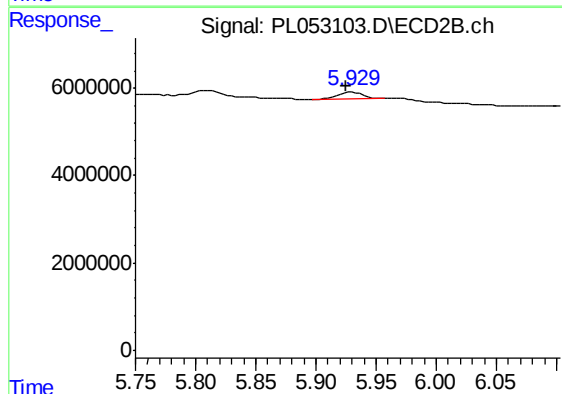


#8 Heptachlor epoxide

R.T.: 5.930 min
Delta R.T.: 0.005 min
Response: 2480200
Conc: 0.74 ng/ml

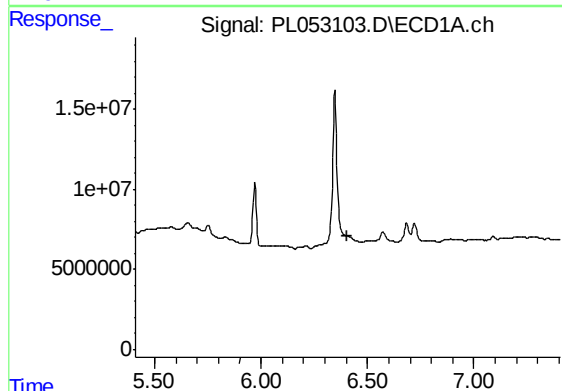


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.408 min
Response: 0
Conc: N.D.

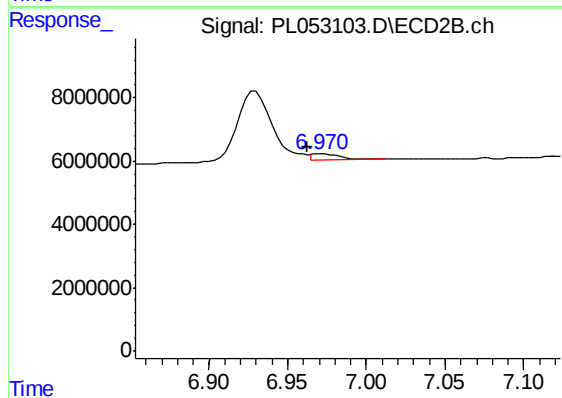

#15 Endosulfan II


R.T.: 6.973 min
Delta R.T.: 0.010 min
Response: 2644990
Conc: 0.89 ng/ml

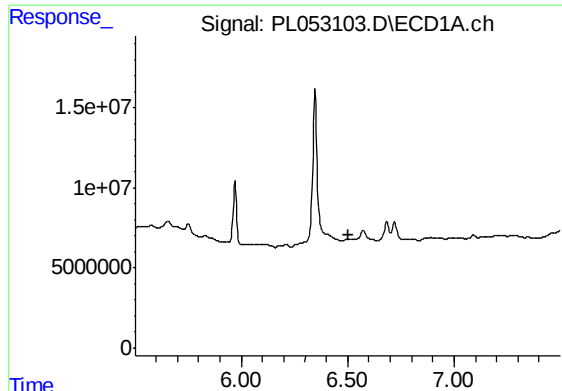

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB123679BL

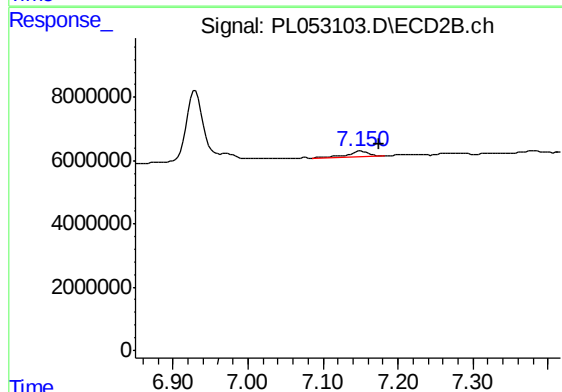


#17 4,4'-DDT

R.T.: 7.151 min
Delta R.T.: -0.023 min
Response: 2859438
Conc: 1.10 ng/ml

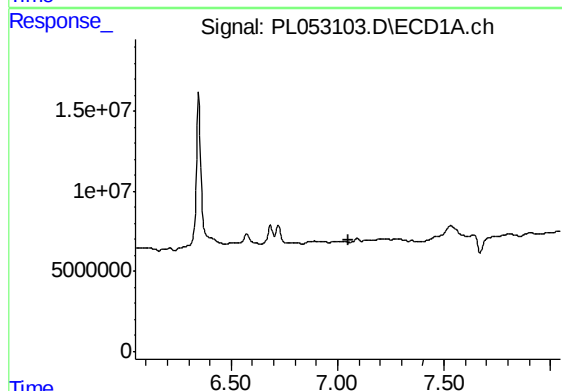


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.049 min
Response: 0
Conc: N.D.

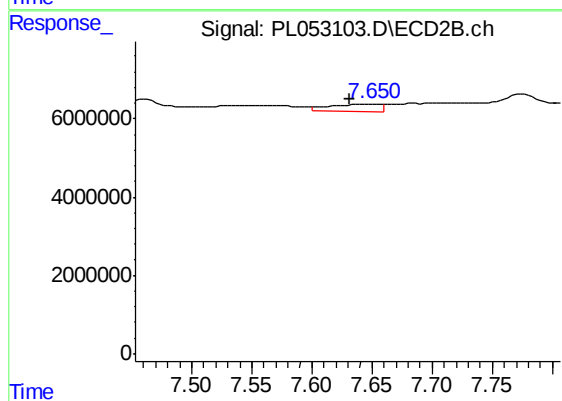

#20 Methoxychlor


R.T.: 7.648 min
Delta R.T.: 0.016 min
Response: 5844467
Conc: 4.15 ng/ml

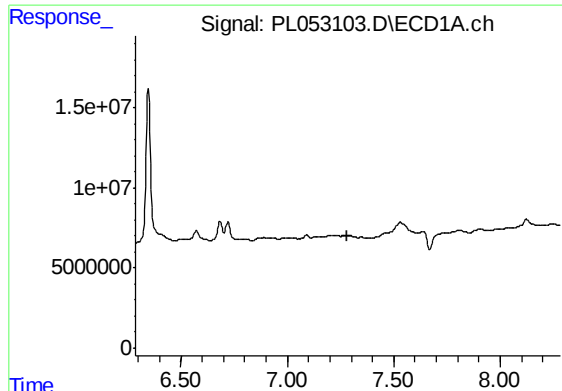

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB123679BL

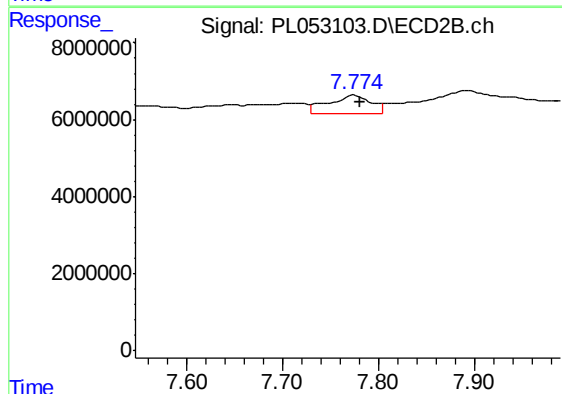


#21 Endrin ketone

R.T.: 7.775 min
Delta R.T.: -0.006 min
Response: 14964373
Conc: 5.25 ng/ml

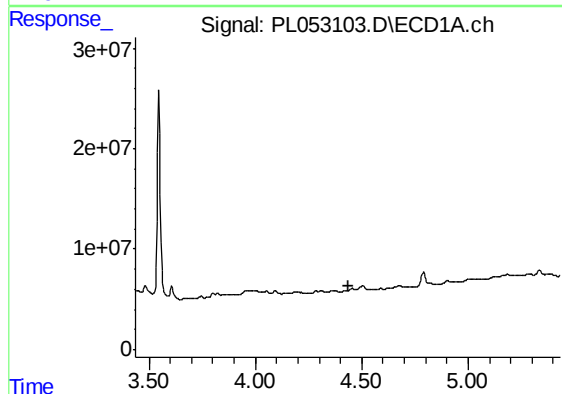

#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.435 min
Response: 0
Conc: N.D.

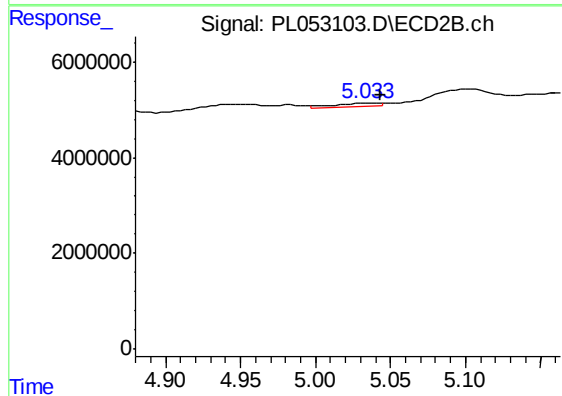

#23 Chlordane-1

R.T.: 5.035 min
Delta R.T.: -0.009 min
Response: 1499176
Conc: 14.78 ng/ml

