

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100719\
 Data File : PL053129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Oct 2019 21:46
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 08 05:39:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 30 08:44:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	4.048	230.6E6	57711758	23.187	21.492
28)	SA Decachlor...	8.337	9.126	213.9E6	60891523	21.351	20.756
Target Compounds							
8)	B Heptachlo...	0.000	5.929	0	2849977	N.D.	0.850 #
11)	B alpha-Chl...	0.000	6.214f	0	1631046	N.D.	0.485 #
17)	MA 4,4'-DDT	0.000	7.148f	0	857648	N.D.	0.330 #
18)	B Endrin al...	0.000	7.114f	0	731929	N.D.	0.298 #
26)	Chlordane-4	0.000	6.214f	0	1631046	N.D.	3.072 #
27)	Chlordane-5	0.000	7.052f	0	677538	N.D.	7.681 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL100719\
Data File : PL053129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Oct 2019 21:46
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 08 05:39:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092919.M
Quant Title : GC Extractables
QLast Update : Mon Sep 30 08:44:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

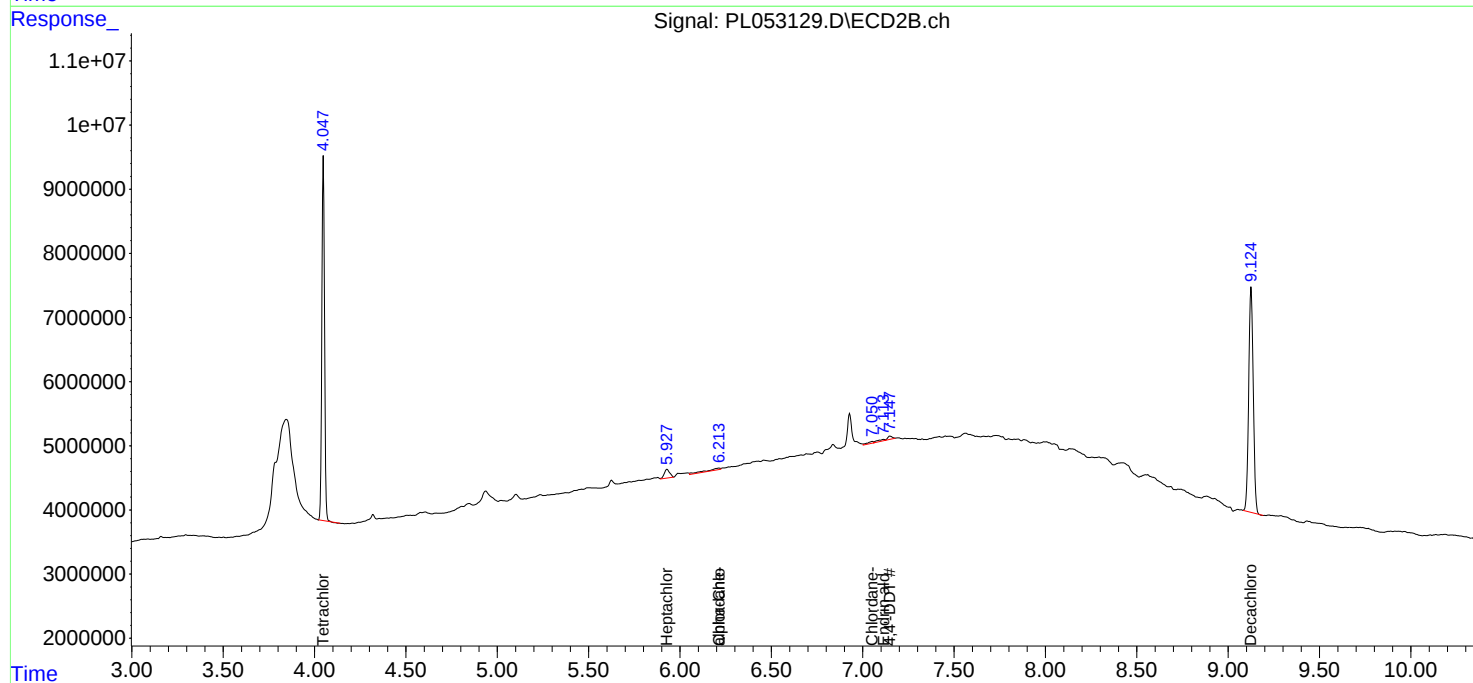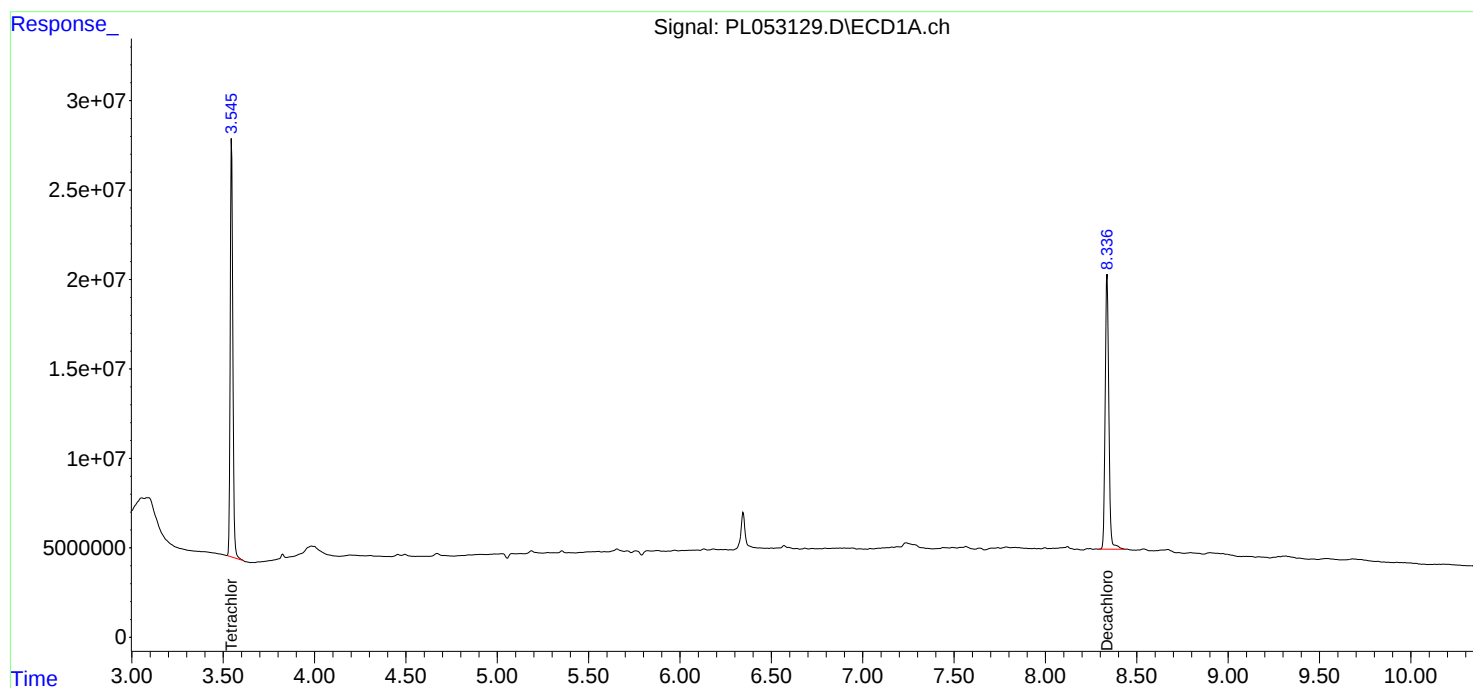


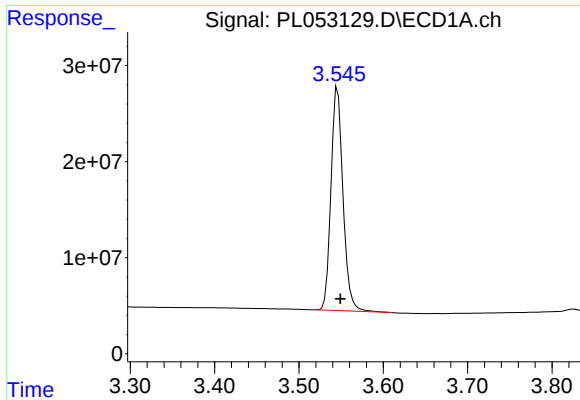

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: -0.003 min
Response: 230630870
Conc: 23.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

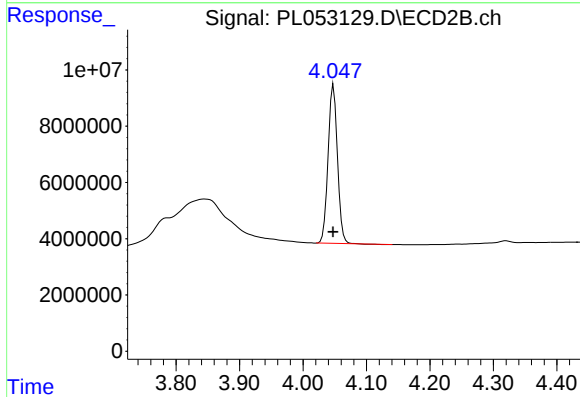


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.000 min
Response: 57711758
Conc: 21.49 ng/ml

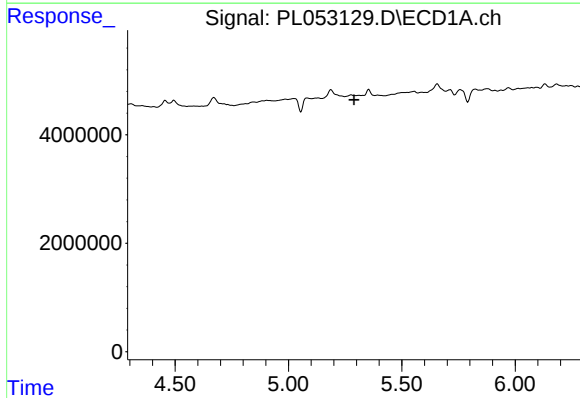


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.289 min
Response: 0
Conc: N.D.

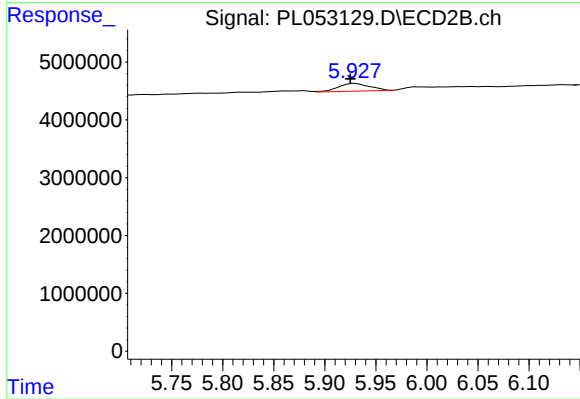

#8 Heptachlor epoxide


R.T.: 5.929 min
Delta R.T.: 0.004 min
Response: 2849977
Conc: 0.85 ng/ml

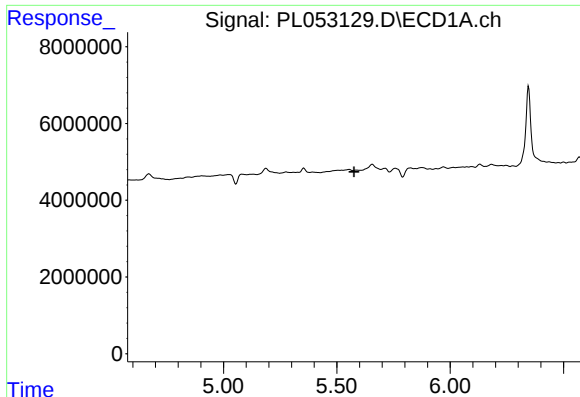

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

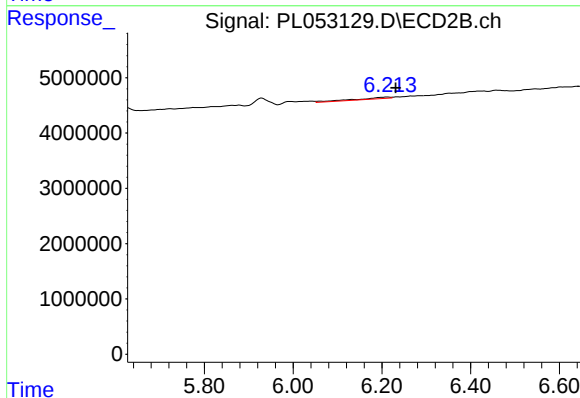


#11 alpha-Chlordane

R.T.: 6.214 min
Delta R.T.: -0.017 min
Response: 1631046
Conc: 0.48 ng/ml

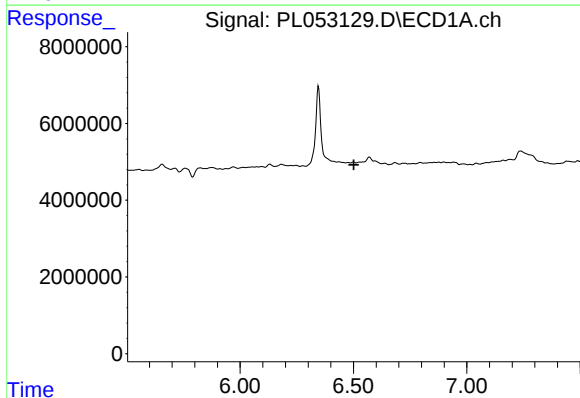


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.502 min
Response: 0
Conc: N.D.

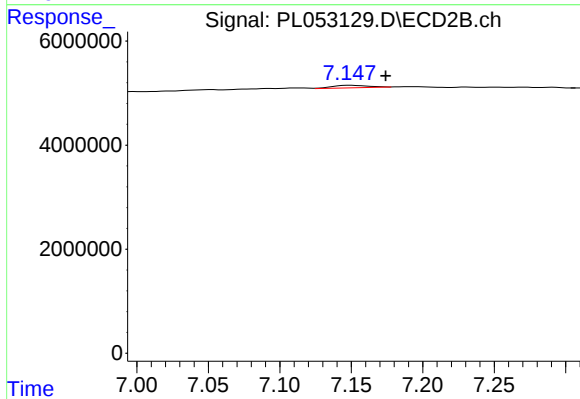

#17 4,4'-DDT


R.T.: 7.148 min
Delta R.T.: -0.026 min
Response: 857648
Conc: 0.33 ng/ml

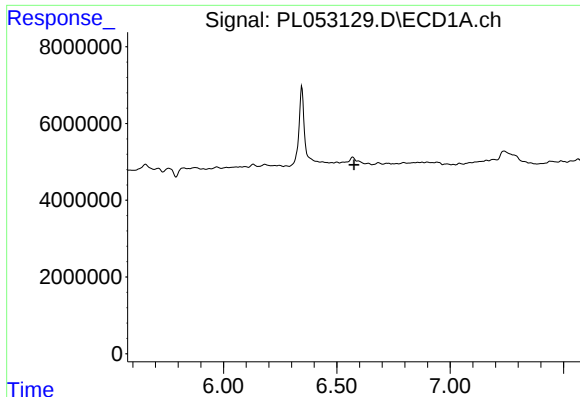

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

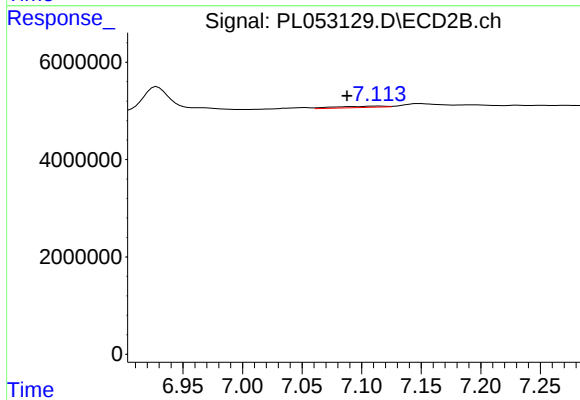


#18 Endrin aldehyde

R.T.: 7.114 min
Delta R.T.: 0.026 min
Response: 731929
Conc: 0.30 ng/ml

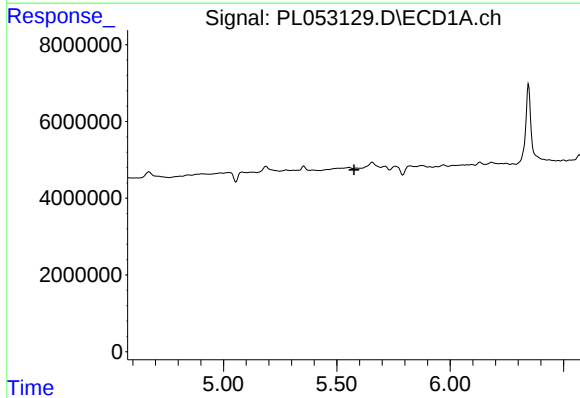


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.577 min
Response: 0
Conc: N.D.

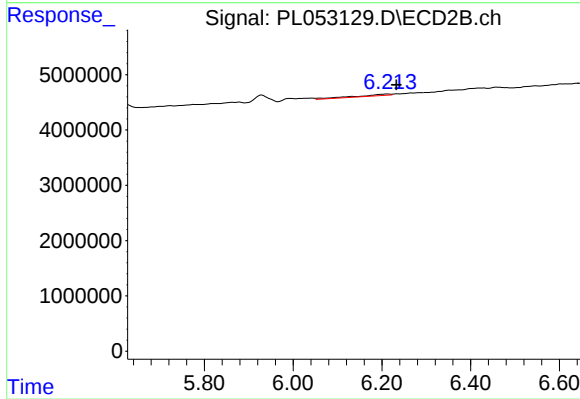

#26 Chlordane-4


R.T.: 6.214 min
Delta R.T.: -0.019 min
Response: 1631046
Conc: 3.07 ng/ml

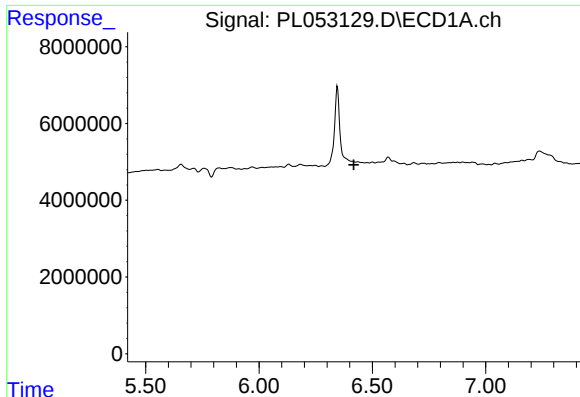

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

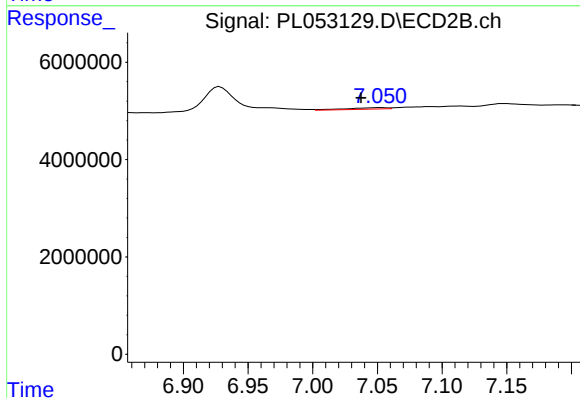


#27 Chlordane-5

R.T.: 7.052 min
Delta R.T.: 0.015 min
Response: 677538
Conc: 7.68 ng/ml

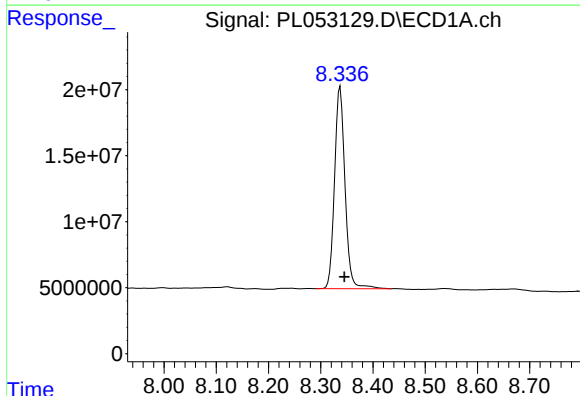

#28 Decachlorobiphenyl

R.T.: 8.337 min
Delta R.T.: -0.008 min
Response: 213850144
Conc: 21.35 ng/ml

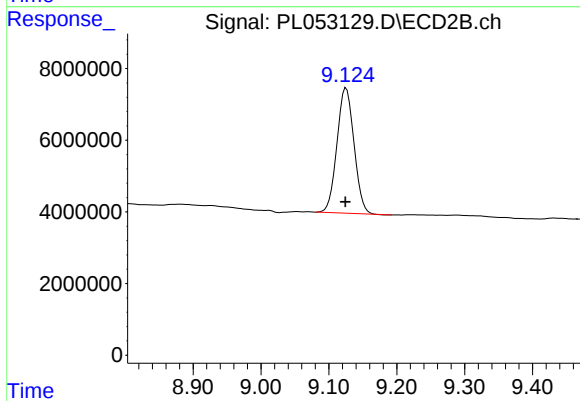

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.001 min
Response: 60891523
Conc: 20.76 ng/ml